

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031220\
 Data File : FE031474.D
 Signal(s) : FID1B.CH
 Acq On : 12 Mar 2020 11:45
 Operator : DD\AJ
 Sample : L1859-11 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 13 01:52:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Wed Mar 11 09:35:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.404	1281448	3.472 ug/ml
Target Compounds			
4) N-TETRADECANE	8.019	384160	0.924 ug/ml
11) N-HEXACOSANE	15.630	836168	1.991 ug/ml
12) N-OCTACOSANE	16.581	1803402	4.297 ug/ml
13) N-TRIACONTANE	17.470	4313592	10.322 ug/ml
14) N-DOTRIACONTANE	18.308	7212321	18.200 ug/ml
15) N-TETRATRIACONTANE	19.092	4659679	13.479 ug/ml
16) N-HEXATRIACONTANE	19.837	4473008	16.012 ug/ml
17) N-OCTATRIACONTANE	20.542	5931223	26.200 ug/ml
18) N-TETRACONTANE	21.361	1565051	7.289 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031220\
Data File : FE031474.D
Signal(s) : FID1B.CH
Acq On : 12 Mar 2020 11:45
Operator : DD\AJ
Sample : L1859-11 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 13 01:52:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Wed Mar 11 09:35:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

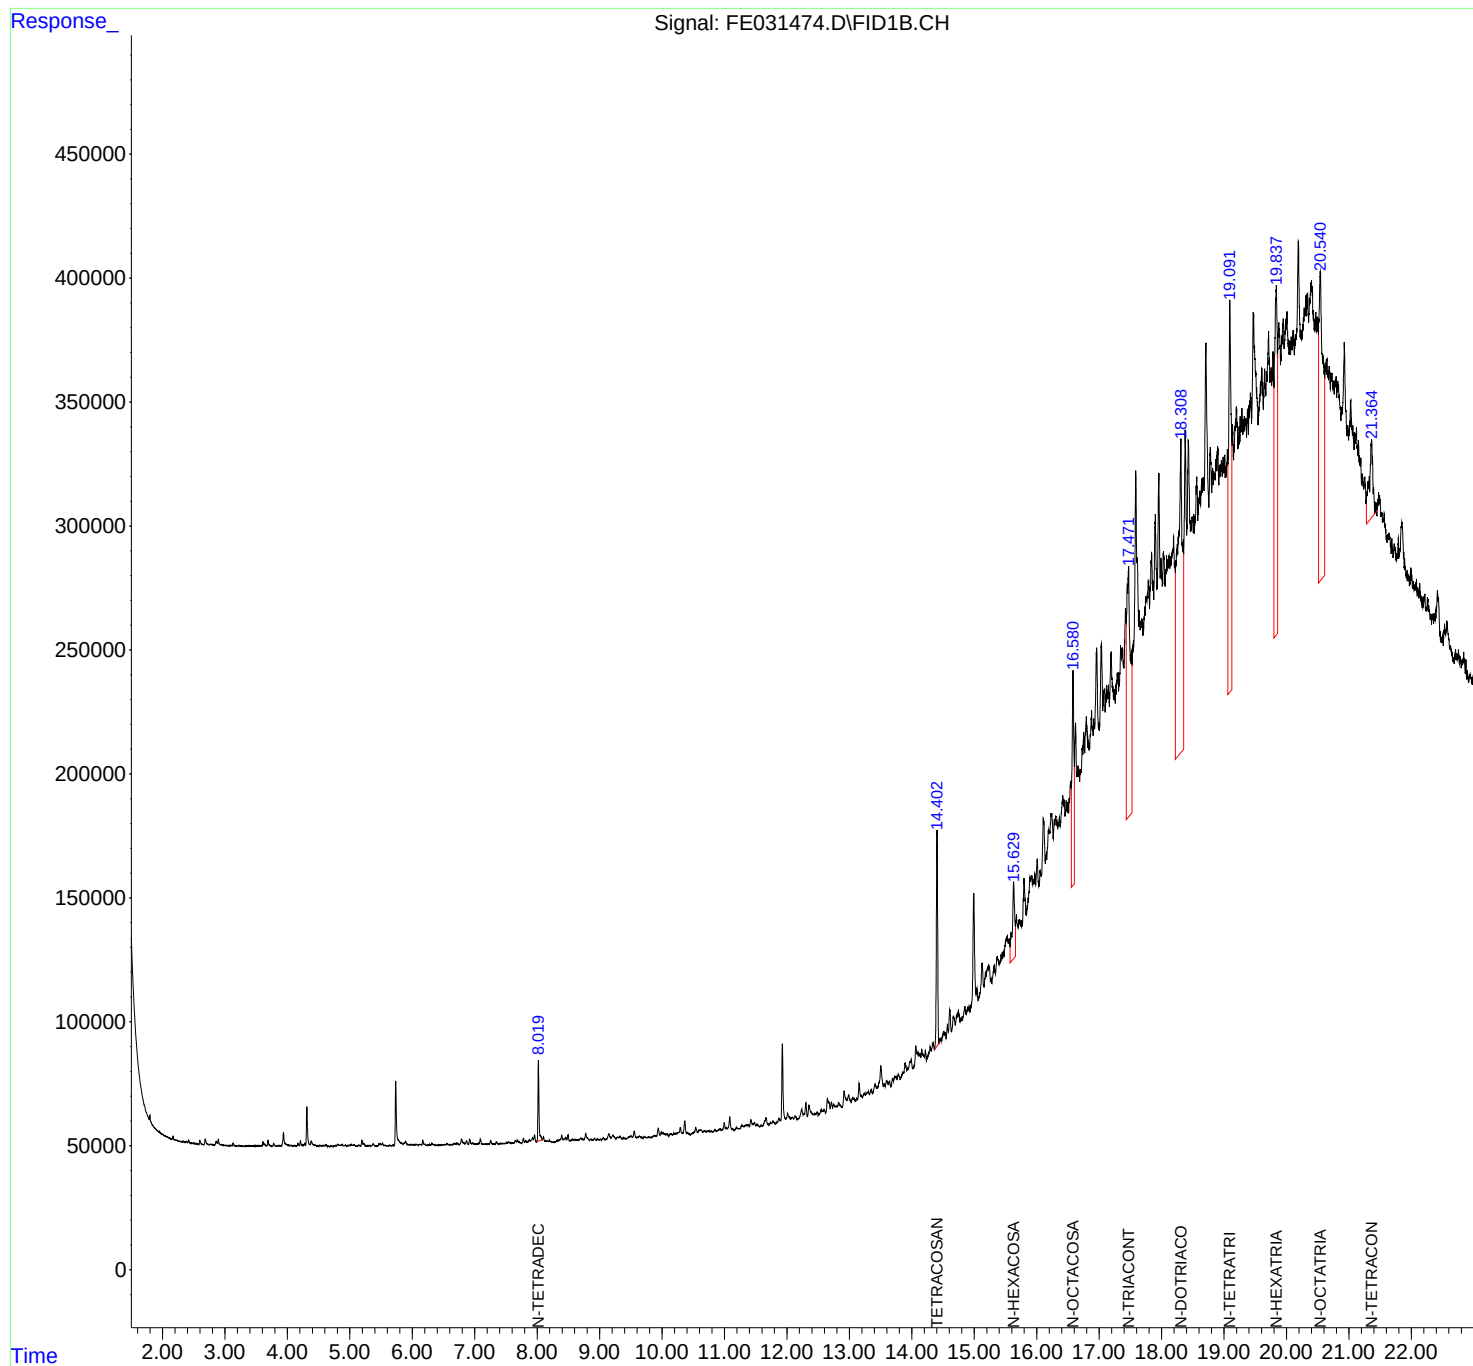

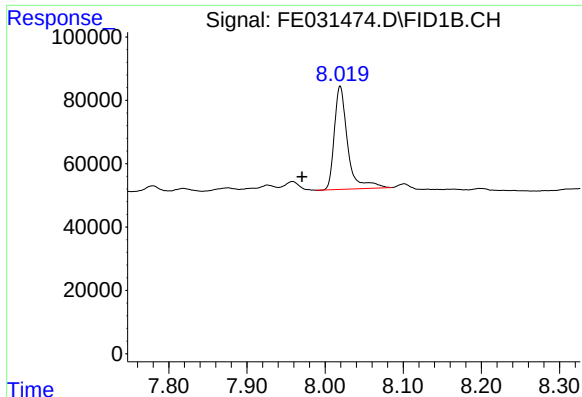


#4 N-TETRADECANE

R.T.: 8.019 min
Delta R.T.: 0.049 min
Response: 384160
Conc: 0.92 ug/ml

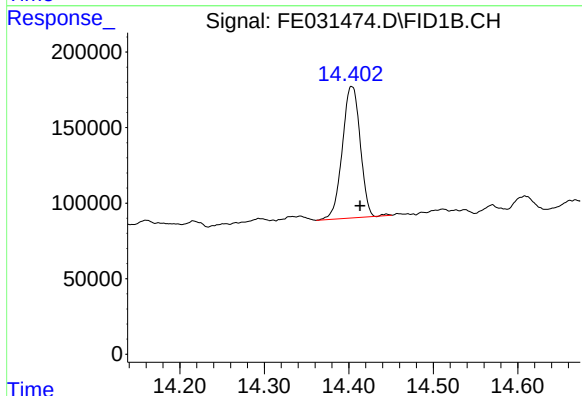


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.404 min
Delta R.T.: -0.010 min
Response: 1281448
Conc: 3.47 ug/ml

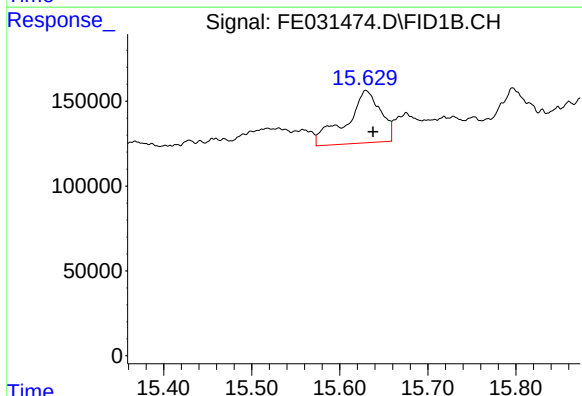


#11 N-HEXACOSANE

R.T.: 15.630 min
Delta R.T.: -0.008 min
Response: 836168
Conc: 1.99 ug/ml

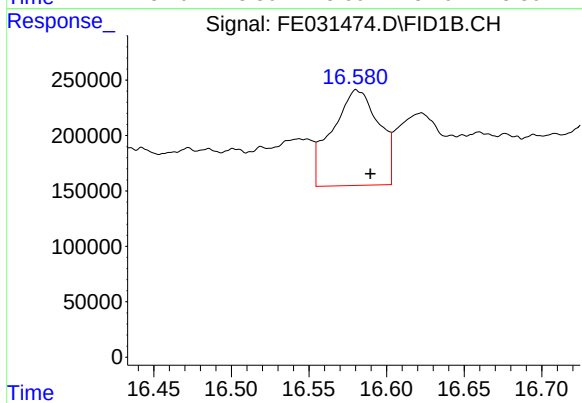


#12 N-OCTACOSANE

R.T.: 16.581 min
Delta R.T.: -0.008 min
Response: 1803402
Conc: 4.30 ug/ml

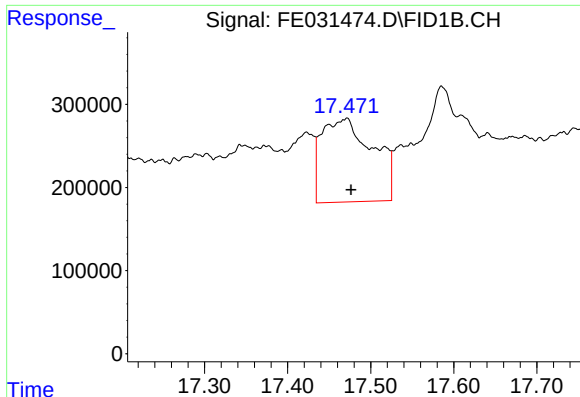


#13 N-TRIACONTANE

R.T.: 17.470 min
Delta R.T.: -0.006 min
Response: 4313592
Conc: 10.32 ug/ml

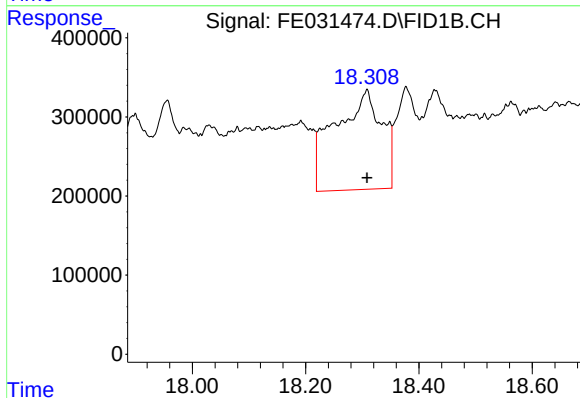


#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: 0.000 min
Response: 7212321
Conc: 18.20 ug/ml

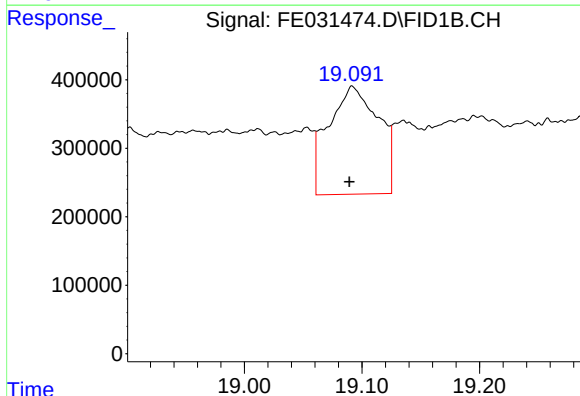


#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: 0.003 min
Response: 4659679
Conc: 13.48 ug/ml

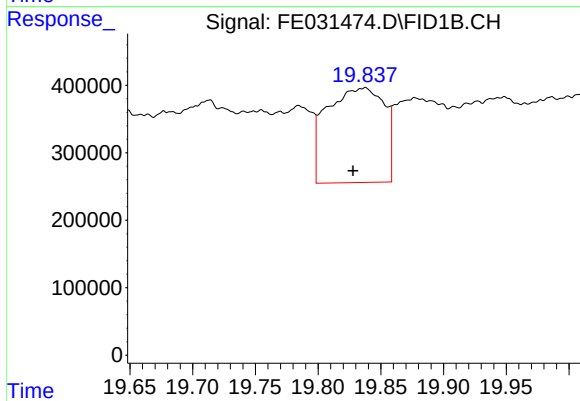


#16 N-HEXATRIACONTANE

R.T.: 19.837 min
Delta R.T.: 0.009 min
Response: 4473008
Conc: 16.01 ug/ml

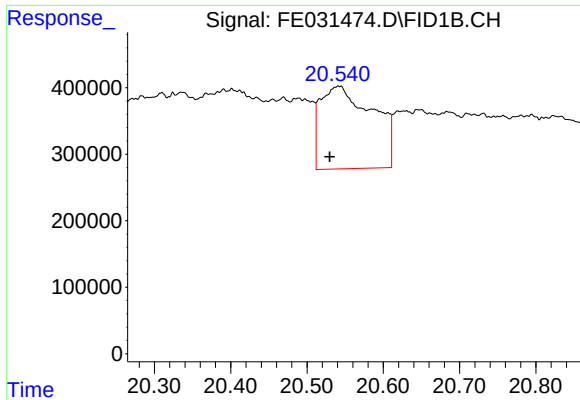

#17 N-OCTATRIACONTANE

R.T.: 20.542 min
Delta R.T.: 0.012 min
Response: 5931223
Conc: 26.20 ug/ml

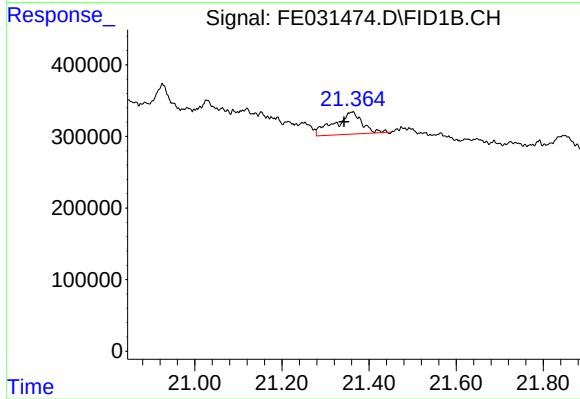

#18 N-TETRACONTANE

R.T.: 21.361 min
Delta R.T.: 0.019 min
Response: 1565051
Conc: 7.29 ug/ml