

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031620\
 Data File : FE031501.D
 Signal(s) : FID1B.CH
 Acq On : 16 Mar 2020 21:59
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 17 00:59:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Wed Mar 11 09:35:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.406	19235183	52.117 ug/ml
Target Compounds			
2) N-DECANE	4.171	22038099	55.309 ug/ml
3) N-DODECANE	6.175	22533007	54.997 ug/ml
4) N-TETRADECANE	7.966	22585523	54.307 ug/ml
5) N-HEXADECANE	9.564	22848158	53.732 ug/ml
6) N-OCTADECANE	11.003	22792224	53.221 ug/ml
7) N-EICOSANE	12.312	22580423	52.823 ug/ml
8) N-DOCOSANE	13.508	22372462	52.437 ug/ml
10) N-TETRACOSANE	14.611	22129301	51.965 ug/ml
11) N-HEXACOSANE	15.631	21709674	51.687 ug/ml
12) N-OCTACOSANE	16.579	21582269	51.424 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031620\
Data File : FE031501.D
Signal(s) : FID1B.CH
Acq On : 16 Mar 2020 21:59
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 17 00:59:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Wed Mar 11 09:35:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

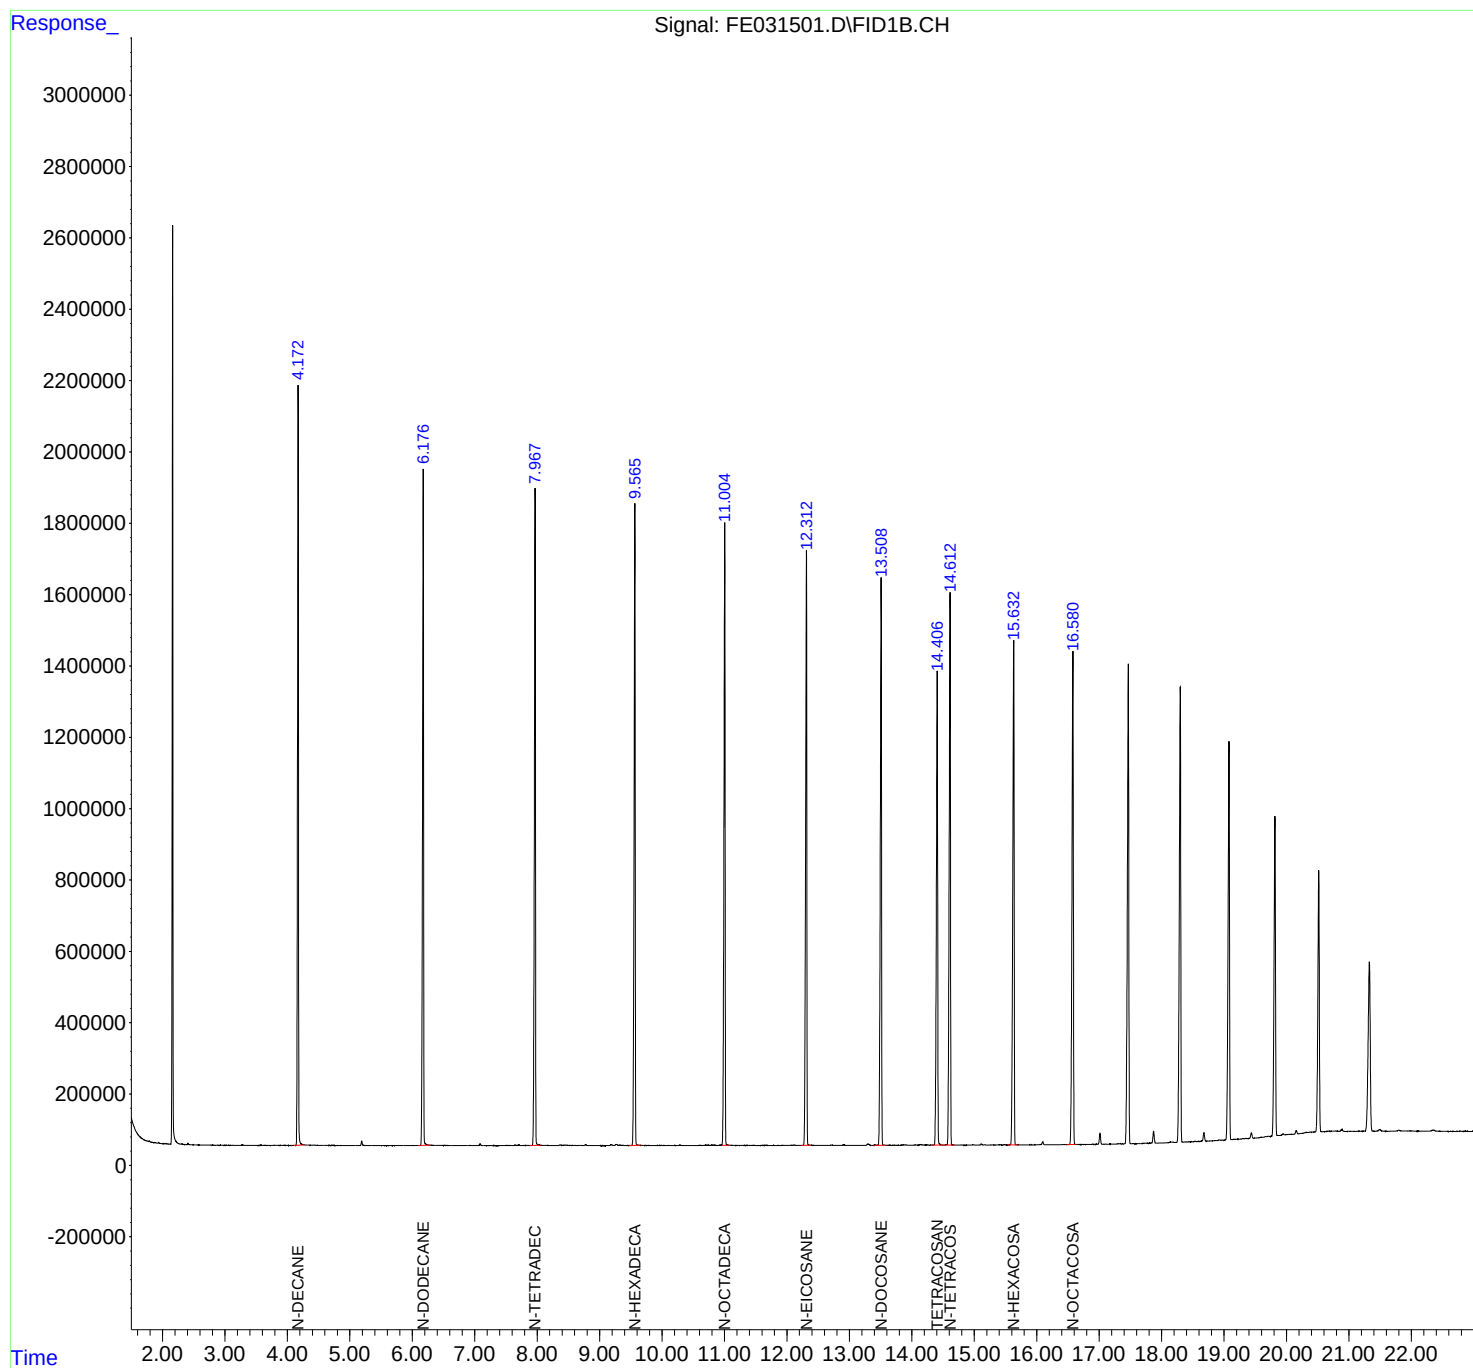

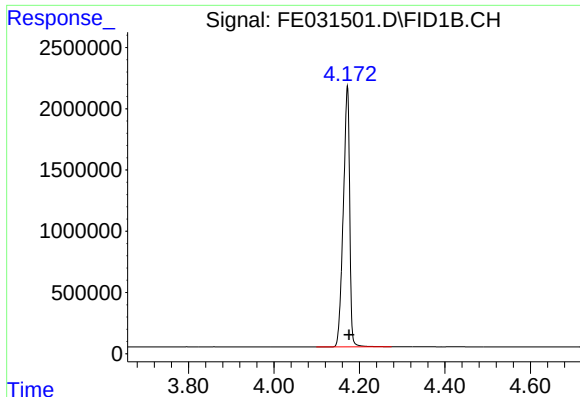


#2 N-DECANE

R.T.: 4.171 min
Delta R.T.: -0.004 min
Response: 22038099
Conc: 55.31 ug/ml

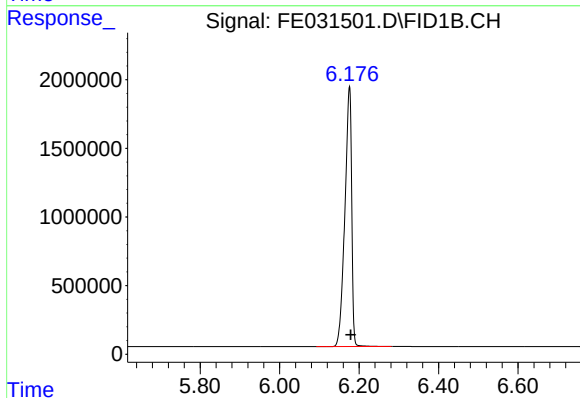


#3 N-DODECANE

R.T.: 6.175 min
Delta R.T.: -0.004 min
Response: 22533007
Conc: 55.00 ug/ml

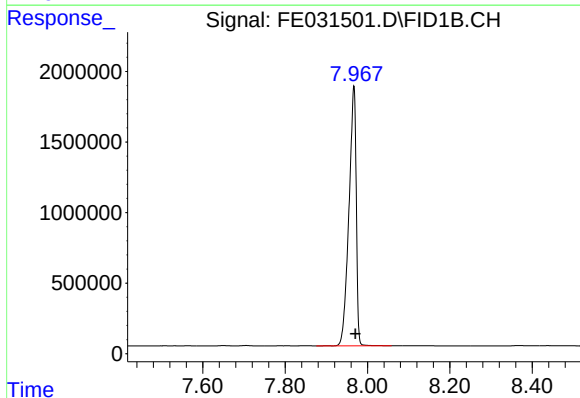


#4 N-TETRADECANE

R.T.: 7.966 min
Delta R.T.: -0.004 min
Response: 22585523
Conc: 54.31 ug/ml

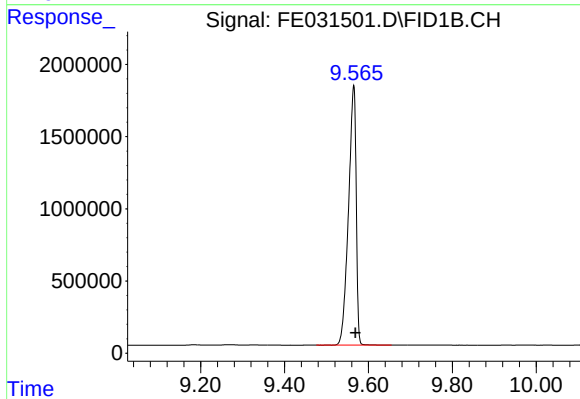


#5 N-HEXADECANE

R.T.: 9.564 min
Delta R.T.: -0.005 min
Response: 22848158
Conc: 53.73 ug/ml

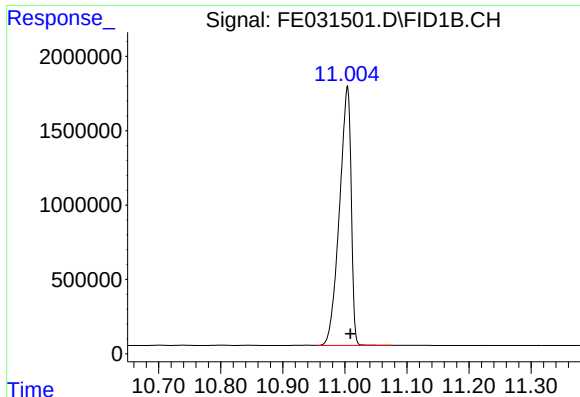


#6 N-OCTADECANE

R.T.: 11.003 min
Delta R.T.: -0.005 min
Response: 22792224
Conc: 53.22 ug/ml

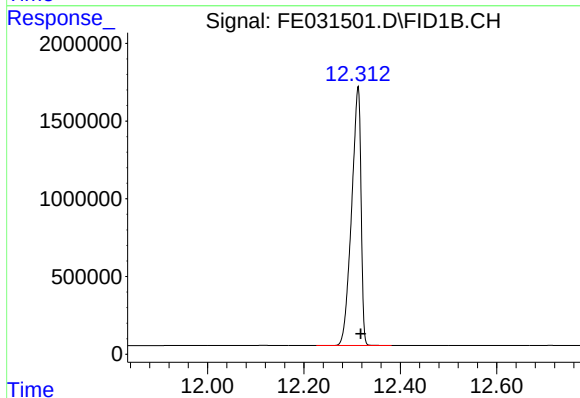


#7 N-EICOSANE

R.T.: 12.312 min
Delta R.T.: -0.006 min
Response: 22580423
Conc: 52.82 ug/ml

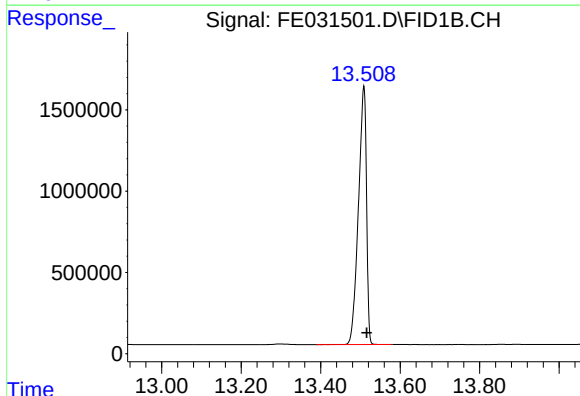


#8 N-DOCOSANE

R.T.: 13.508 min
Delta R.T.: -0.008 min
Response: 22372462
Conc: 52.44 ug/ml

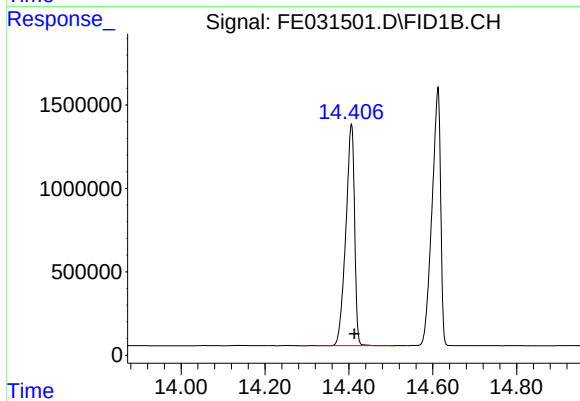


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.406 min
Delta R.T.: -0.008 min
Response: 19235183
Conc: 52.12 ug/ml

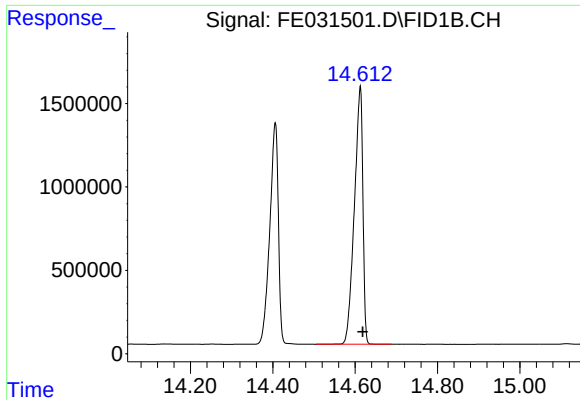


#10 N-TETRACOSANE

R.T.: 14.611 min
Delta R.T.: -0.007 min
Response: 22129301
Conc: 51.96 ug/ml

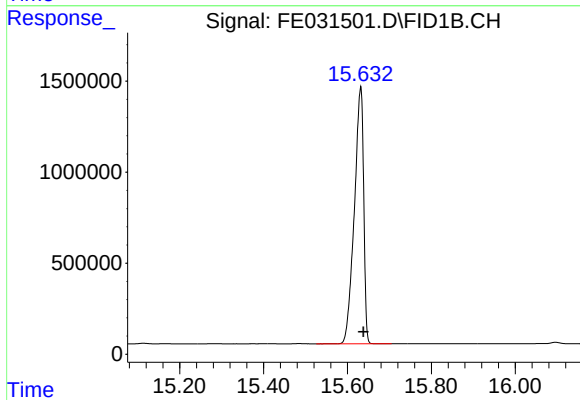

#11 N-HEXACOSANE

R.T.: 15.631 min
Delta R.T.: -0.007 min
Response: 21709674
Conc: 51.69 ug/ml

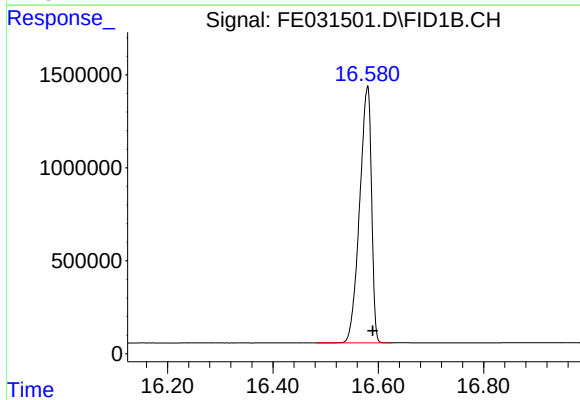

#12 N-OCTACOSANE

R.T.: 16.579 min
Delta R.T.: -0.011 min
Response: 21582269
Conc: 51.42 ug/ml