

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
 Data File : FE035376.D
 Signal(s) : FID1B.CH
 Acq On : 17 Mar 2022 15:39
 Operator : YP\AJ
 Sample : N1956-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 17 22:50:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 02:07:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.795	4747972	43.833 ug/ml
Spiked Amount 50.000		Recovery =	87.67%
Target Compounds			
4) T n-Dodecane (C12)	6.236	172556	<MDL ug/ml
6) T n-Tetradecane (C14)	8.021	94531	<MDL ug/ml
7) T n-Hexadecane (C16)	9.614	106711	<MDL ug/ml
8) T n-Octadecane (C18)	11.047	108160	<MDL ug/ml
10) T n-Eicosane (C20)	12.350	82738	<MDL ug/ml
11) T n-Heneicosane (C21)	12.960	54558	<MDL ug/ml
13) T n-Docosane (C22)	13.543	63881	<MDL ug/ml
15) T n-Hexacosane (C26)	15.656	34336	<MDL ug/ml
16) T n-Octacosane (C28)	16.603	201622	<MDL ug/ml
17) T n-Tricontane (C30)	17.481	162331	<MDL ug/ml
18) T n-Dotriacontane (C32)	18.313	78827	<MDL ug/ml
19) T n-Tetratriacontane (C34)	19.096	190326	2.133 ug/ml
20) T n-Hexatriacontane (C36)	19.831	99058	<MDL ug/ml
21) T n-Octatriacontane (C38)	20.532	65071	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
Data File : FE035376.D
Signal(s) : FID1B.CH
Acq On : 17 Mar 2022 15:39
Operator : YP\AJ
Sample : N1956-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 22:50:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 02:07:56 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

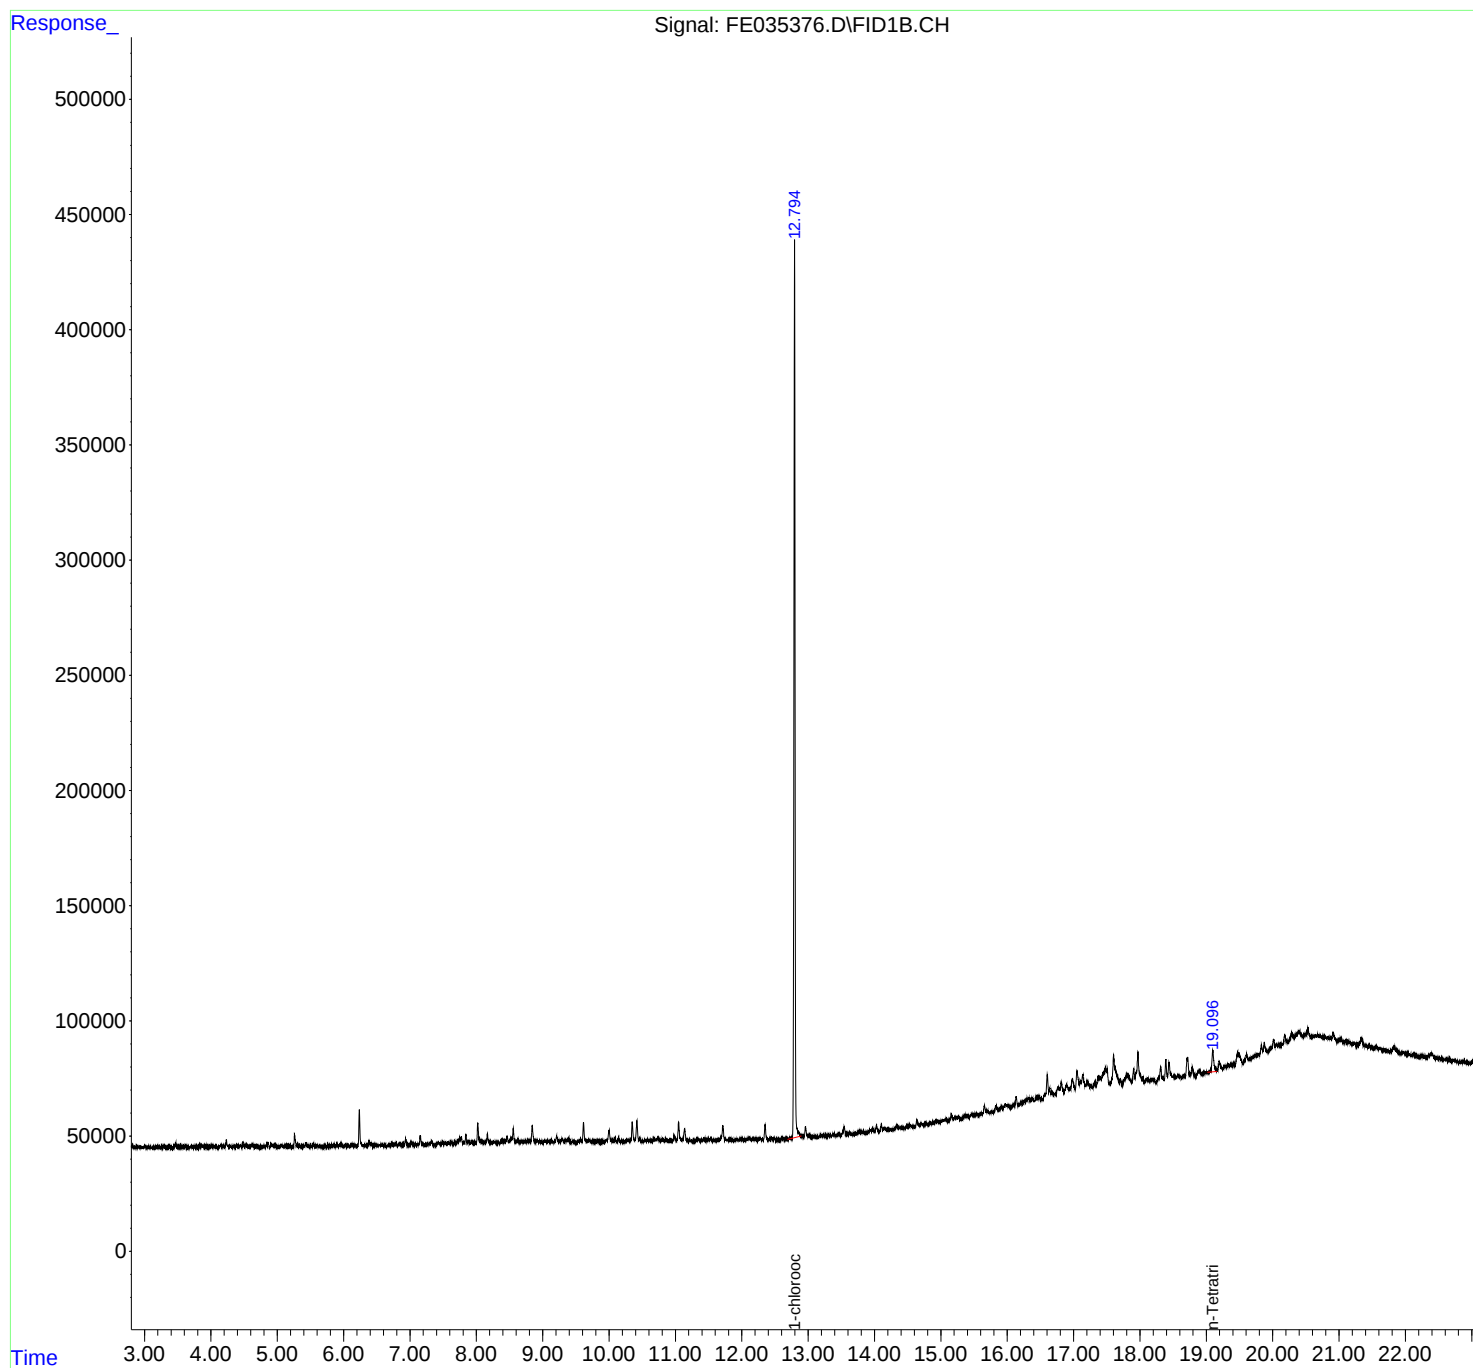


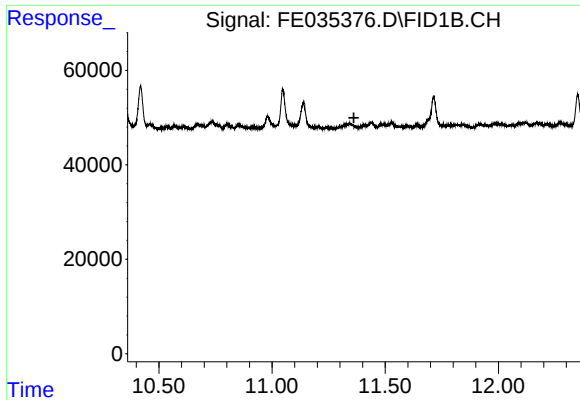

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.362 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

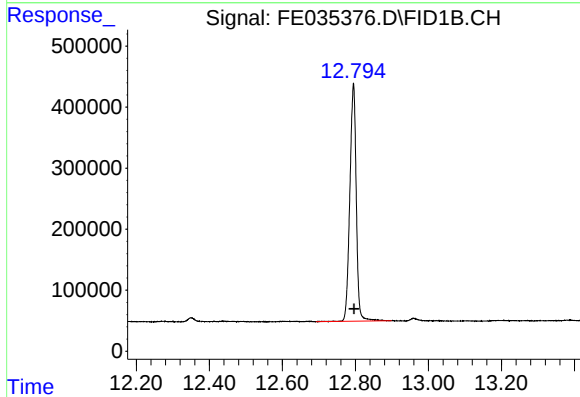

#12 1-chlorooctadecane (SURR)

R.T.: 12.795 min
Delta R.T.: -0.002 min
Response: 4747972
Conc: 43.83 ug/ml

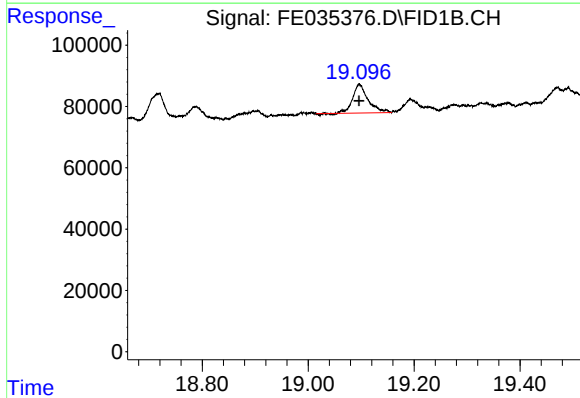

#19 n-Tetratriacontane (C34)

R.T.: 19.096 min
Delta R.T.: 0.000 min
Response: 190326
Conc: 2.13 ug/ml