

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
 Data File : FE035386.D
 Signal(s) : FID1B.CH
 Acq On : 17 Mar 2022 21:03
 Operator : YP\AJ
 Sample : N1924-09DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 33606DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2022
 Supervised By :Ankita Jodhani 03/18/2022

Integration File: sample.E
 Quant Time: Mar 17 22:52:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 02:07:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.356	1108300	8.002 ug/ml
Spiked Amount 50.000		Recovery =	16.00%
12) S 1-chlorooctadecane (S...	12.790	617081	5.697 ug/mlm
Spiked Amount 50.000		Recovery =	11.39%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
Data File : FE035386.D
Signal(s) : FID1B.CH
Acq On : 17 Mar 2022 21:03
Operator : YP\AJ
Sample : N1924-09DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
33606DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2022
Supervised By :Ankita Jodhani 03/18/2022

Integration File: sample.E
Quant Time: Mar 17 22:52:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 02:07:56 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

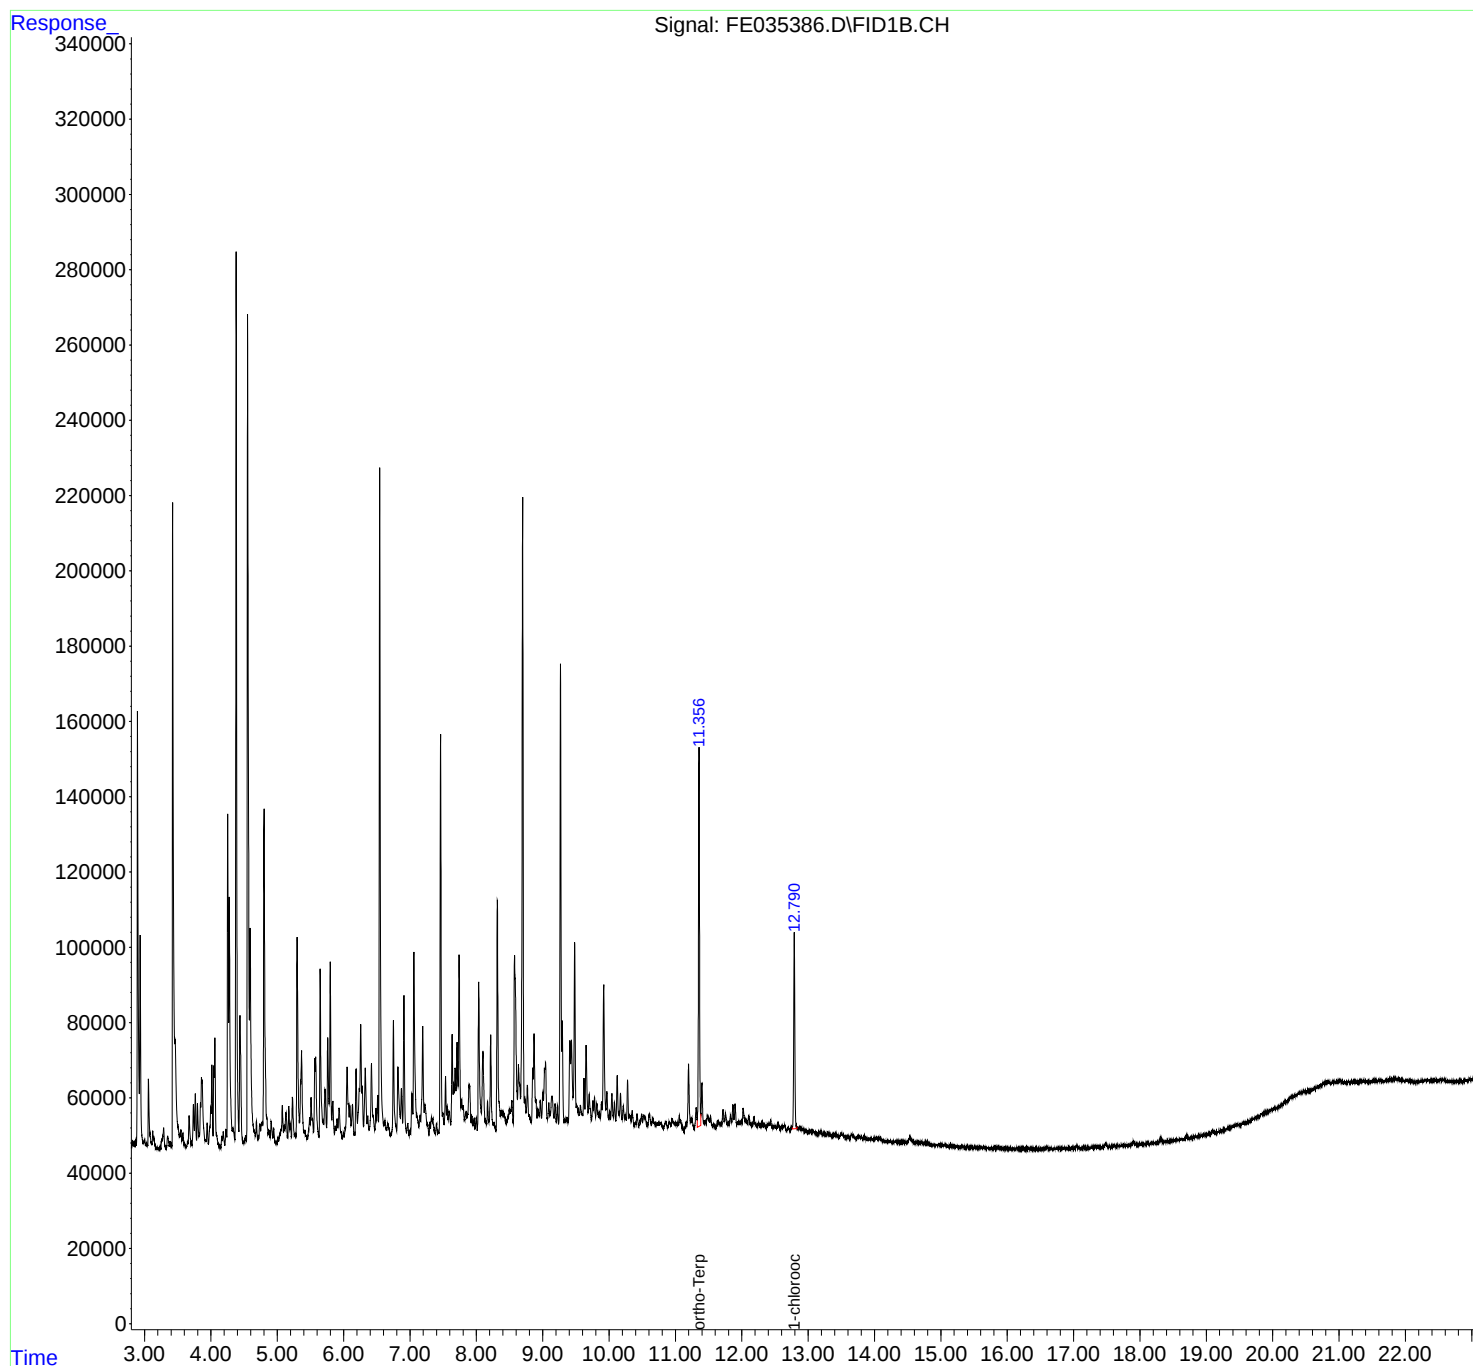

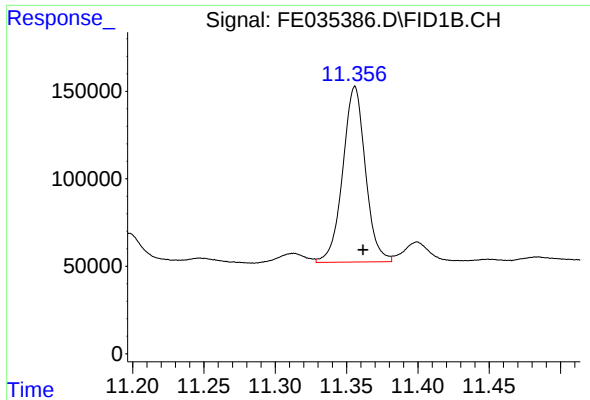


#9 ortho-Terphenyl (SURR)

R.T.: 11.356 min
Delta R.T.: -0.006 min
Response: 1108300
Conc: 8.00 ug/ml

Instrument :
FID_E
ClientSampleId :
33606DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2022
Supervised By :Ankita Jodhani 03/18/2022

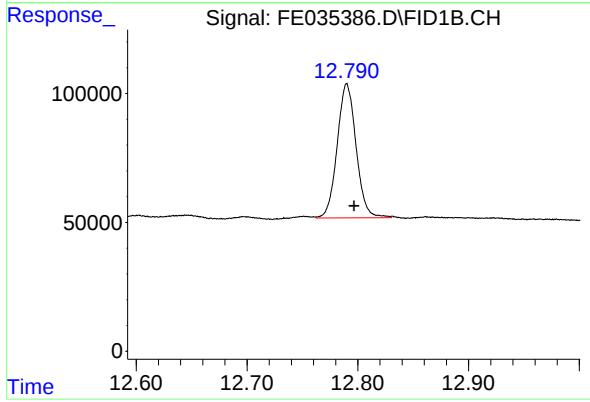

#12 1-chlorooctadecane (SURR)

R.T.: 12.790 min
Delta R.T.: -0.007 min
Response: 617081
Conc: 5.70 ug/ml m