

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
 Data File : FE035393.D
 Signal(s) : FID1B.CH
 Acq On : 18 Mar 2022 00:49
 Operator : YP\AJ
 Sample : N1944-03DL 50X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 CHRT-24449DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2022
 Supervised By :Ankita Jodhani 03/18/2022

Integration File: sample.E
 Quant Time: Mar 18 02:59:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 02:07:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.360	277106	2.001 ug/mlm
Spiked Amount 50.000		Recovery =	4.00%
12) S 1-chlorooctadecane (S...	12.797	75656	<MDL ug/mlm
Spiked Amount 50.000		Recovery =	0.00%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031722AL\
Data File : FE035393.D
Signal(s) : FID1B.CH
Acq On : 18 Mar 2022 00:49
Operator : YP\AJ
Sample : N1944-03DL 50X
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
CHRT-24449DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2022
Supervised By :Ankita Jodhani 03/18/2022

Integration File: sample.E
Quant Time: Mar 18 02:59:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 02:07:56 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

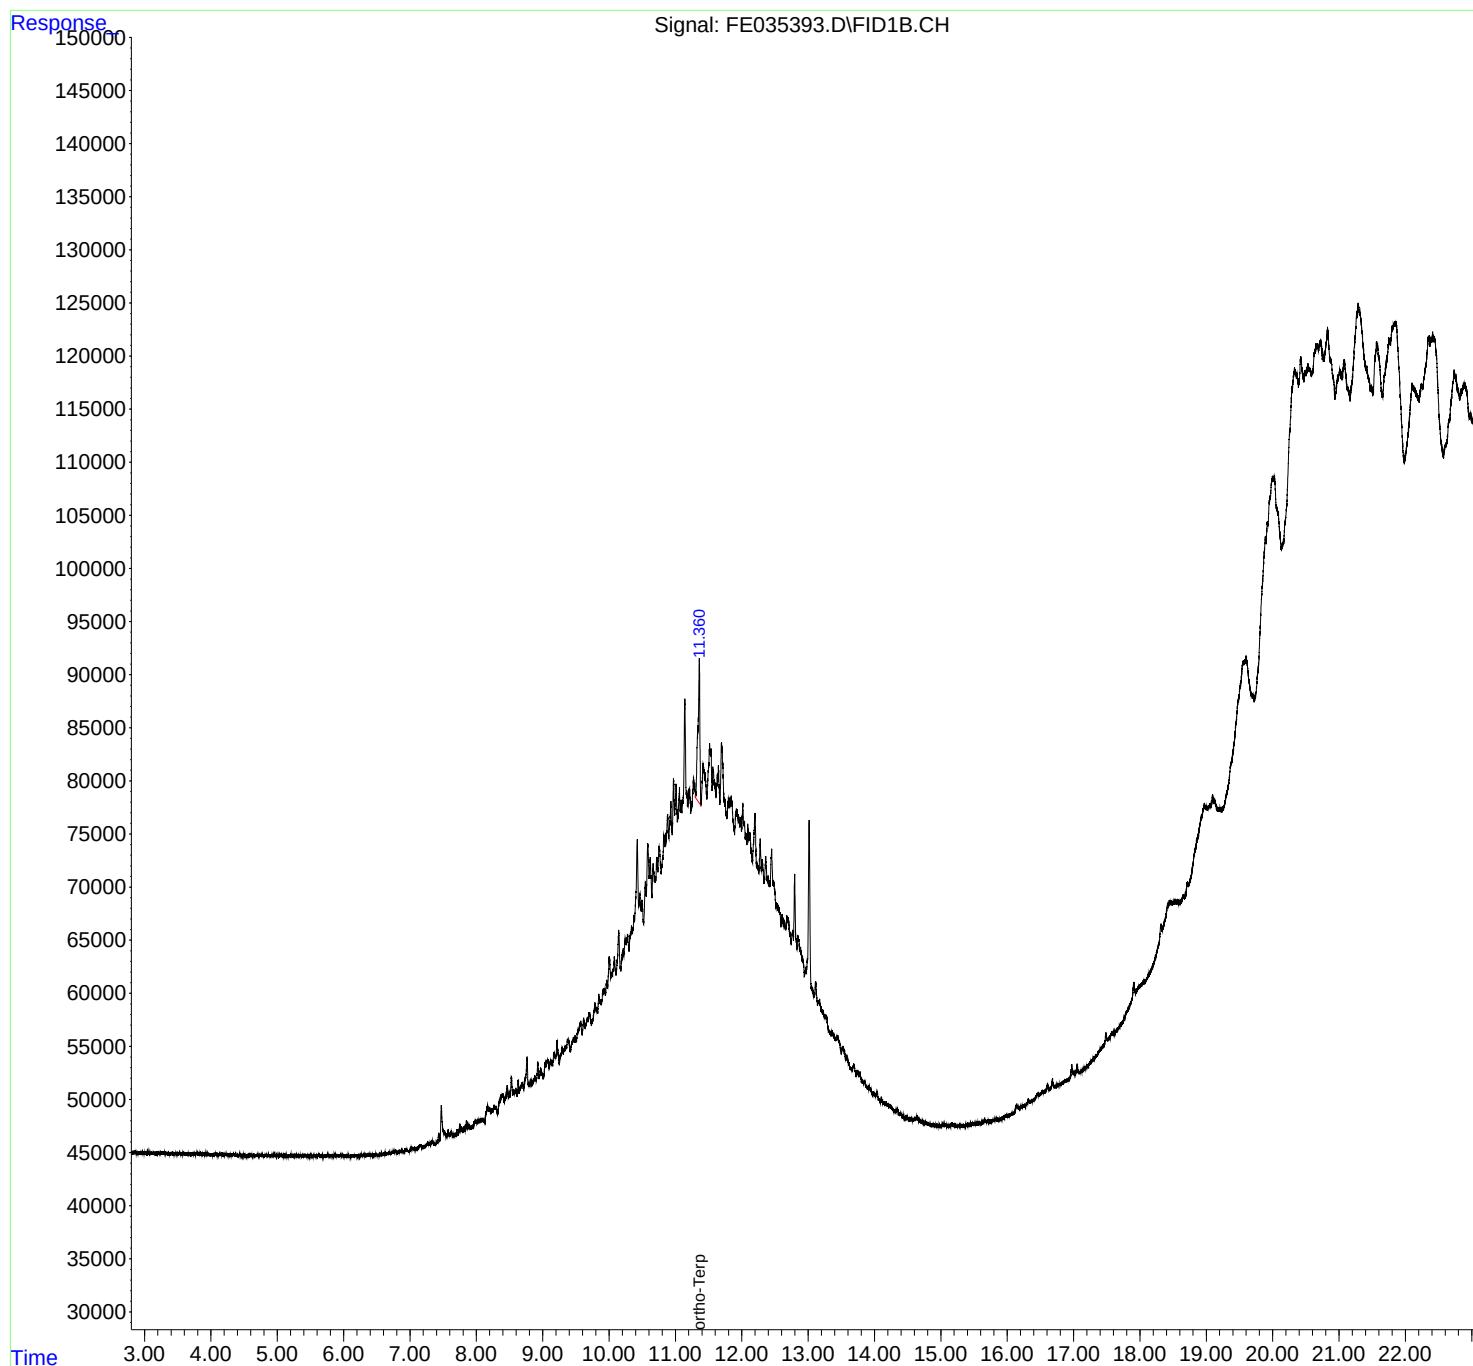

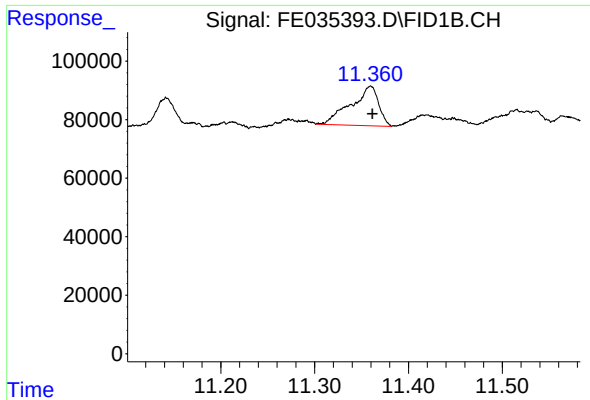


#9 ortho-Terphenyl (SURR)

R.T.: 11.360 min
Delta R.T.: -0.002 min
Response: 277106
Conc: 2.00 ug/ml

Instrument :
FID_E
ClientSampleId :
CHRT-24449DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2022
Supervised By :Ankita Jodhani 03/18/2022

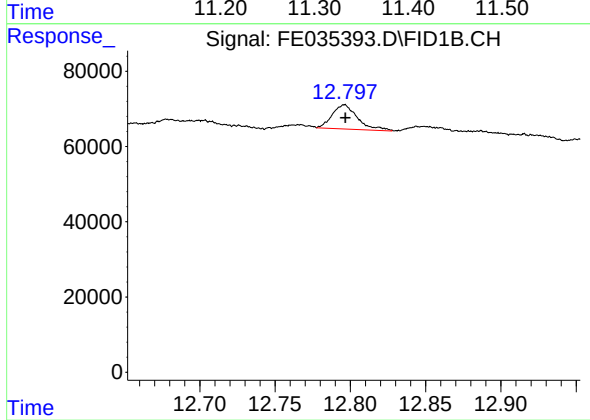

#12 1-chlorooctadecane (SURR)

R.T.: 12.797 min
Delta R.T.: 0.000 min
Response: 75656
Conc: N.D.