

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031820\
 Data File : FE031504.D
 Signal(s) : FID1B.CH
 Acq On : 18 Mar 2020 10:55
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 19 00:54:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Wed Mar 11 09:35:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.401	18179168	49.256 ug/ml
Target Compounds			
2) N-DECANE	4.171	21030637	52.781 ug/ml
3) N-DODECANE	6.173	21423809	52.290 ug/ml
4) N-TETRADECANE	7.964	21453781	51.586 ug/ml
5) N-HEXADECANE	9.562	21657510	50.932 ug/ml
6) N-OCTADECANE	11.000	21580517	50.392 ug/ml
7) N-EICOSANE	12.307	21348236	49.940 ug/ml
8) N-DOCOSANE	13.504	21121825	49.506 ug/ml
10) N-TETRACOSANE	14.607	20853264	48.968 ug/ml
11) N-HEXACOSANE	15.625	20425101	48.629 ug/ml
12) N-OCTACOSANE	16.573	20320464	48.418 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031820\
Data File : FE031504.D
Signal(s) : FID1B.CH
Acq On : 18 Mar 2020 10:55
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 00:54:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Wed Mar 11 09:35:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

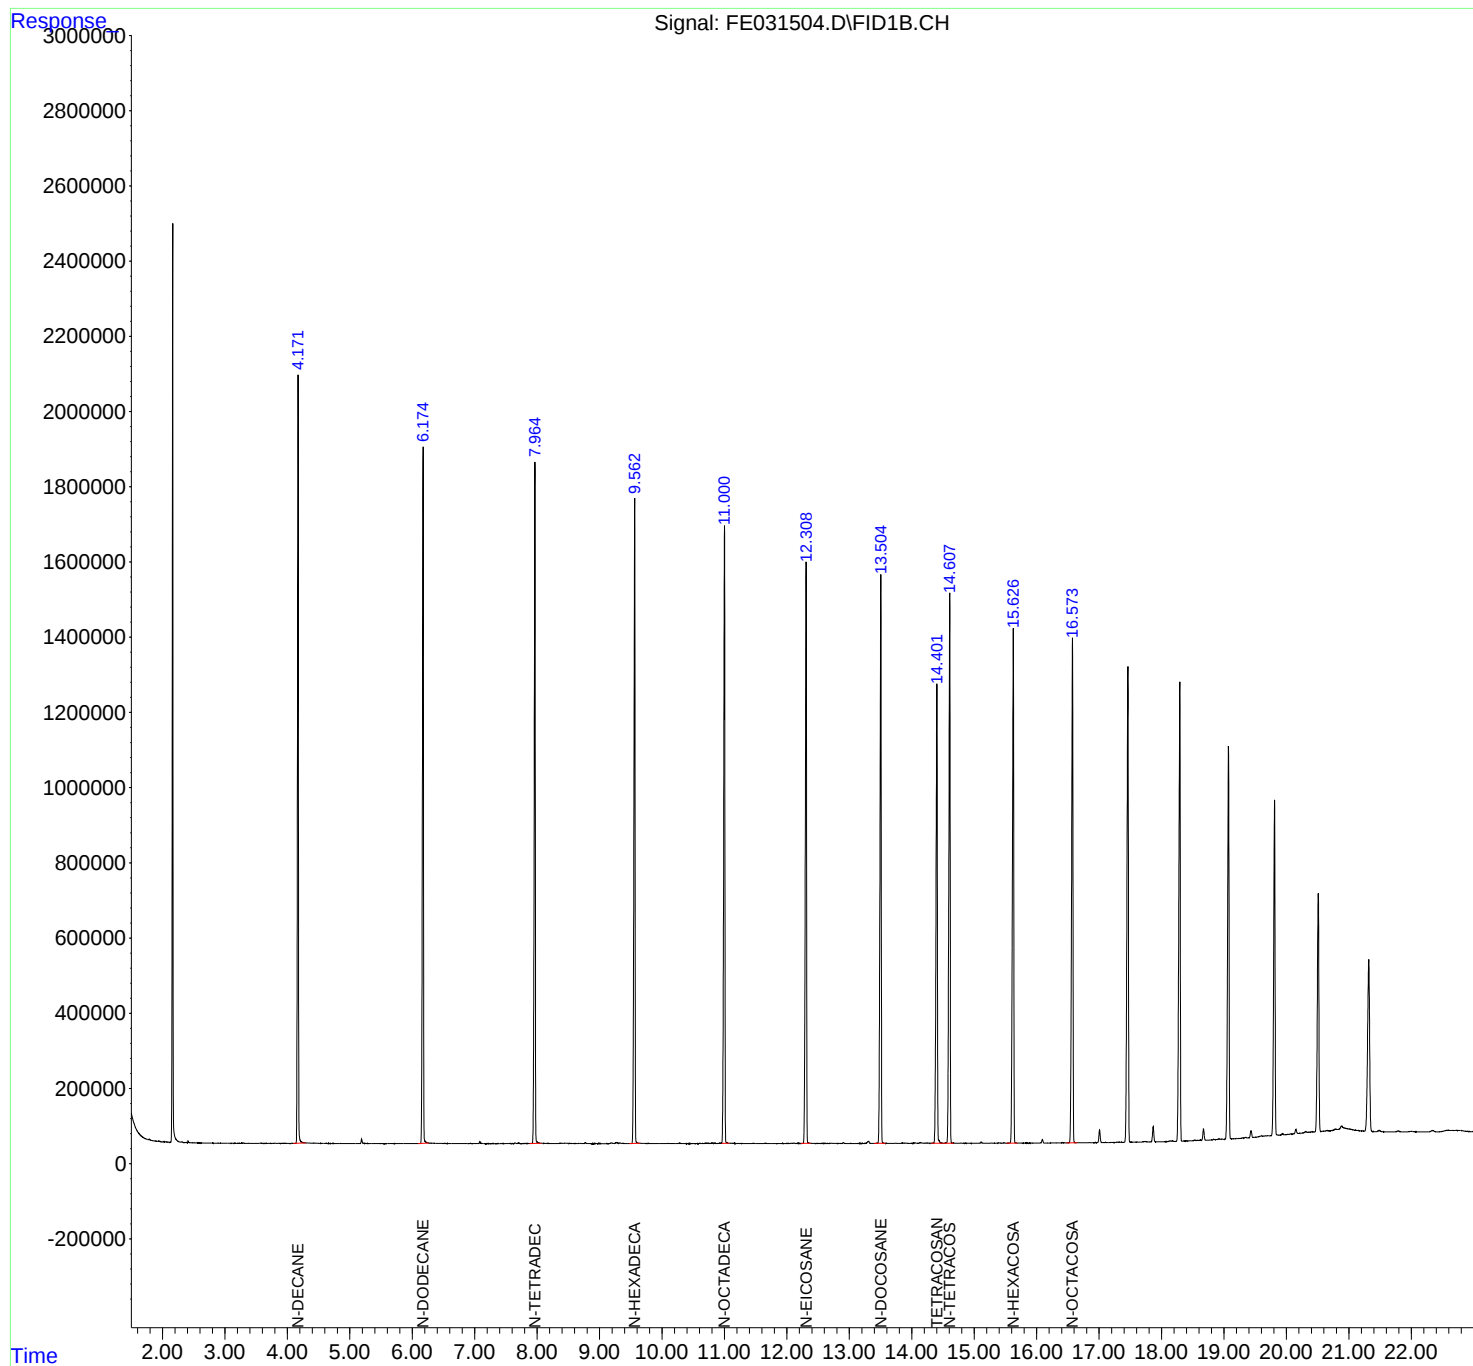

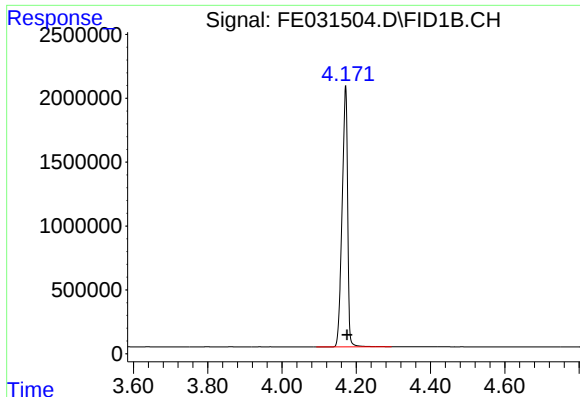


#2 N-DECANE

R.T.: 4.171 min
Delta R.T.: -0.004 min
Response: 21030637
Conc: 52.78 ug/ml

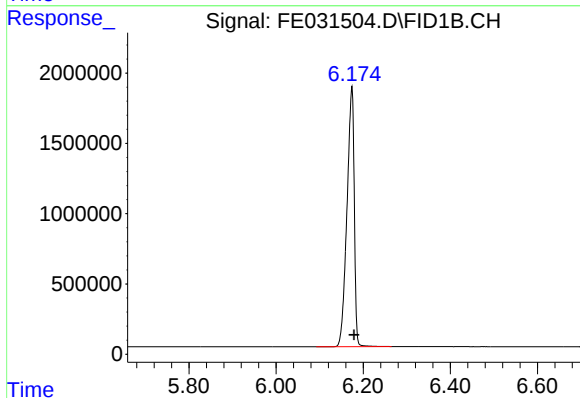


#3 N-DODECANE

R.T.: 6.173 min
Delta R.T.: -0.006 min
Response: 21423809
Conc: 52.29 ug/ml

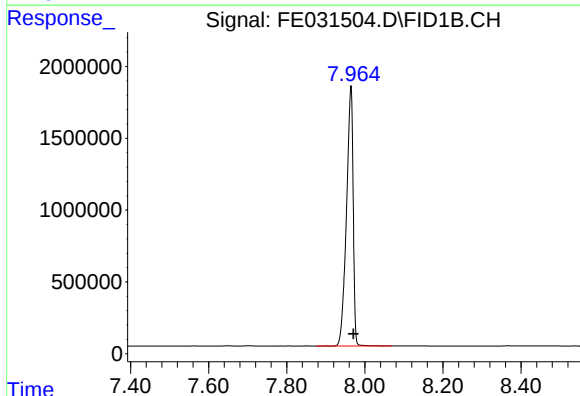


#4 N-TETRADECANE

R.T.: 7.964 min
Delta R.T.: -0.007 min
Response: 21453781
Conc: 51.59 ug/ml

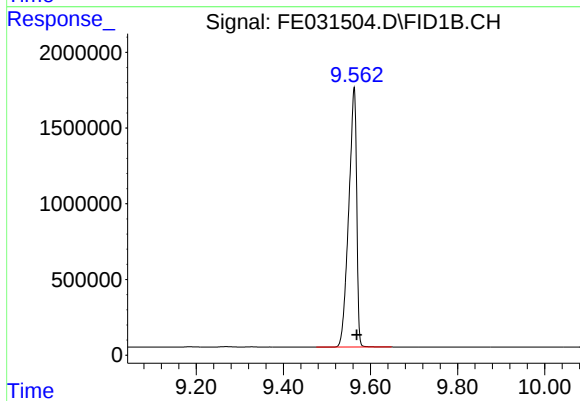


#5 N-HEXADECANE

R.T.: 9.562 min
Delta R.T.: -0.007 min
Response: 21657510
Conc: 50.93 ug/ml

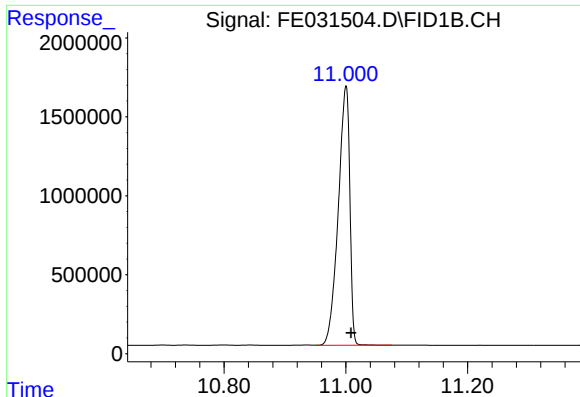


#6 N-OCTADECANE

R.T.: 11.000 min
Delta R.T.: -0.009 min
Response: 21580517
Conc: 50.39 ug/ml

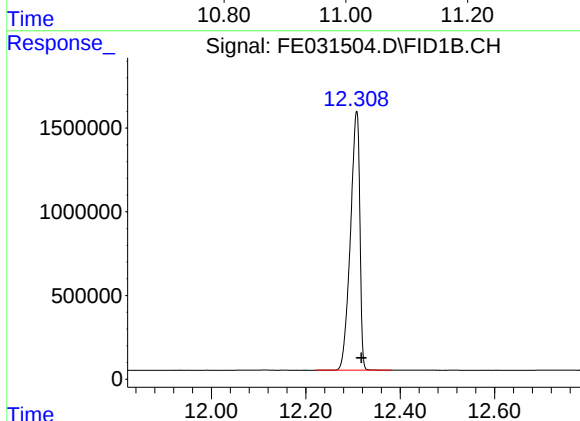


#7 N-EICOSANE

R.T.: 12.307 min
Delta R.T.: -0.010 min
Response: 21348236
Conc: 49.94 ug/ml

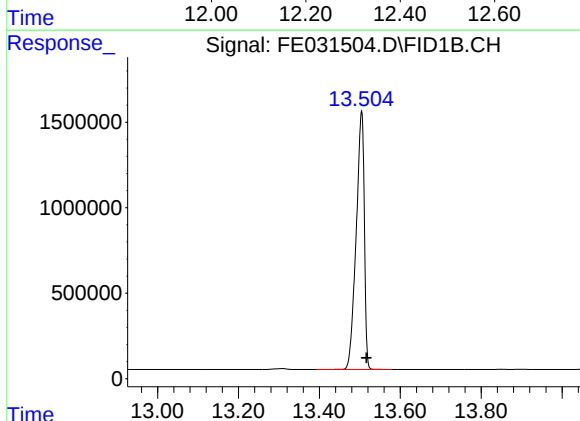


#8 N-DOCOSANE

R.T.: 13.504 min
Delta R.T.: -0.012 min
Response: 21121825
Conc: 49.51 ug/ml

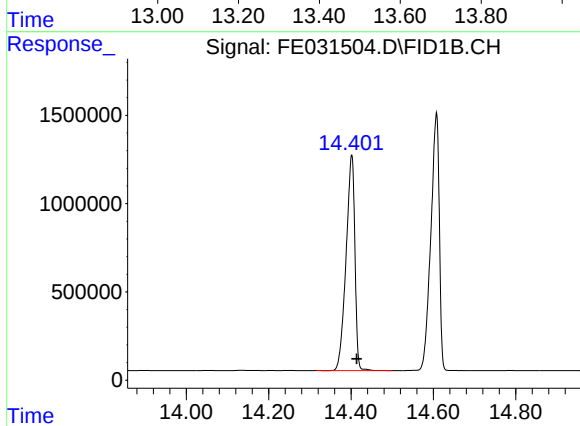


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.401 min
Delta R.T.: -0.012 min
Response: 18179168
Conc: 49.26 ug/ml

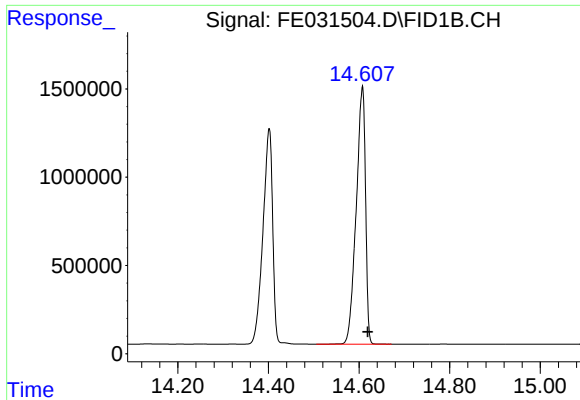


#10 N-TETRACOSANE

R.T.: 14.607 min
Delta R.T.: -0.012 min
Response: 20853264
Conc: 48.97 ug/ml

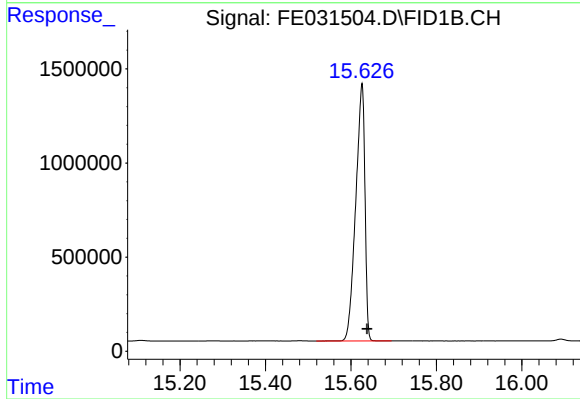

#11 N-HEXACOSANE

R.T.: 15.625 min
Delta R.T.: -0.013 min
Response: 20425101
Conc: 48.63 ug/ml

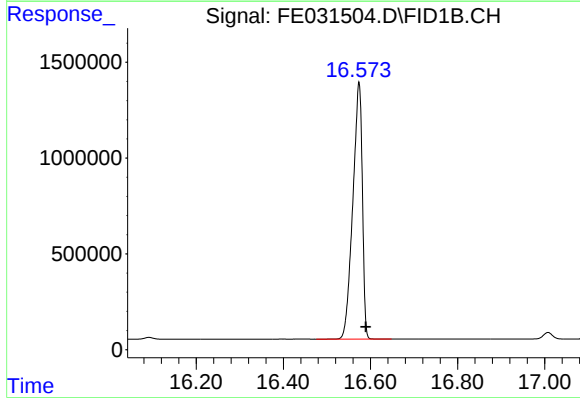

#12 N-OCTACOSANE

R.T.: 16.573 min
Delta R.T.: -0.016 min
Response: 20320464
Conc: 48.42 ug/ml