

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031824AL\
 Data File : FE047202.D
 Signal(s) : FID1B.ch
 Acq On : 18 Mar 2024 16:04
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 04:07:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 031324.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 14 01:54:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.942	13913	0.101 ug/ml
19) T	n-Tetratriacontane (C34)	19.721	29824	0.228 ug/ml
20) T	n-Hexatriacontane (C36)	20.460	27926	0.224 ug/ml
21) T	n-Octatriacontane (C38)	21.203	45396	0.366 ug/ml
22) T	n-Tetracontane (C40)	22.129	39024	0.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031824AL\
Data File : FE047202.D
Signal(s) : FID1B.ch
Acq On : 18 Mar 2024 16:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 04:07:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 031324.M
Quant Title : GC Extractables
QLast Update : Thu Mar 14 01:54:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

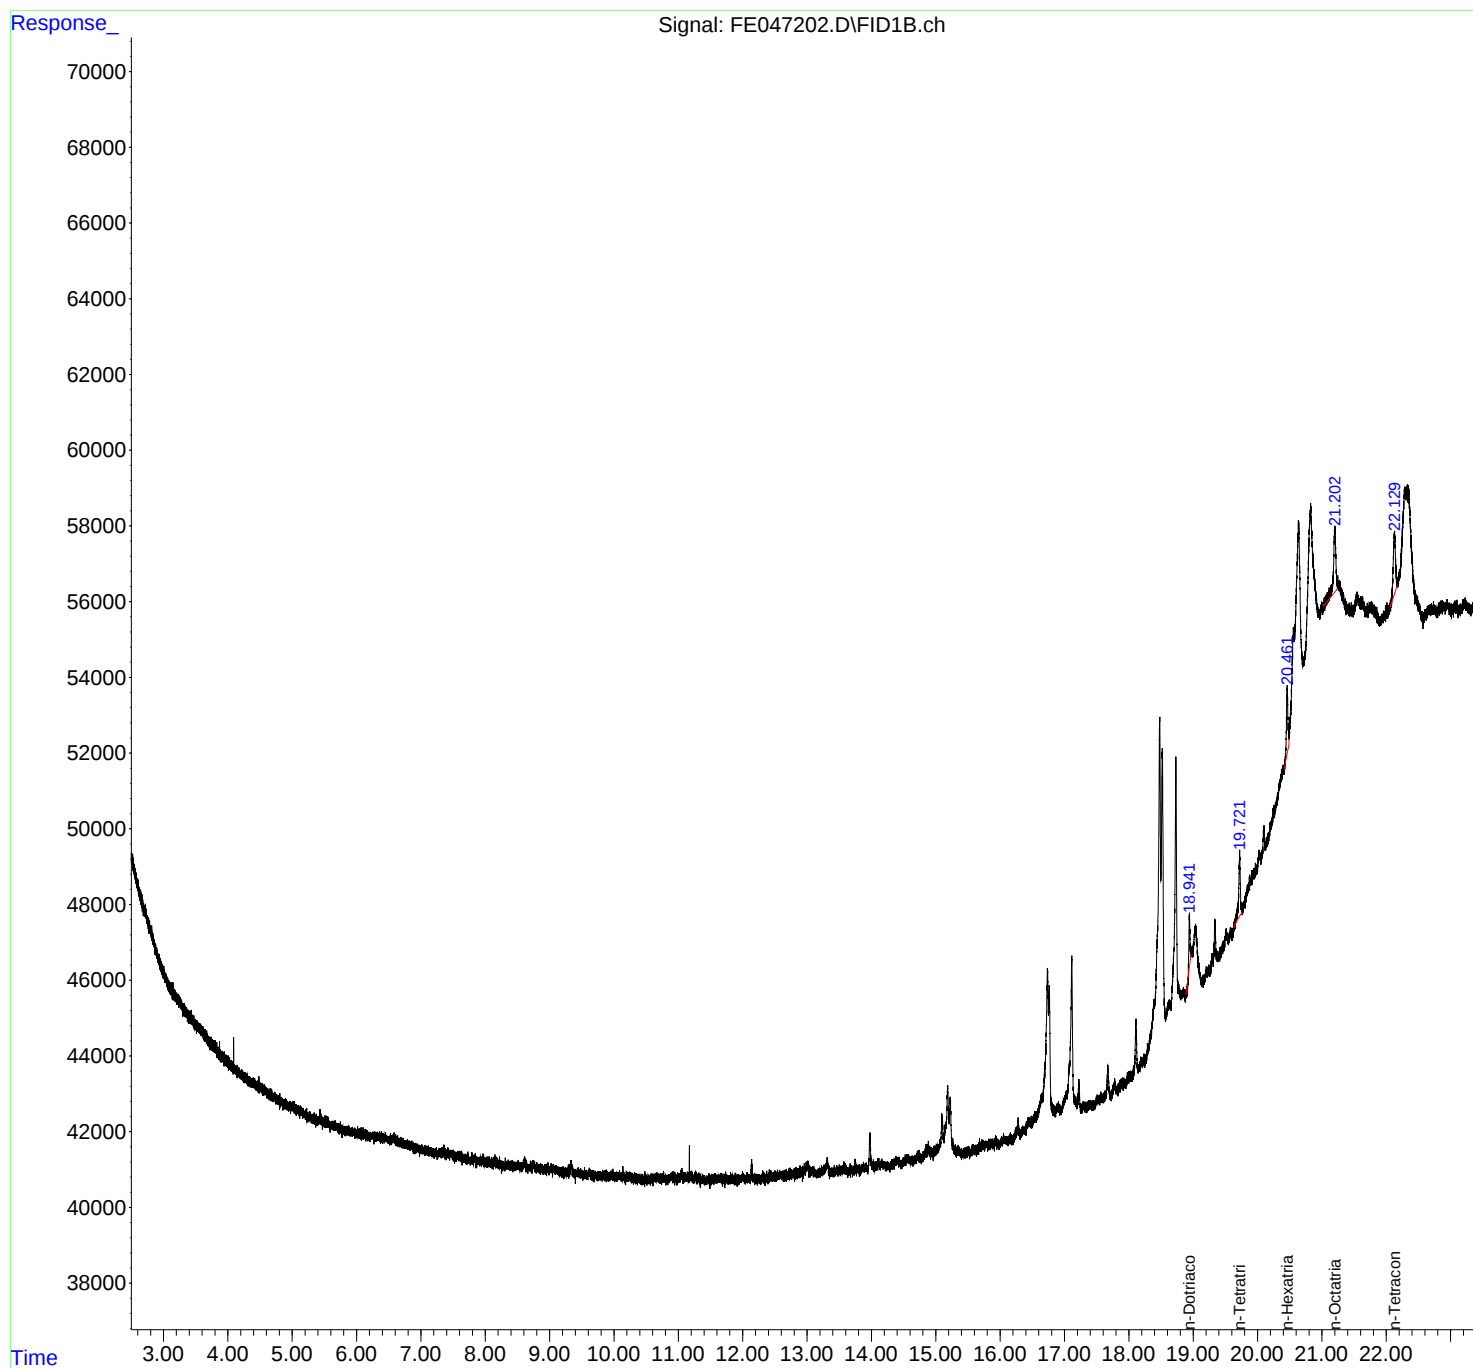


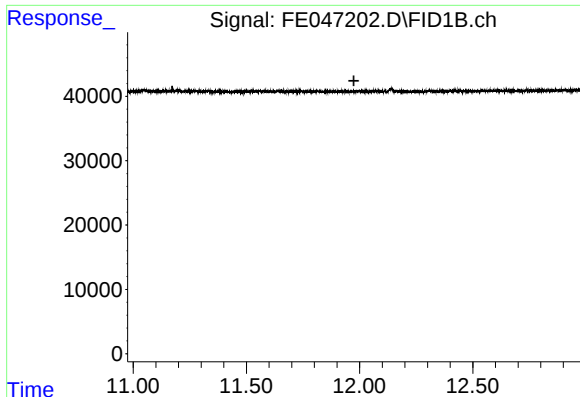

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.975 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

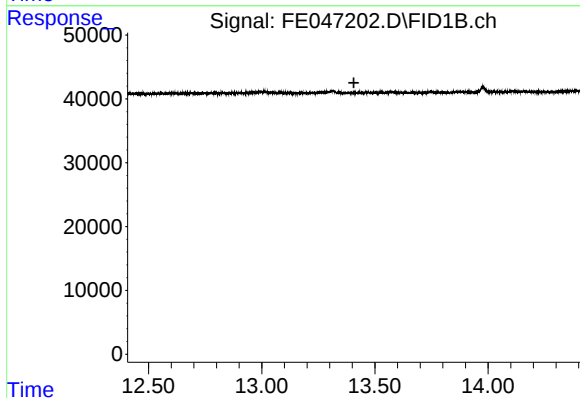


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.407 min
Response: 0
Conc: N.D.

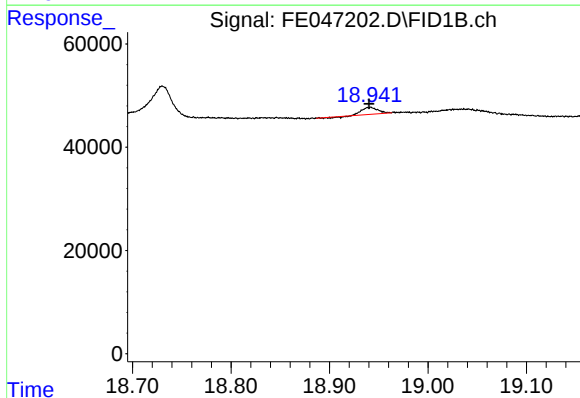


#18 n-Dotriacontane (C32)

R.T.: 18.942 min
Delta R.T.: 0.002 min
Response: 13913
Conc: 0.10 ug/ml

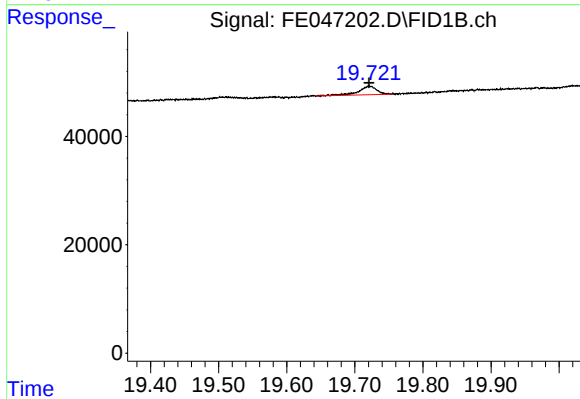

#19 n-Tetratriacontane (C34)


R.T.: 19.721 min
Delta R.T.: 0.000 min
Response: 29824
Conc: 0.23 ug/ml

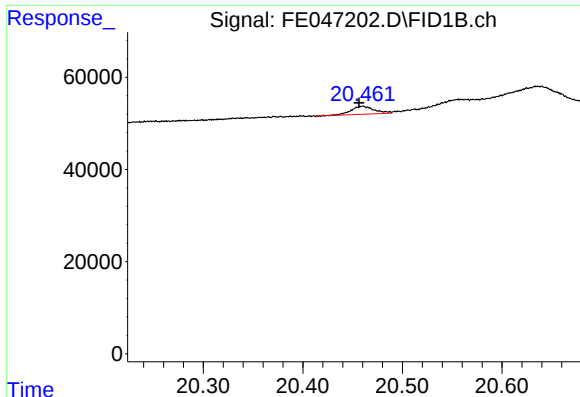

#20 n-Hexatriacontane (C36)


R.T.: 20.460 min
Delta R.T.: 0.003 min
Response: 27926
Conc: 0.22 ug/ml

Instrument :
FID_E
ClientSampleId :

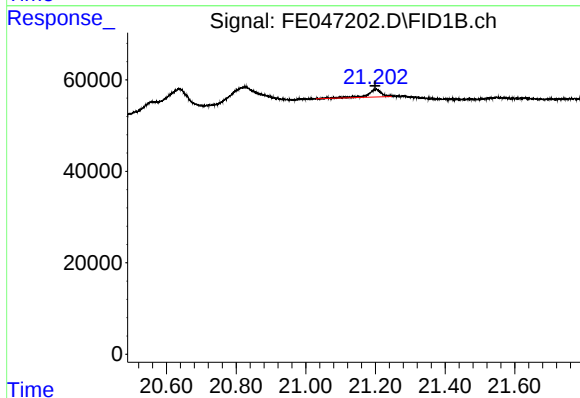

#21 n-Octatriacontane (C38)

R.T.: 21.203 min
Delta R.T.: 0.003 min
Response: 45396
Conc: 0.37 ug/ml

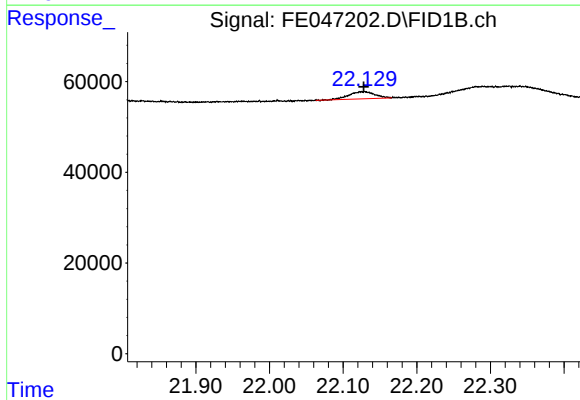

#22 n-Tetracontane (C40)

R.T.: 22.129 min
Delta R.T.: 0.001 min
Response: 39024
Conc: 0.33 ug/ml