

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031920\
 Data File : FE031519.D
 Signal(s) : FID1B.CH
 Acq On : 19 Mar 2020 13:45
 Operator : DD\AJ
 Sample : L1759-11MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 20 08:14:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:14:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.442	9411414	25.500 ug/mlm
Target Compounds			
2) N-DECANE	4.171	6190561	15.536 ug/ml
3) N-DODECANE	6.178	7738668	18.888 ug/ml
4) N-TETRADECANE	7.971	8949116	21.518 ug/ml
5) N-HEXADECANE	9.571	8784460	20.658 ug/ml
6) N-OCTADECANE	11.014	9061739	21.160 ug/ml
7) N-EICOSANE	12.331	9014919	21.089 ug/mlm
8) N-DOCOSANE	13.530	10533619	24.689 ug/mlm
10) N-TETRACOSANE	14.648	20792870	48.826 ug/mlm
11) N-HEXACOSANE	15.681	8838457	21.043 ug/mlm
12) N-OCTACOSANE	16.656	9747756	23.226 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031920\
Data File : FE031519.D
Signal(s) : FID1B.CH
Acq On : 19 Mar 2020 13:45
Operator : DD\AJ
Sample : L1759-11MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 08:14:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:14:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

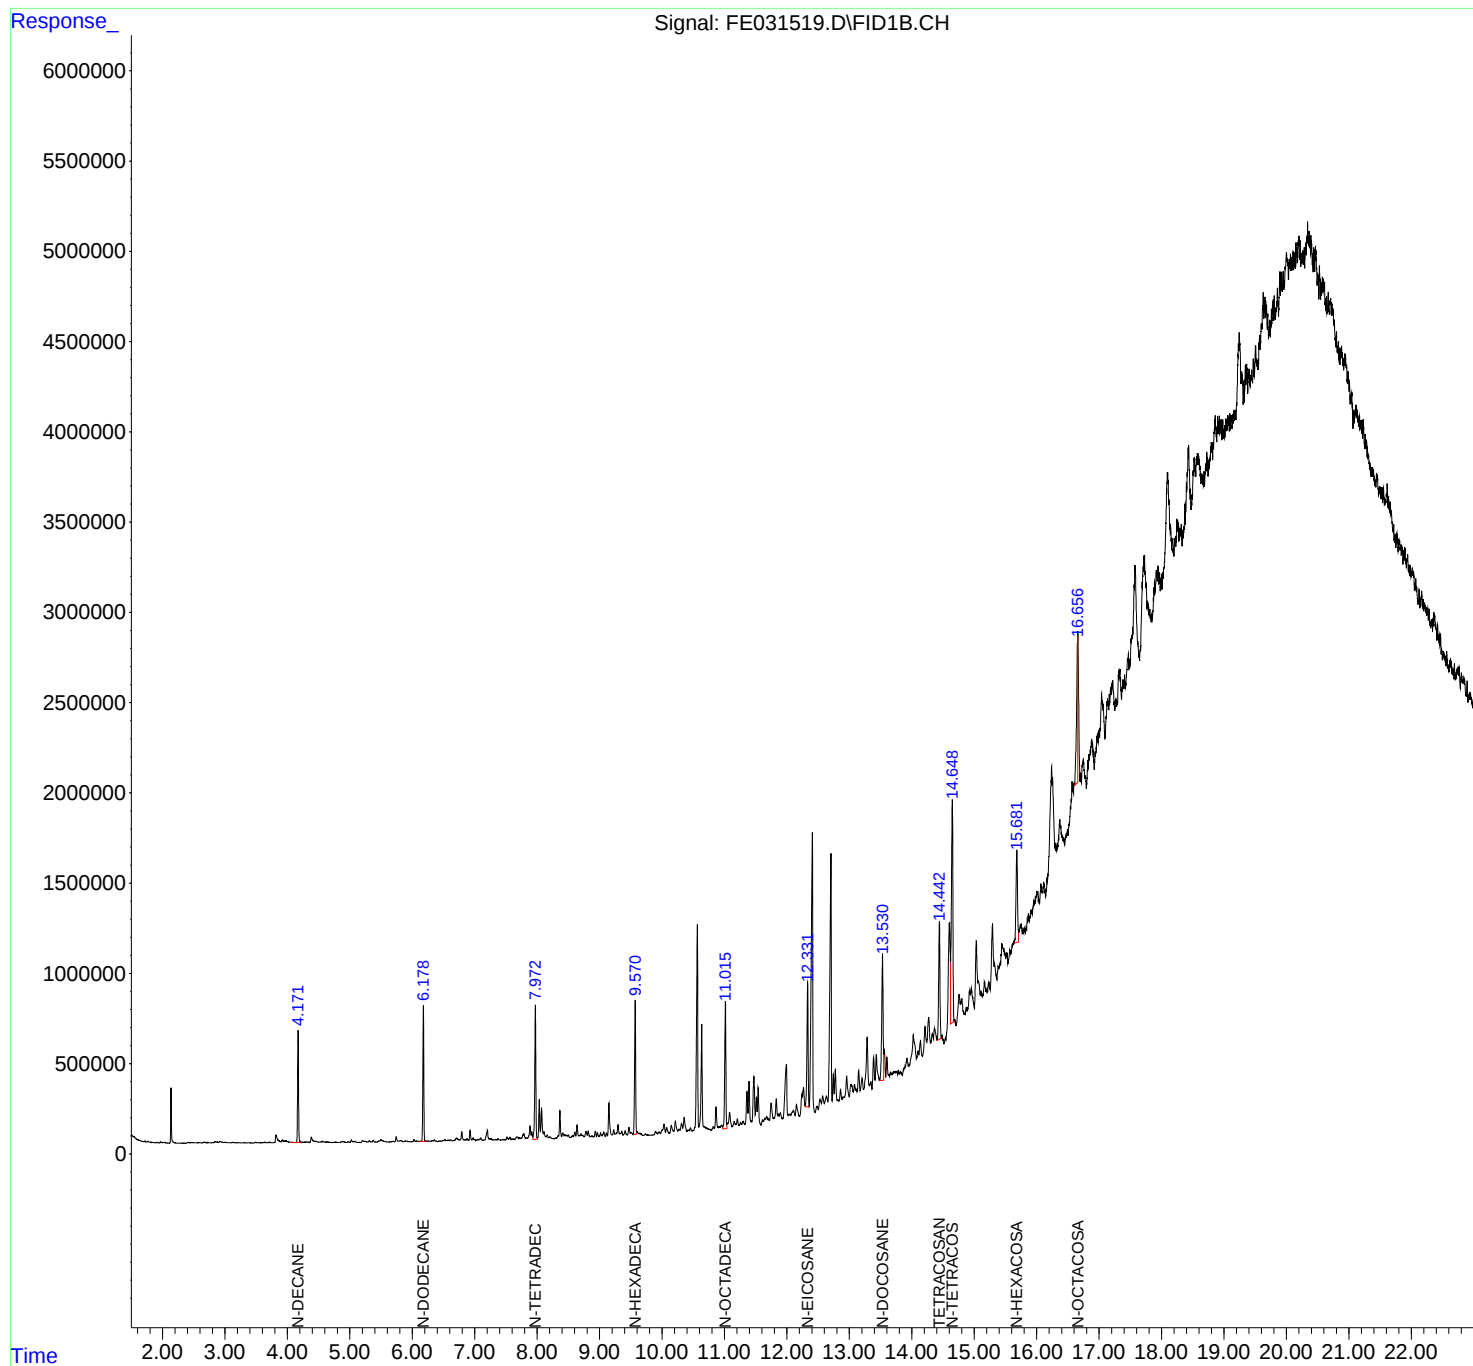

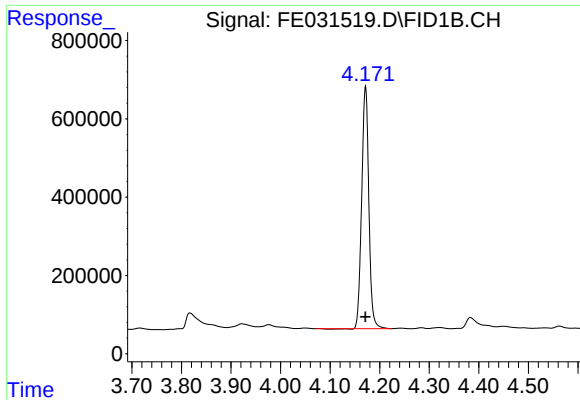


#2 N-DECANE

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 6190561
Conc: 15.54 ug/ml

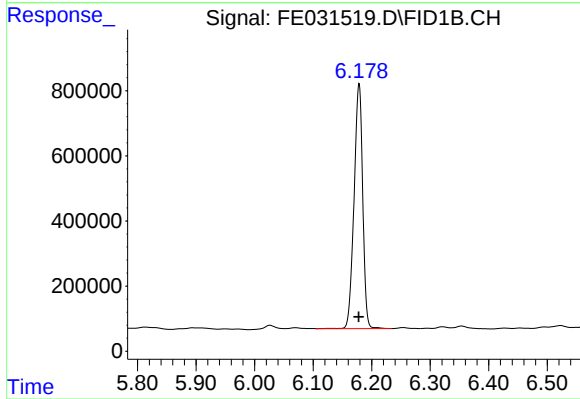


#3 N-DODECANE

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 7738668
Conc: 18.89 ug/ml

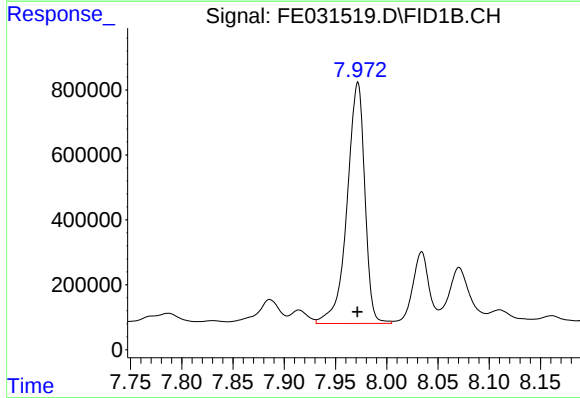


#4 N-TETRADECANE

R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 8949116
Conc: 21.52 ug/ml

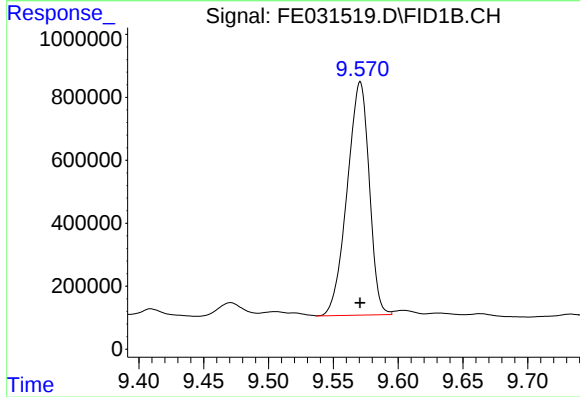


#5 N-HEXADECANE

R.T.: 9.571 min
Delta R.T.: 0.000 min
Response: 8784460
Conc: 20.66 ug/ml

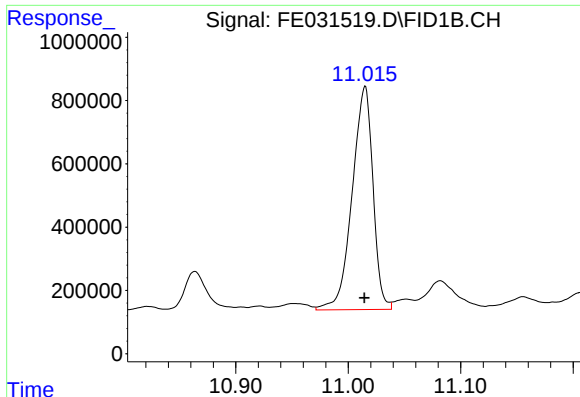


#6 N-OCTADECANE

R.T.: 11.014 min
Delta R.T.: 0.000 min
Response: 9061739
Conc: 21.16 ug/ml

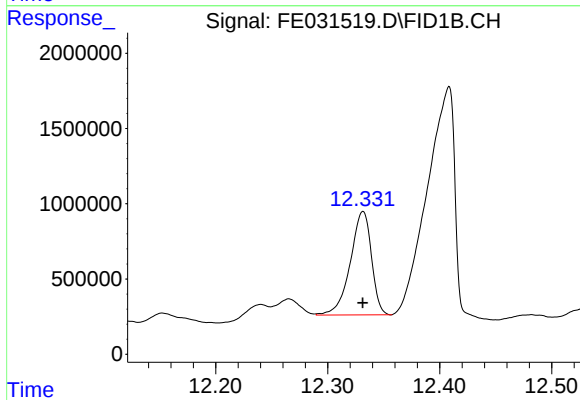


#7 N-EICOSANE

R.T.: 12.331 min
Delta R.T.: 0.000 min
Response: 9014919
Conc: 21.09 ug/ml m

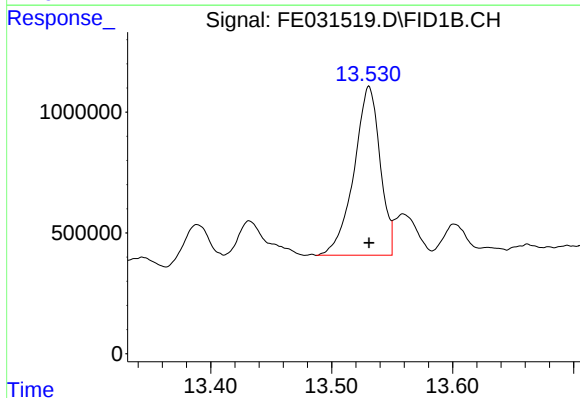


#8 N-DOCOSANE

R.T.: 13.530 min
Delta R.T.: 0.000 min
Response: 10533619
Conc: 24.69 ug/ml m

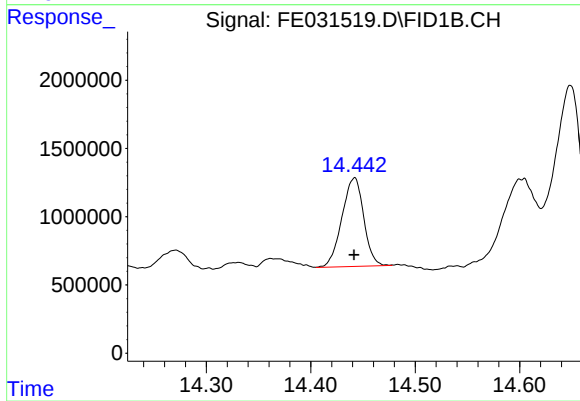


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.442 min
Delta R.T.: 0.000 min
Response: 9411414
Conc: 25.50 ug/ml m

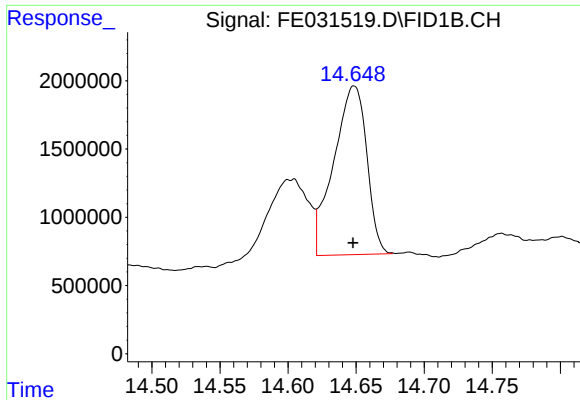


#10 N-TETRACOSANE

R.T.: 14.648 min
Delta R.T.: 0.000 min
Response: 20792870
Conc: 48.83 ug/ml m

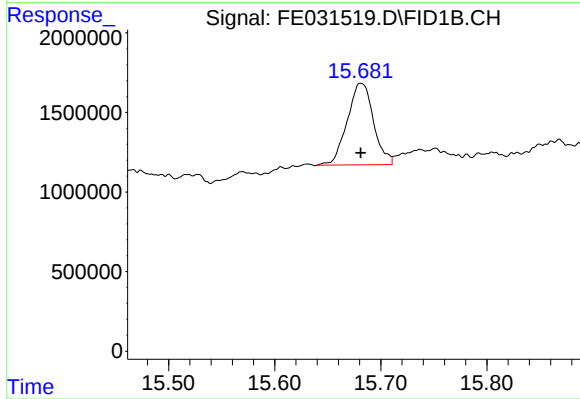

#11 N-HEXACOSANE

R.T.: 15.681 min
Delta R.T.: 0.000 min
Response: 8838457
Conc: 21.04 ug/ml m

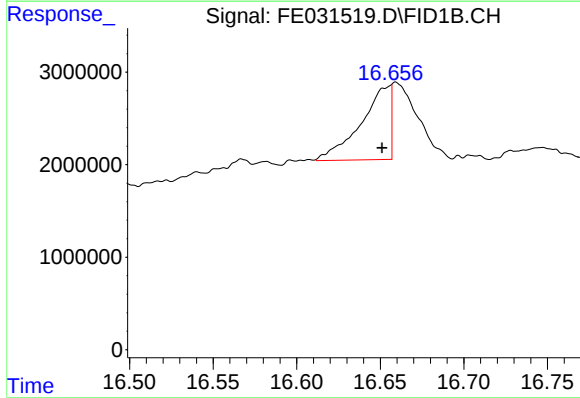

#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: 0.005 min
Response: 9747756
Conc: 23.23 ug/ml m