

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032119\
 Data File : FE029746.D
 Signal(s) : FID1B.CH
 Acq On : 21 Mar 2019 13:31
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 22 02:34:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
 Quant Title :
 QLast Update : Wed Mar 20 08:08:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
5) N-DODECANE	6.400	4050382	25.041 ug/ml
8) N-OCTADECANE	11.236	55454	0.297 ug/ml
11) N-OCTACOSANE	16.834	3981365	27.547 ug/ml
12) N-DOTRIACONTANE	18.553	319370	1.949 ug/ml
14) N-HEXATRIACONTANE	20.080	75818	0.525 ug/ml
16) N-TETRTETRACOCANE	24.387	310329	3.174 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032119\
Data File : FE029746.D
Signal(s) : FID1B.CH
Acq On : 21 Mar 2019 13:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 02:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
Quant Title :
QLast Update : Wed Mar 20 08:08:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

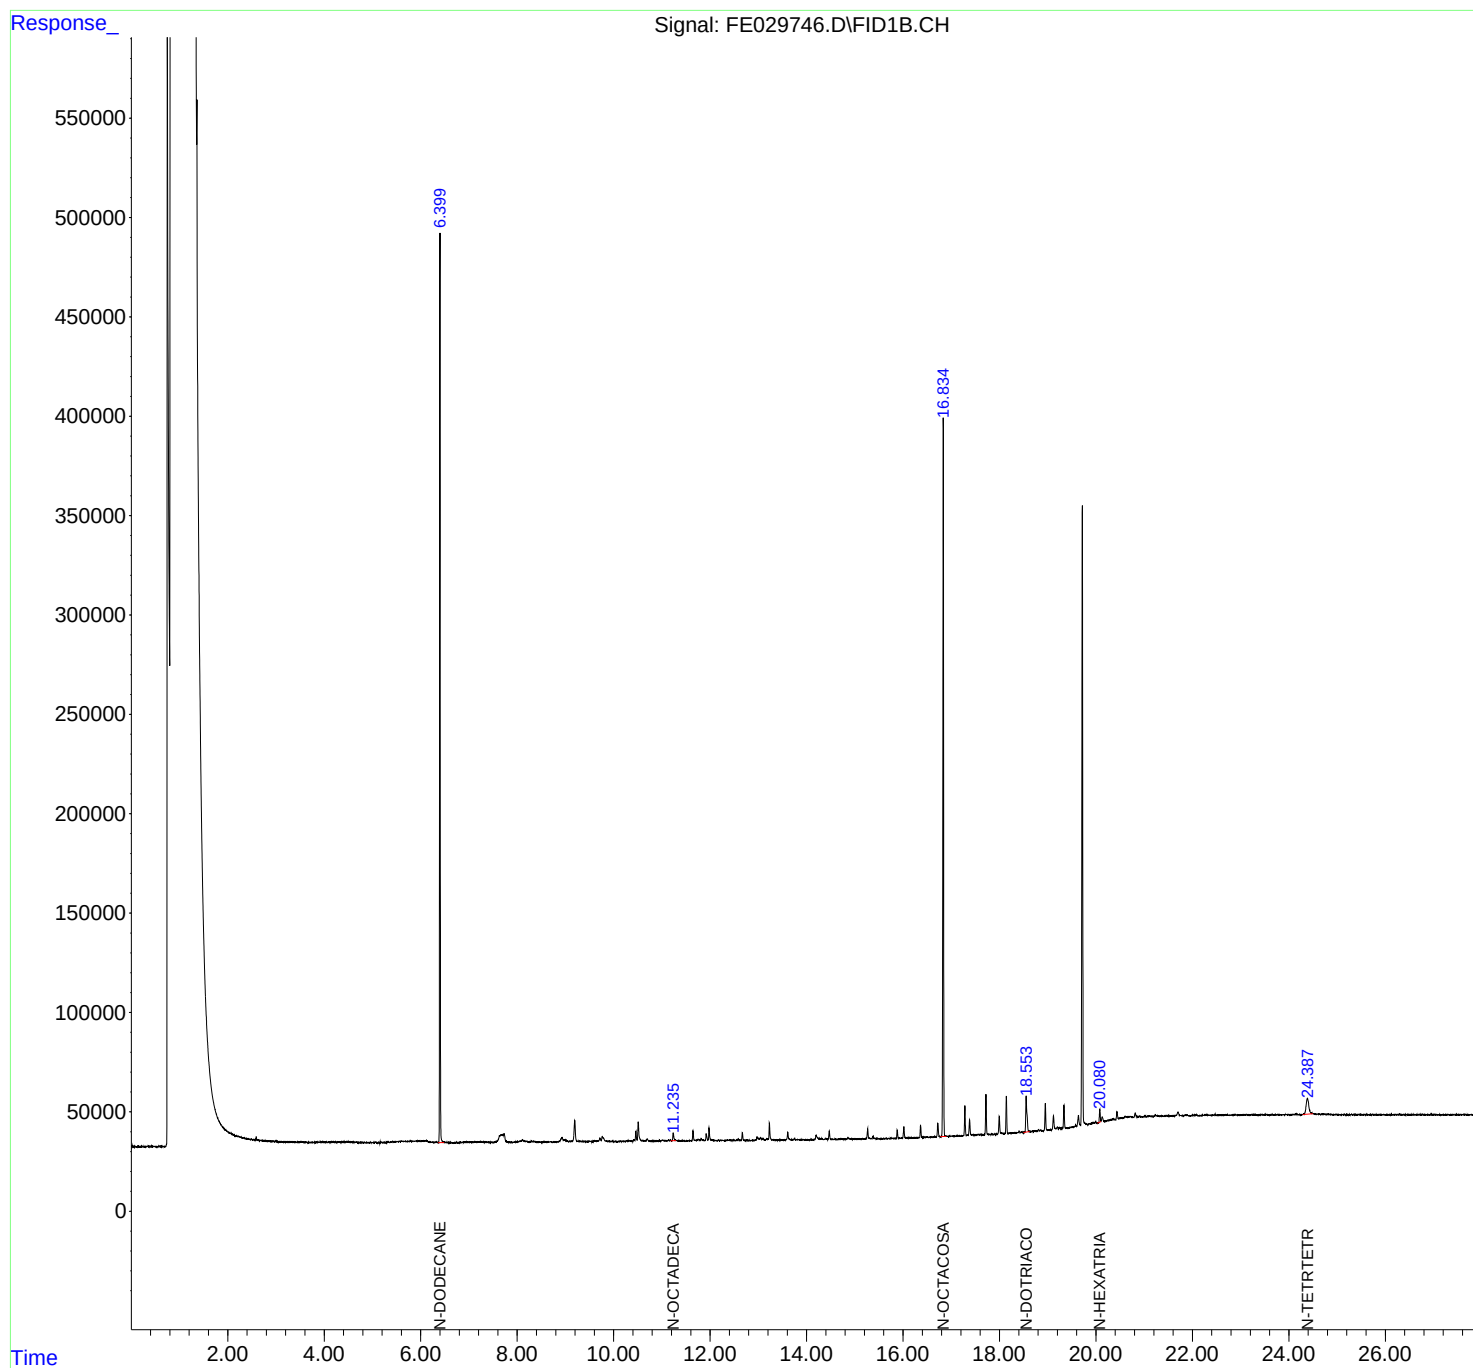


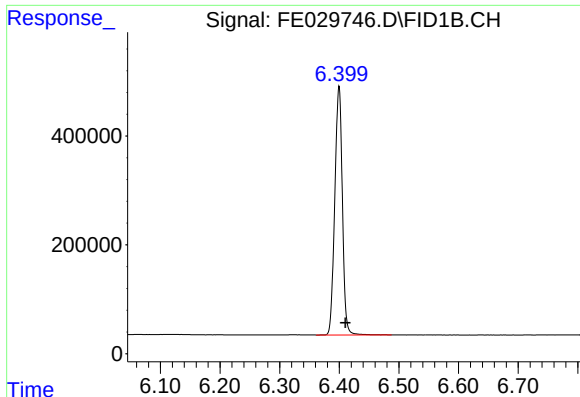

#5 N-DODECANE


R.T.: 6.400 min
Delta R.T.: -0.011 min
Response: 4050382
Conc: 25.04 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

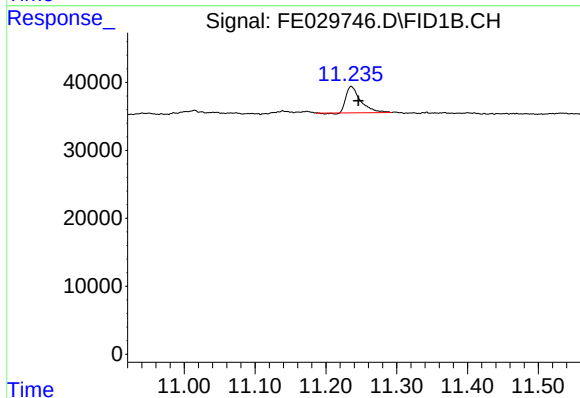


#8 N-OCTADECANE

R.T.: 11.236 min
Delta R.T.: -0.010 min
Response: 55454
Conc: 0.30 ug/ml

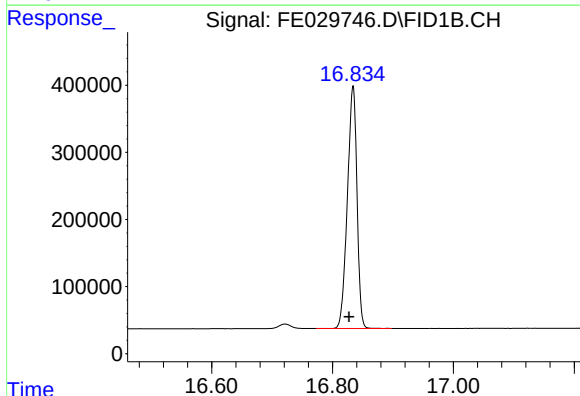


#11 N-OCTACOSANE

R.T.: 16.834 min
Delta R.T.: 0.006 min
Response: 3981365
Conc: 27.55 ug/ml

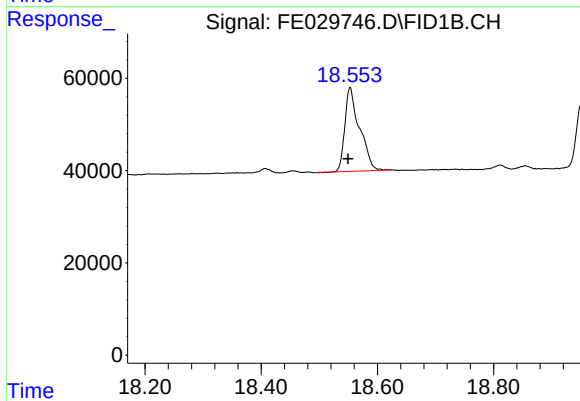

#12 N-DOTRIACONTANE


R.T.: 18.553 min
Delta R.T.: 0.004 min
Response: 319370
Conc: 1.95 ug/ml

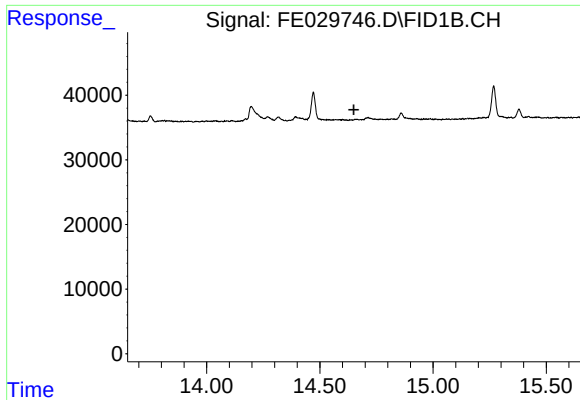

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.651 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
RT MARKER

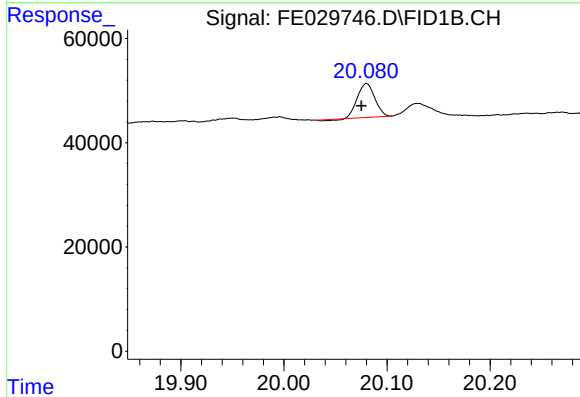

#14 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.005 min
Response: 75818
Conc: 0.52 ug/ml

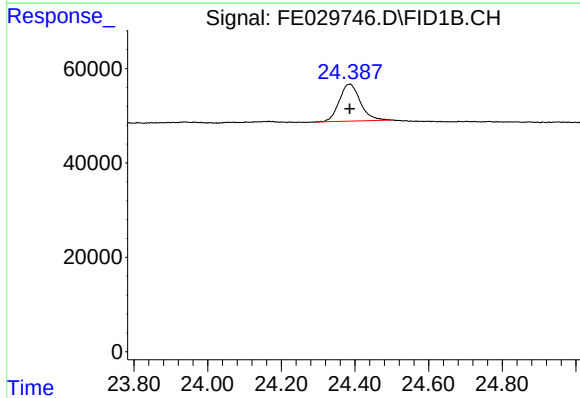

#16 N-TETRTETRACOOCTANE

R.T.: 24.387 min
Delta R.T.: 0.002 min
Response: 310329
Conc: 3.17 ug/ml