

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
 Data File : FE035476.D
 Signal(s) : FID1B.CH
 Acq On : 21 Mar 2022 15:45
 Operator : YP\AJ
 Sample : N1962-07 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 02:01:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
 Quant Title :
 QLast Update : Wed Mar 09 13:31:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	395510	4.417 ug/ml
Target Compounds			
7) N-EICOSANE	12.311f	154973	1.435 ug/ml
8) N-DOCOSANE	13.562	88763	0.849 ug/ml
10) N-TETRACOSANE	14.639	720850	7.125 ug/ml
12) N-OCTACOSANE	16.634	148983	1.588 ug/ml
14) N-DOTRIACONTANE	18.335	89281	1.016 ug/ml
15) N-TETRATRIACONTANE	19.120	20681	0.241 ug/ml
16) N-HEXATRIACONTANE	19.856	123657	1.565 ug/ml
18) N-TETRACONTANE	21.397	93196	1.355 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
Data File : FE035476.D
Signal(s) : FID1B.CH
Acq On : 21 Mar 2022 15:45
Operator : YP\AJ
Sample : N1962-07 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 02:01:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
Quant Title :
QLast Update : Wed Mar 09 13:31:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

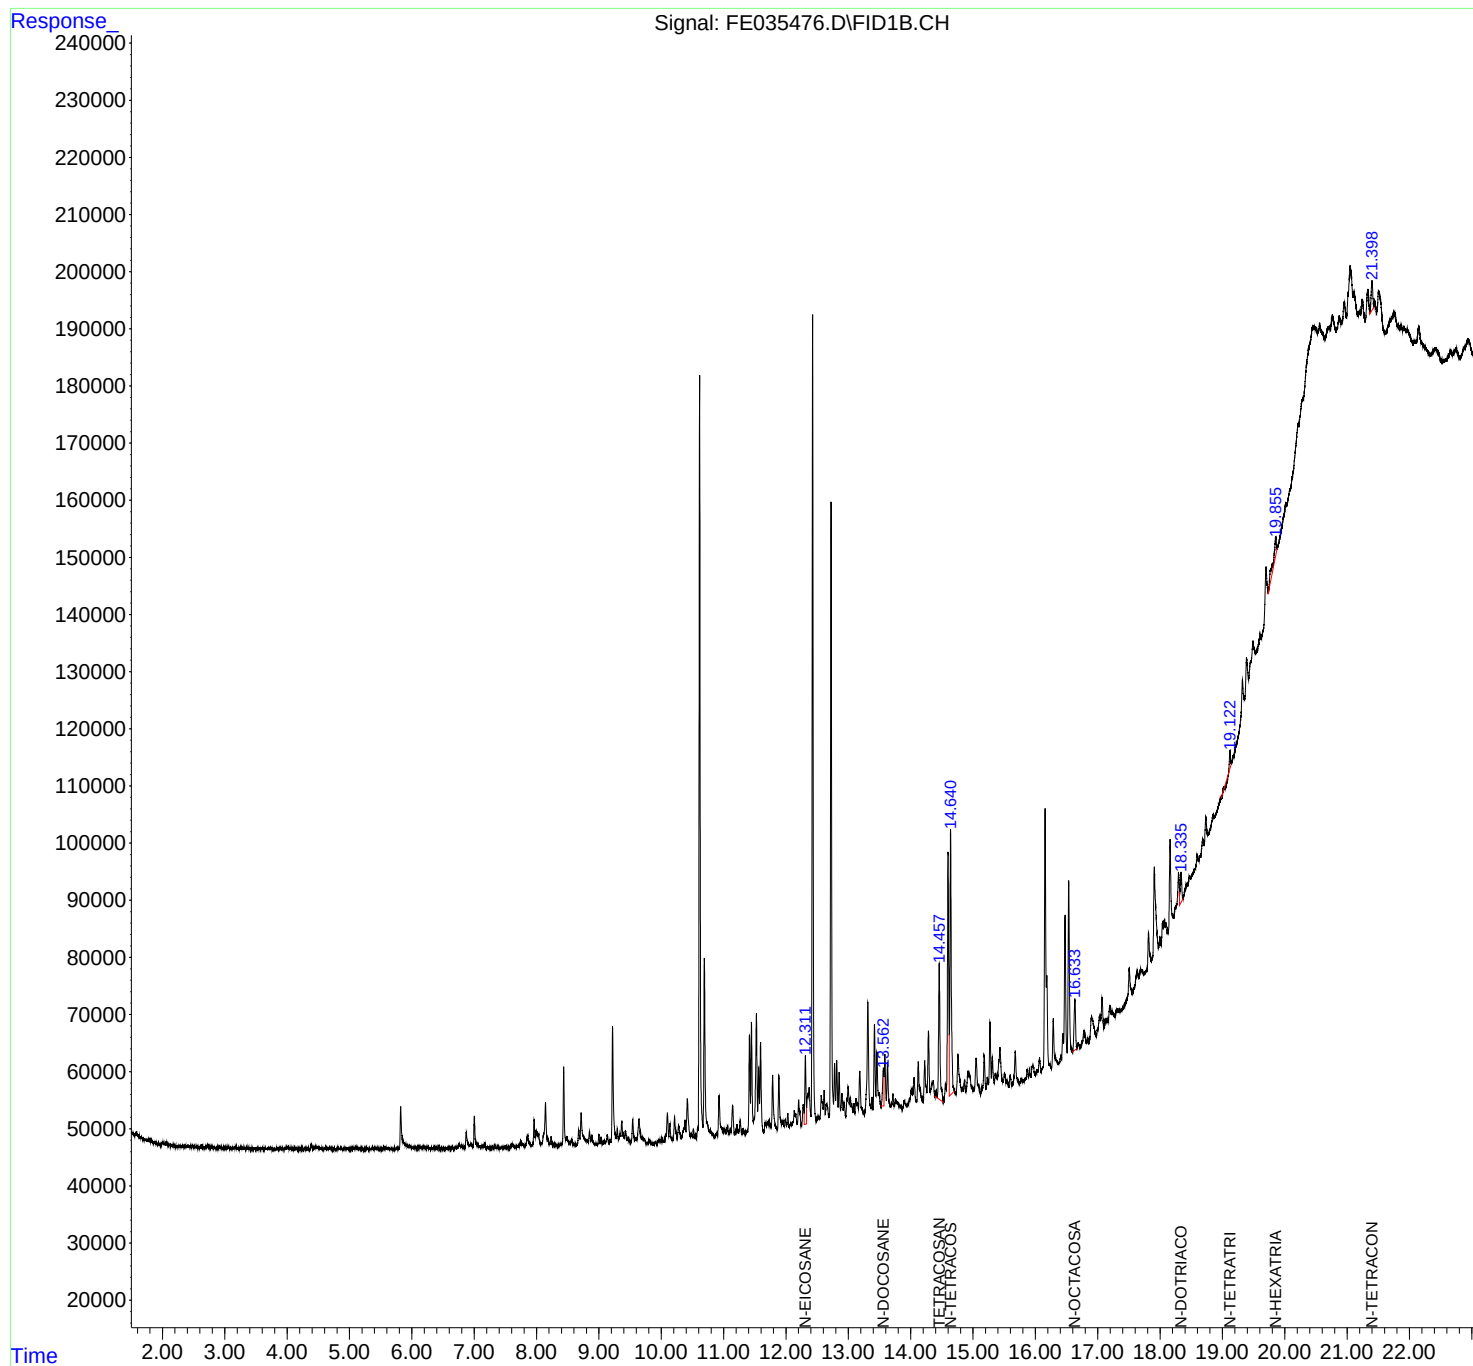


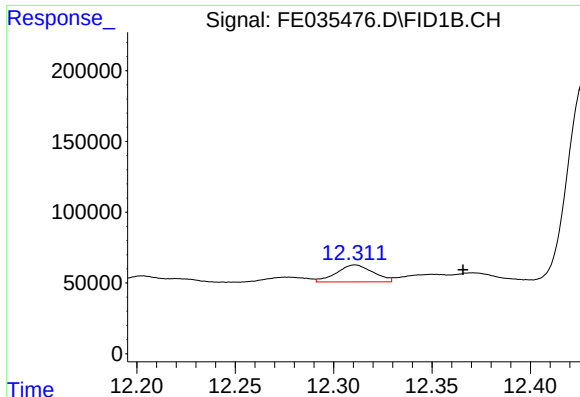

#7 N-EICOSANE


R.T.: 12.311 min
Delta R.T.: -0.055 min
Response: 154973
Conc: 1.44 ug/ml

Instrument :
FID_E
ClientSampleId :

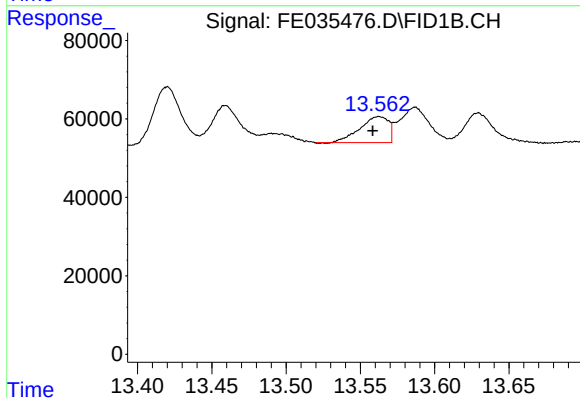


#8 N-DOCOSANE

R.T.: 13.562 min
Delta R.T.: 0.004 min
Response: 88763
Conc: 0.85 ug/ml

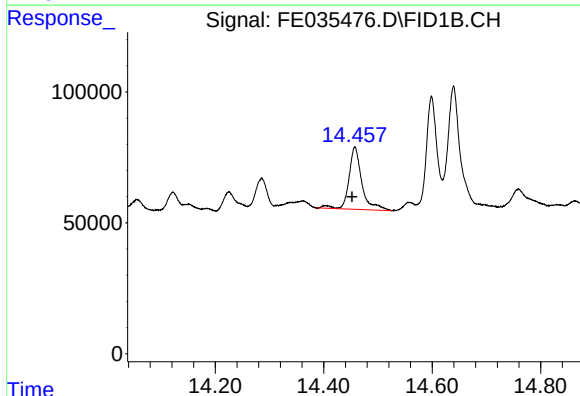


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: 0.005 min
Response: 395510
Conc: 4.42 ug/ml

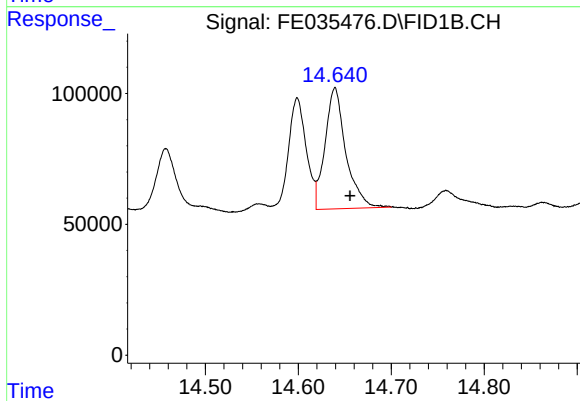

#10 N-TETRACOSANE


R.T.: 14.639 min
Delta R.T.: -0.016 min
Response: 720850
Conc: 7.12 ug/ml

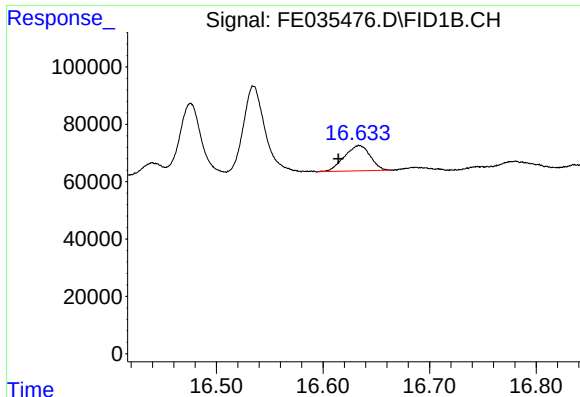

#12 N-OCTACOSANE


R.T.: 16.634 min
Delta R.T.: 0.020 min
Response: 148983
Conc: 1.59 ug/ml

Instrument :
FID_E
ClientSampleId :

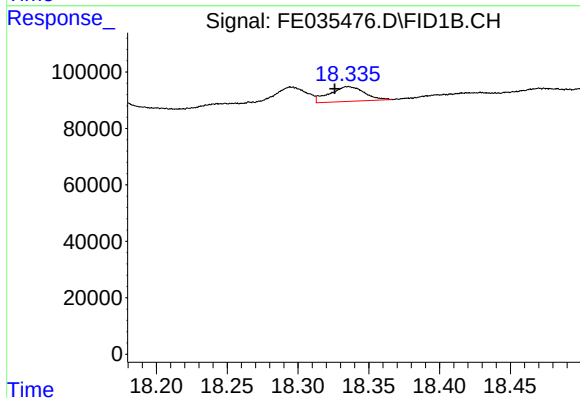


#14 N-DOTRIACONTANE

R.T.: 18.335 min
Delta R.T.: 0.009 min
Response: 89281
Conc: 1.02 ug/ml

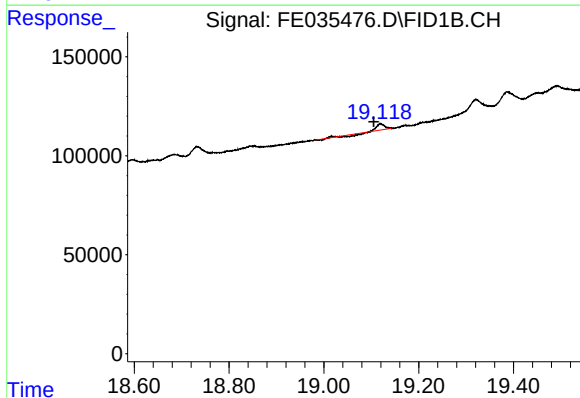


#15 N-TETRATRIACONTANE

R.T.: 19.120 min
Delta R.T.: 0.015 min
Response: 20681
Conc: 0.24 ug/ml

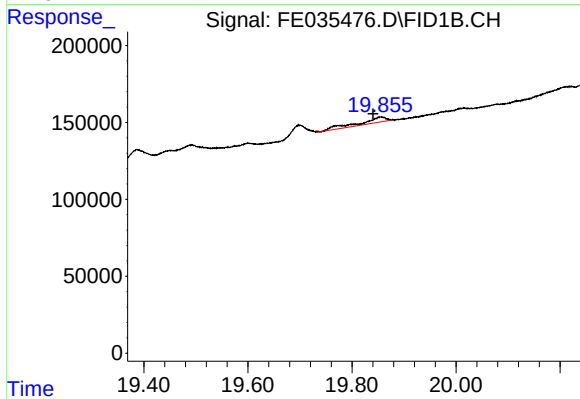

#16 N-HEXATRIACONTANE

R.T.: 19.856 min
Delta R.T.: 0.016 min
Response: 123657
Conc: 1.56 ug/ml

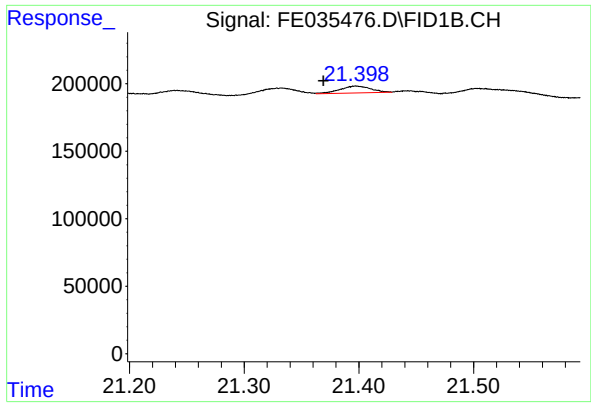

#18 N-TETRACONTANE

R.T.: 21.397 min
Delta R.T.: 0.028 min
Response: 93196
Conc: 1.36 ug/ml

Instrument :
FID_E
ClientSampleId :