

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
 Data File : FE035484.D
 Signal(s) : FID1B.CH
 Acq On : 22 Mar 2022 1:30
 Operator : YP\AJ
 Sample : N1966-09 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 02:04:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
 Quant Title :
 QLast Update : Wed Mar 09 13:31:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.453	388555	4.339 ug/ml
Target Compounds			
7) N-EICOSANE	12.423f	402242	3.726 ug/ml
10) N-TETRACOSANE	14.637	165927	1.640 ug/ml
15) N-TETRATRIACONTANE	19.111	304143	3.549 ug/ml
16) N-HEXATRIACONTANE	19.846	49324	0.624 ug/ml
17) N-OCTATRIACONTANE	20.522	27995	0.394 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
Data File : FE035484.D
Signal(s) : FID1B.CH
Acq On : 22 Mar 2022 1:30
Operator : YP\AJ
Sample : N1966-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 02:04:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
Quant Title :
QLast Update : Wed Mar 09 13:31:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

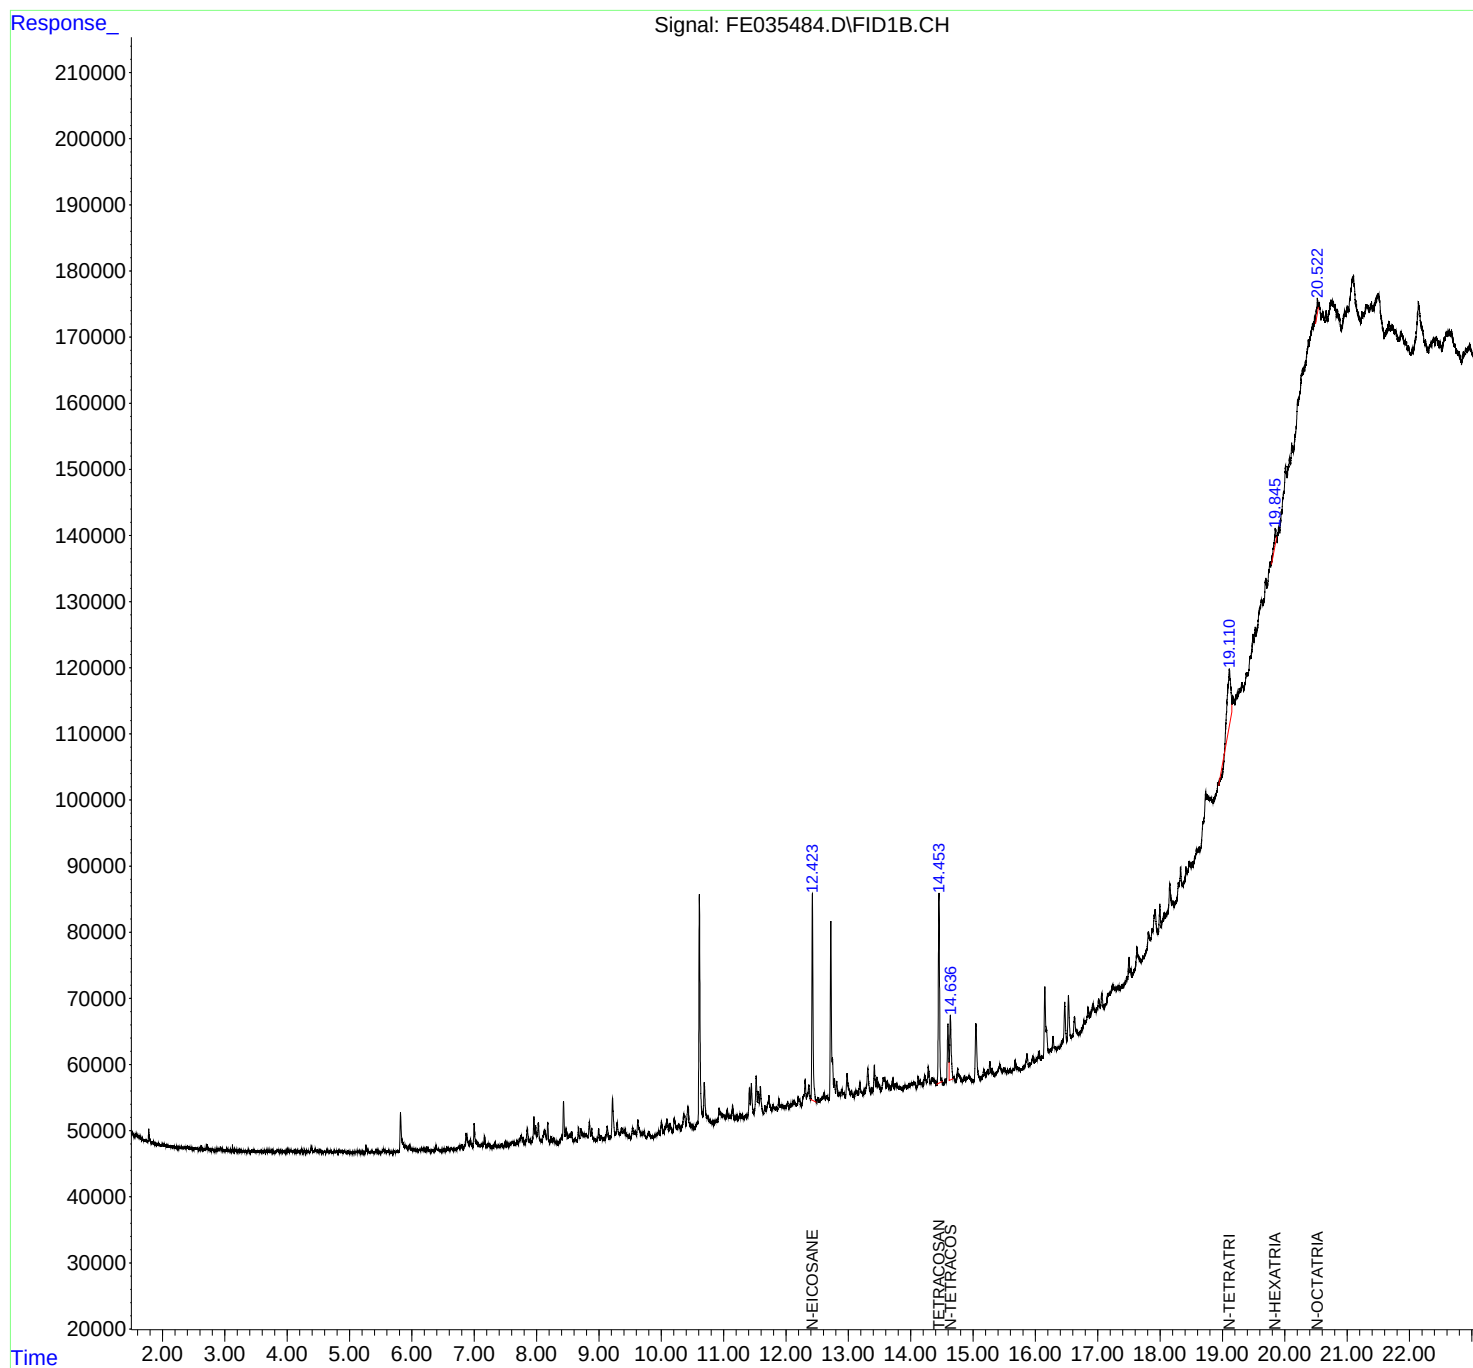


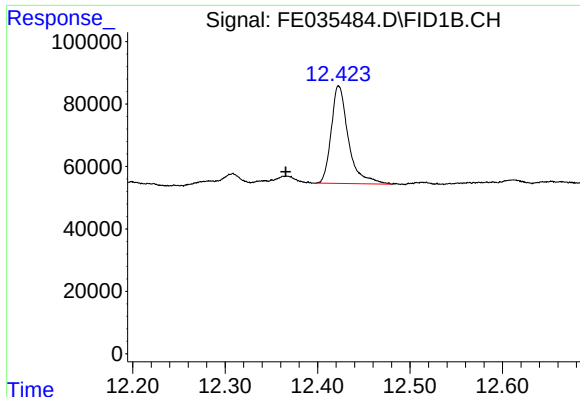

#7 N-EICOSANE


R.T.: 12.423 min
Delta R.T.: 0.057 min
Response: 402242
Conc: 3.73 ug/ml

Instrument :
FID_E
ClientSampleId :

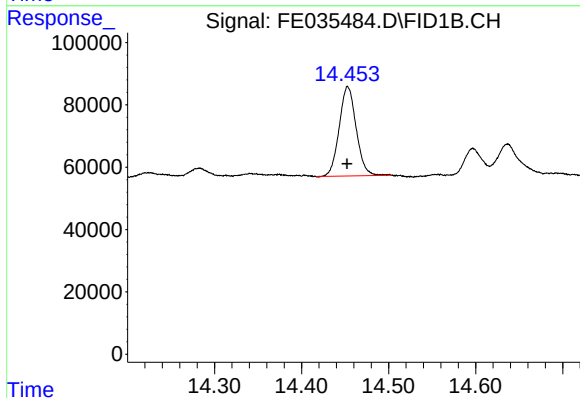


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.453 min
Delta R.T.: 0.000 min
Response: 388555
Conc: 4.34 ug/ml

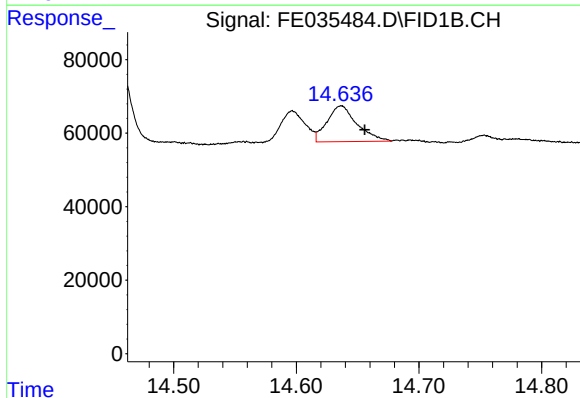


#10 N-TETRACOSANE

R.T.: 14.637 min
Delta R.T.: -0.019 min
Response: 165927
Conc: 1.64 ug/ml

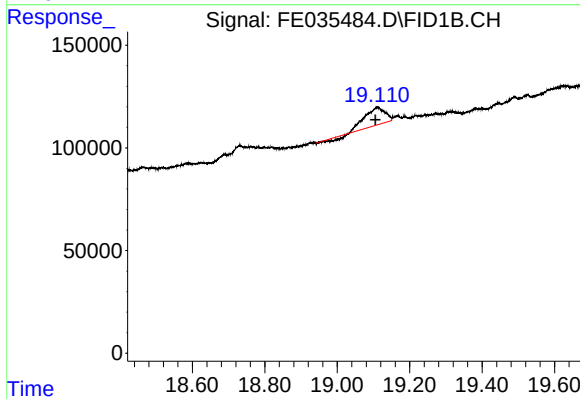

#15 N-TETRATRIACONTANE


R.T.: 19.111 min
Delta R.T.: 0.006 min
Response: 304143
Conc: 3.55 ug/ml

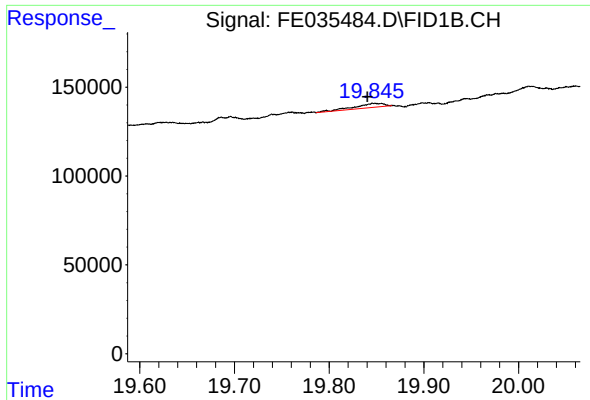

#16 N-HEXATRIACONTANE

R.T.: 19.846 min
Delta R.T.: 0.006 min
Response: 49324
Conc: 0.62 ug/ml

Instrument :
FID_E
ClientSampleId :

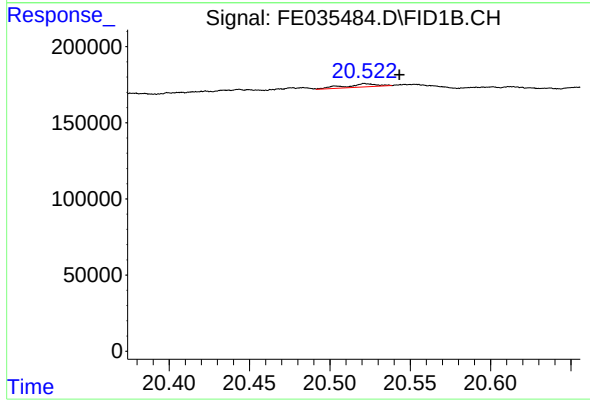

#17 N-OCTATRIACONTANE

R.T.: 20.522 min
Delta R.T.: -0.022 min
Response: 27995
Conc: 0.39 ug/ml