

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
Data File : FE035485.D
Signal(s) : FID1B.CH
Acq On : 22 Mar 2022 2:02
Operator : YP\AJ
Sample : N1966-10 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
G-1-10-18-19

Integration File: Sample.e
Quant Time: Mar 22 03:21:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
Quant Title :
QLast Update : Wed Mar 09 13:31:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.453	932263	10.412 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032122\
Data File : FE035485.D
Signal(s) : FID1B.CH
Acq On : 22 Mar 2022 2:02
Operator : YP\AJ
Sample : N1966-10 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
G-1-10-18-19

Integration File: Sample.e
Quant Time: Mar 22 03:21:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE030922.M
Quant Title :
QLast Update : Wed Mar 09 13:31:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

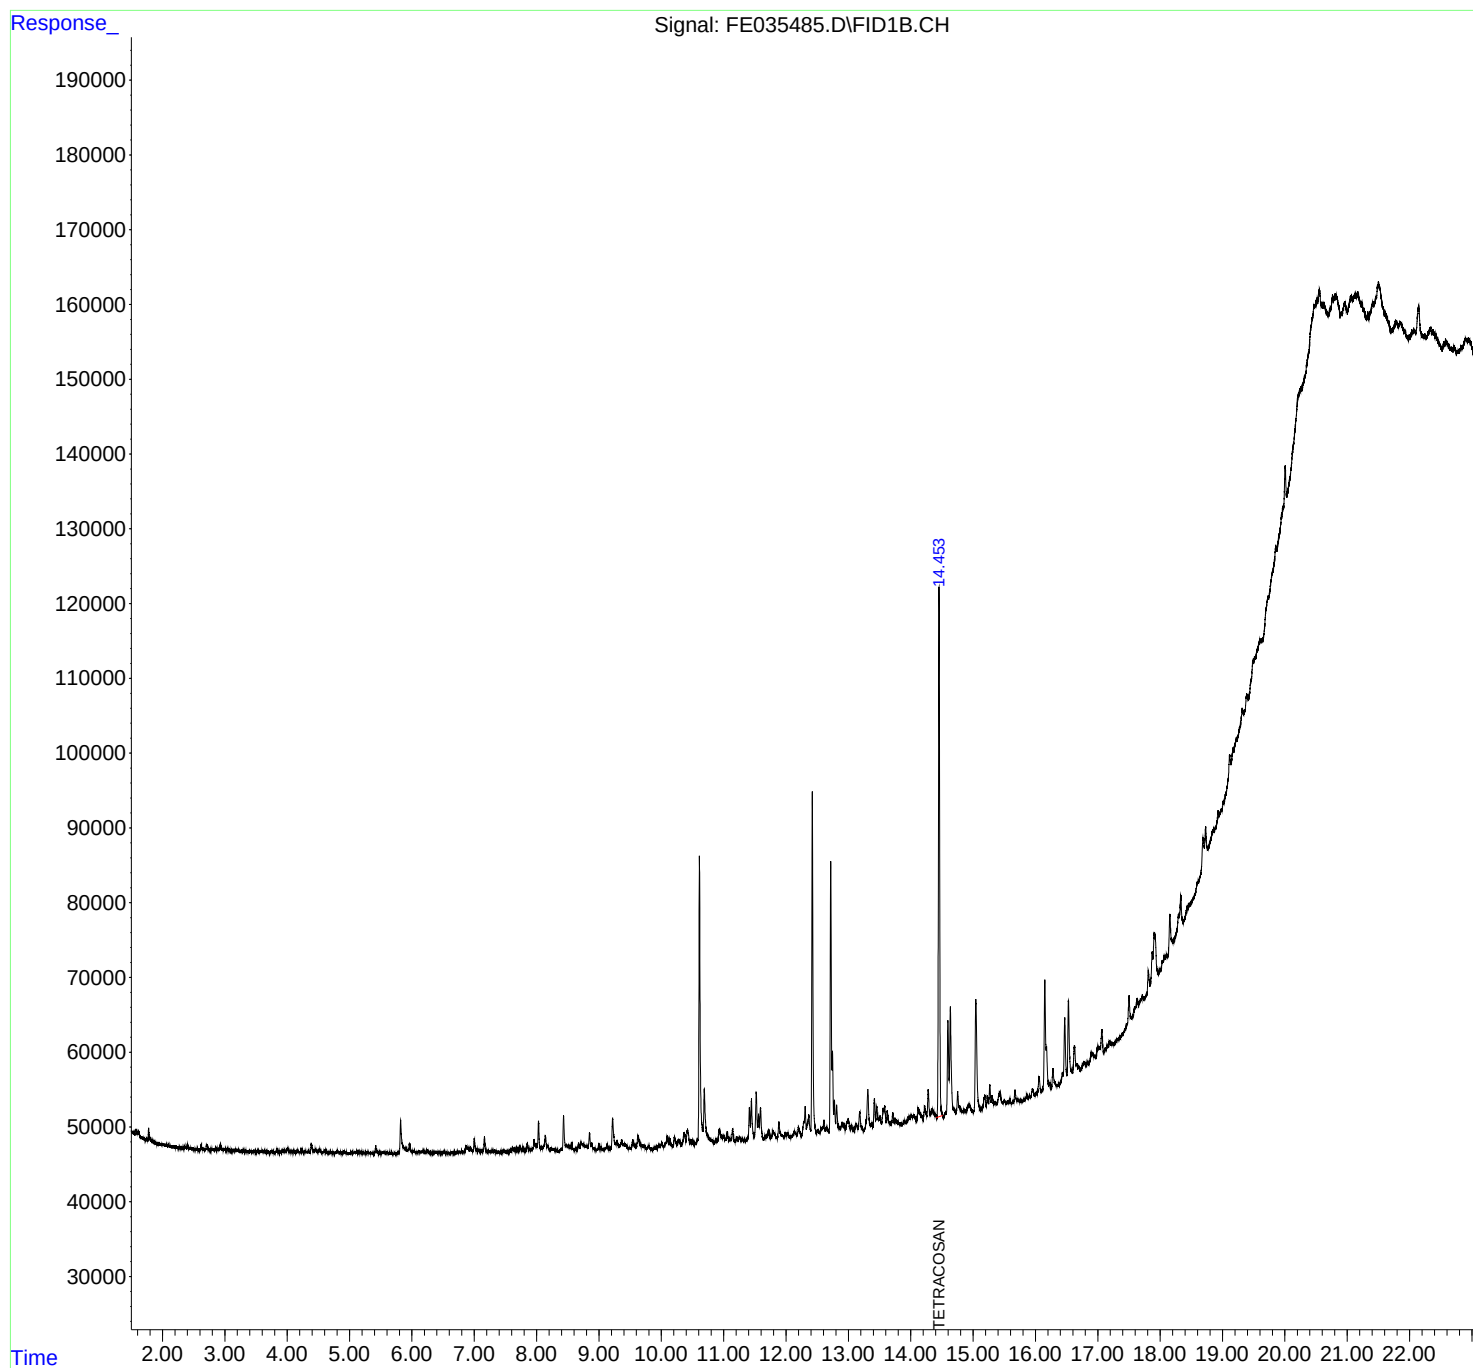

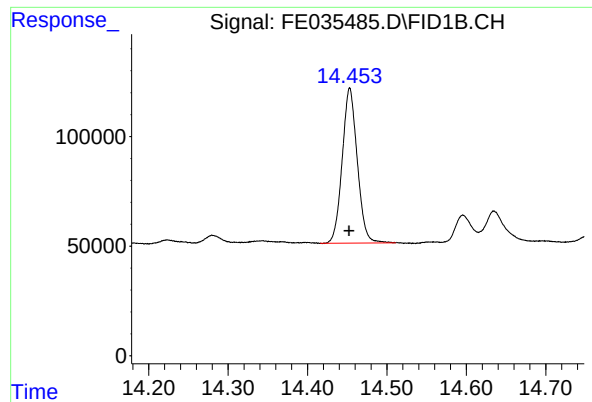

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.453 min
Delta R.T.: 0.000 min
Response: 932263
Conc: 10.41 ug/ml

Instrument :
FID_E
ClientSampleId :
G-1-10-18-19