

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032323AL\
 Data File : FE040971.D
 Signal(s) : FID1B.ch
 Acq On : 23 Mar 2023 13:44
 Operator : YP\AJ
 Sample : PB151633BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 24 02:54:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.867	9123227	48.836 ug/ml
Spiked Amount 50.000		Recovery =	97.67%
12) S 1-chlorooctadecane (S...	13.306	7301371	49.332 ug/ml
Spiked Amount 50.000		Recovery =	98.66%
Target Compounds			
14) T n-Tetracosane (C24)	15.139	71619	0.415 ug/ml
18) T n-Dotriacontane (C32)	18.874	63762	0.373 ug/ml
20) T n-Hexatriacontane (C36)	20.431	39137	0.269 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032323AL\
Data File : FE040971.D
Signal(s) : FID1B.ch
Acq On : 23 Mar 2023 13:44
Operator : YP\AJ
Sample : PB151633BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 24 02:54:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

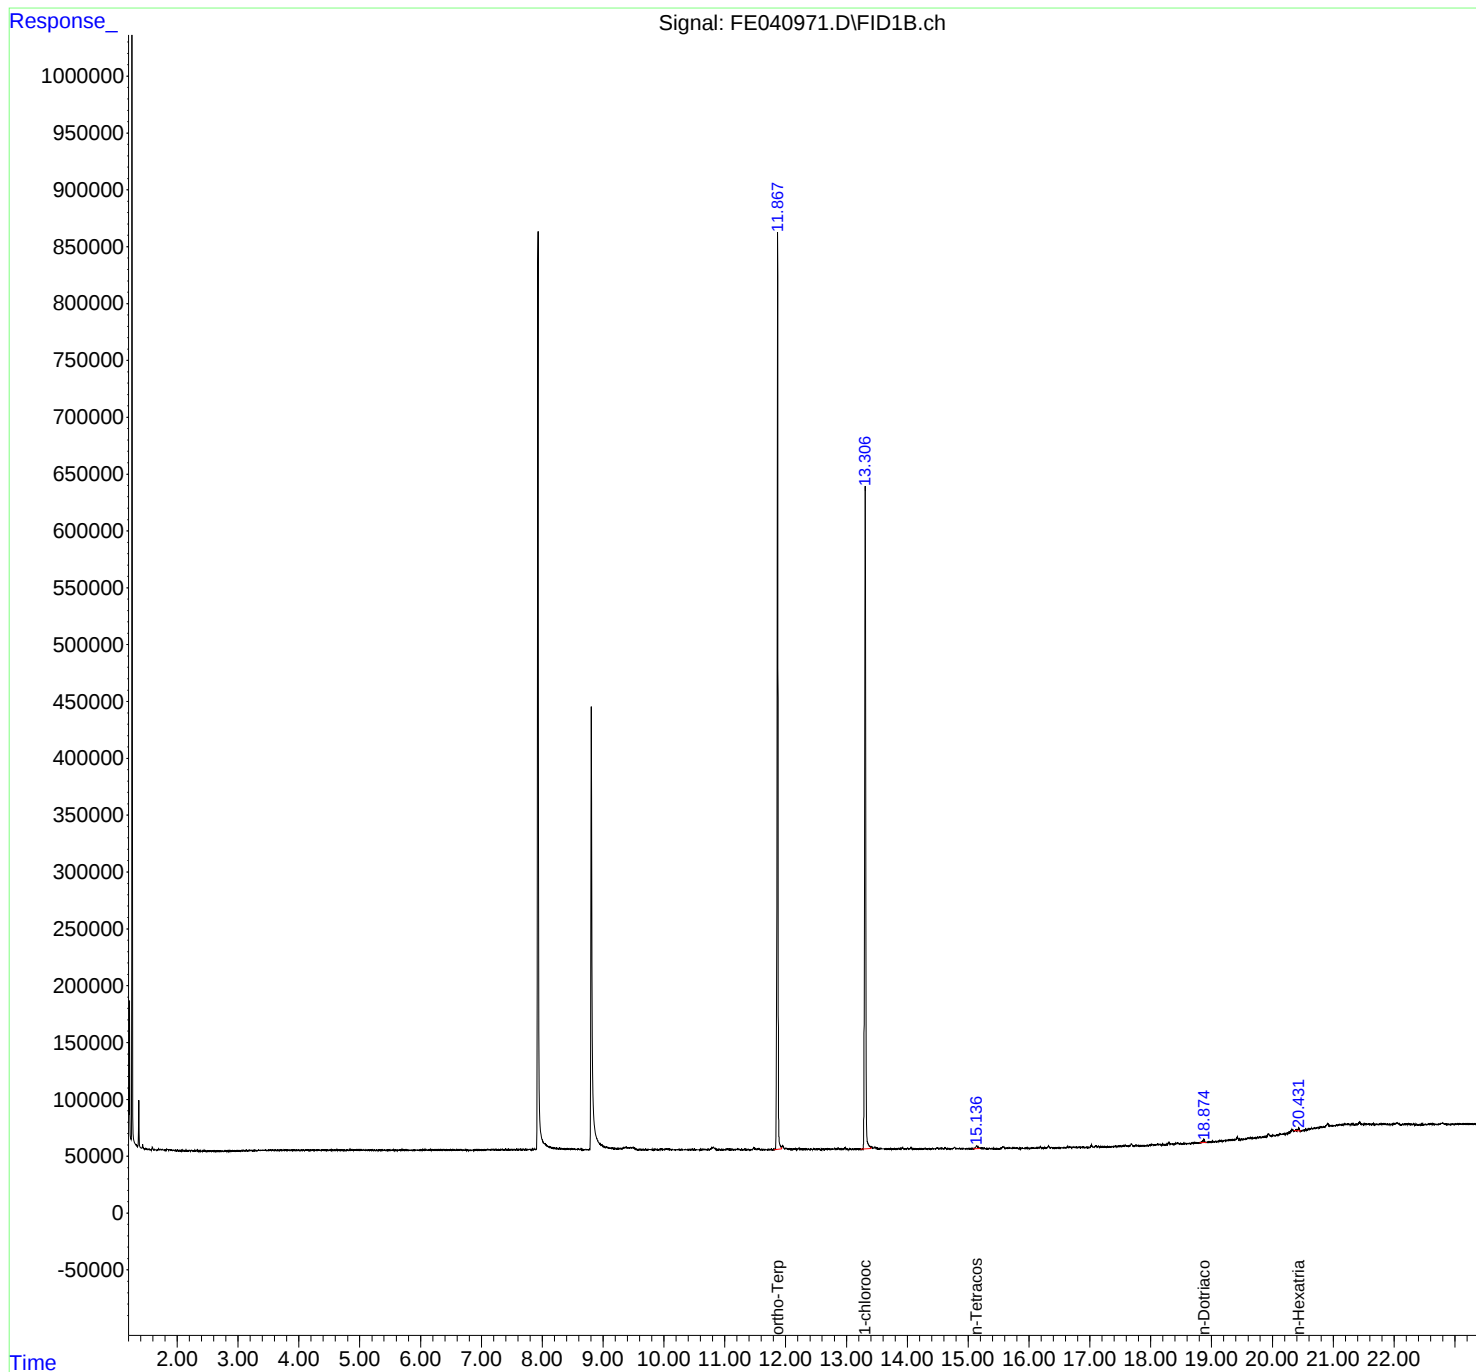


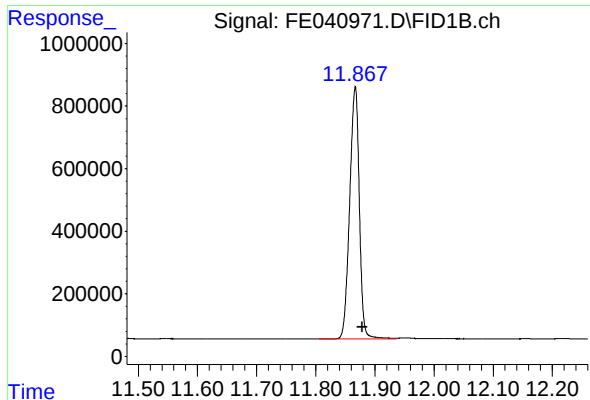

#9 ortho-Terphenyl (SURRE)


R.T.: 11.867 min
Delta R.T.: -0.012 min
Response: 9123227
Conc: 48.84 ug/ml

Instrument :
FID_E
ClientSampleId :

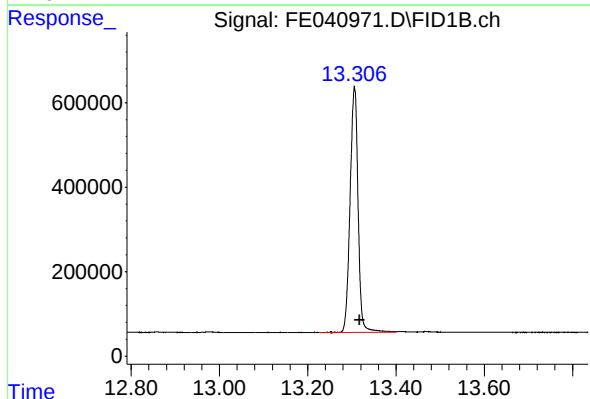


#12 1-chlorooctadecane (SURRE)

R.T.: 13.306 min
Delta R.T.: -0.012 min
Response: 7301371
Conc: 49.33 ug/ml

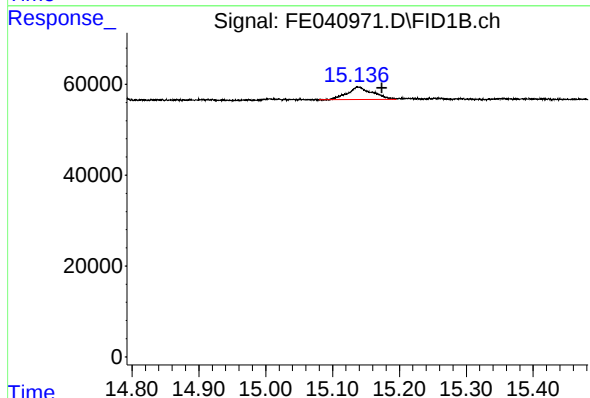


#14 n-Tetracosane (C24)

R.T.: 15.139 min
Delta R.T.: -0.036 min
Response: 71619
Conc: 0.42 ug/ml

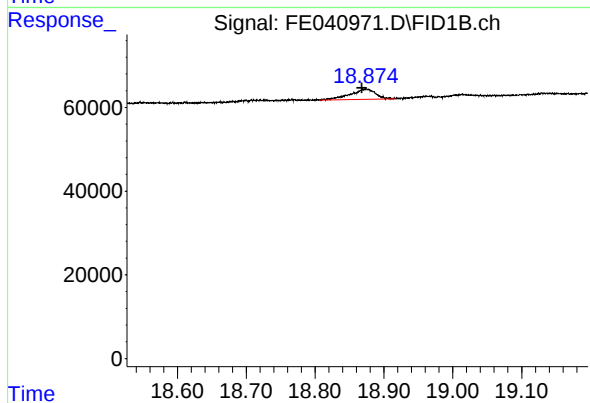

#18 n-Dotriacontane (C32)

R.T.: 18.874 min
Delta R.T.: 0.005 min
Response: 63762
Conc: 0.37 ug/ml

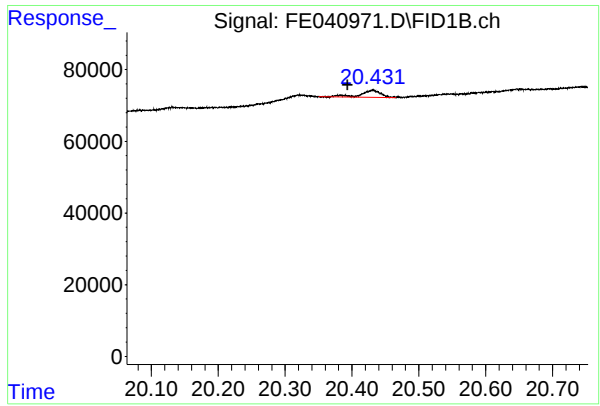

#20 n-Hexatriacontane (C36)

R.T.: 20.431 min
Delta R.T.: 0.038 min
Response: 39137
Conc: 0.27 ug/ml

Instrument :

FID_E

ClientSampleId :