

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032323AL\
 Data File : FE040983.D
 Signal(s) : FID1B.ch
 Acq On : 23 Mar 2023 20:35
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 24 02:55:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
20) T n-Hexatriacontane (C36)	20.393	80096	0.551 ug/ml
21) T n-Octatriacontane (C38)	21.147	119231	0.867 ug/ml
22) T n-Tetracontane (C40)	22.012	599135	3.877 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032323AL\
Data File : FE040983.D
Signal(s) : FID1B.ch
Acq On : 23 Mar 2023 20:35
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 24 02:55:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

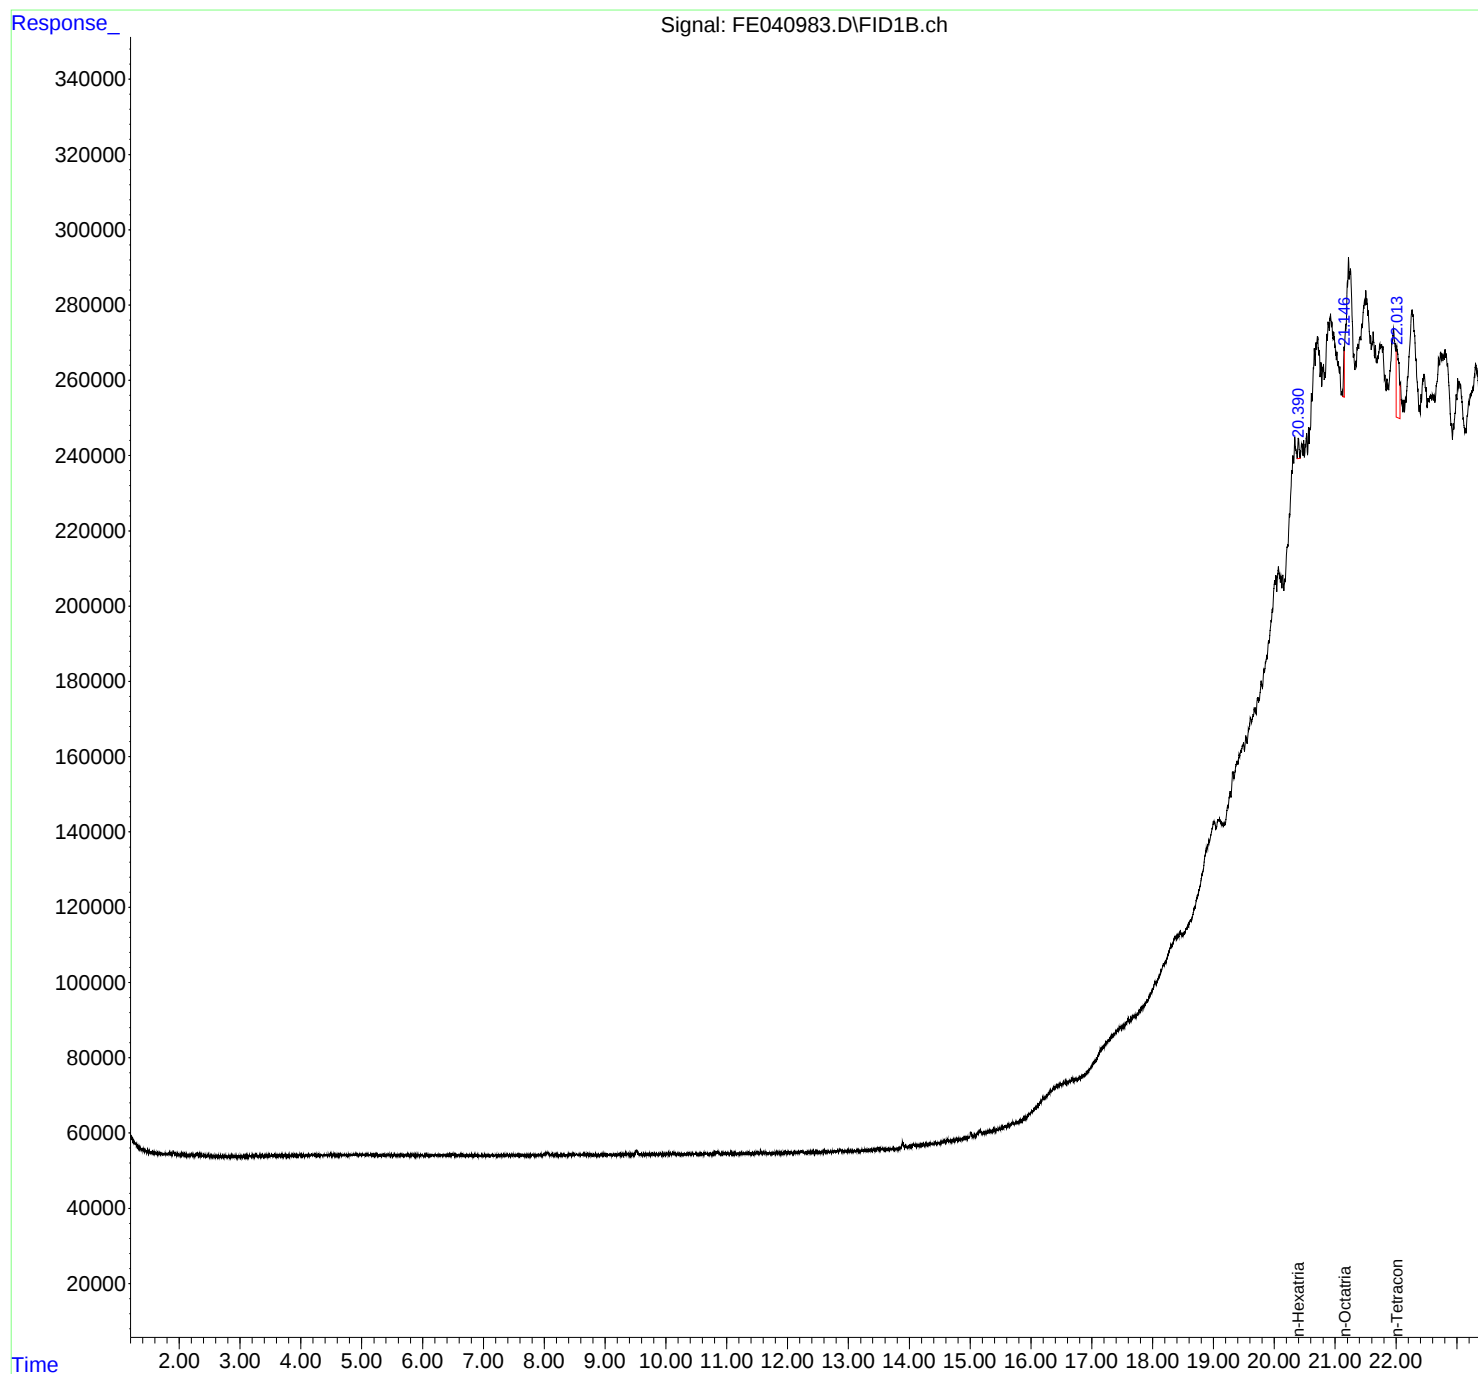


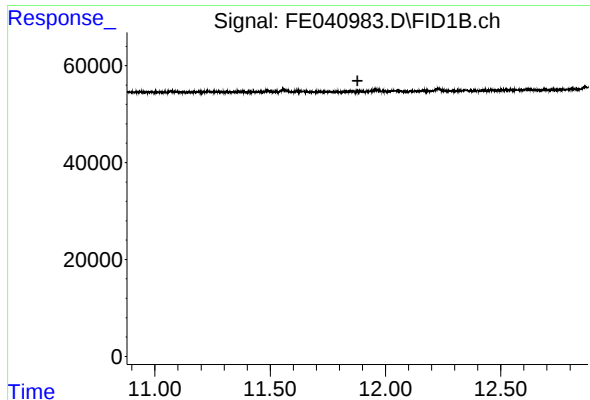

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.879 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

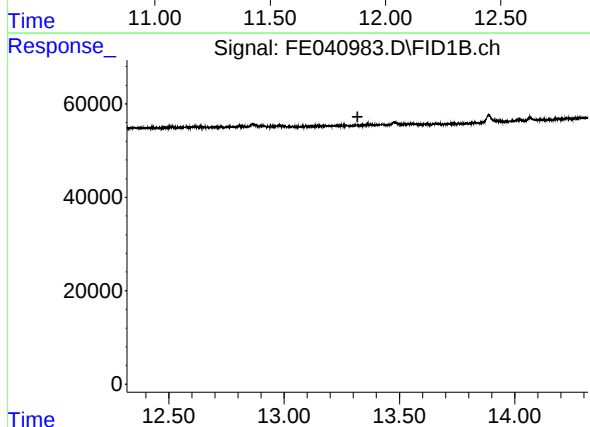


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.318 min
Response: 0
Conc: N.D.

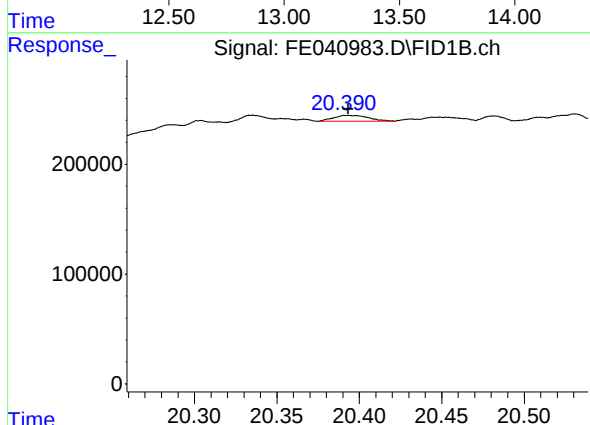


#20 n-Hexatriacontane (C36)

R.T.: 20.393 min
Delta R.T.: 0.000 min
Response: 80096
Conc: 0.55 ug/ml

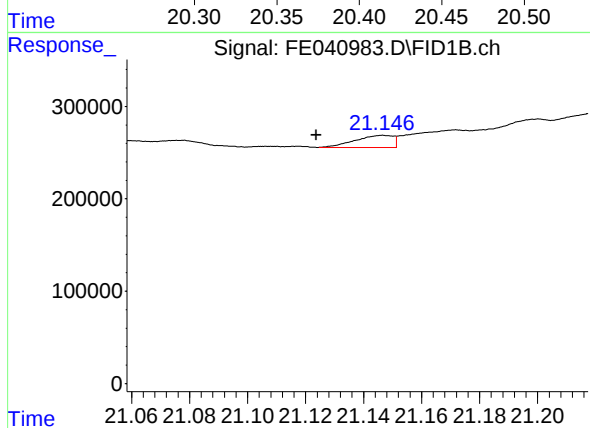

#21 n-Octatriacontane (C38)

R.T.: 21.147 min
Delta R.T.: 0.023 min
Response: 119231
Conc: 0.87 ug/ml

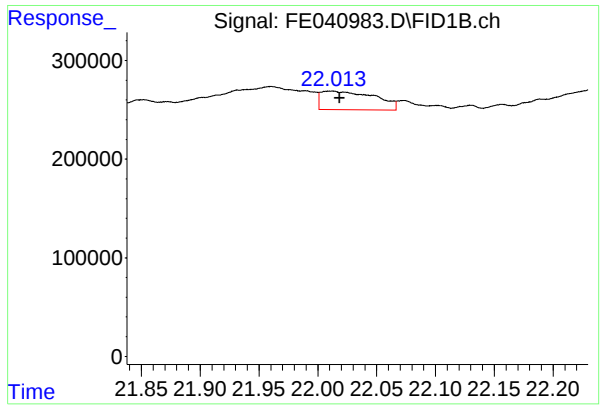

#22 n-Tetracontane (C40)

R.T.: 22.012 min
Delta R.T.: -0.006 min
Response: 599135
Conc: 3.88 ug/ml

Instrument :
FID_E
ClientSampleId :