

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032421\
 Data File : FE033436.D
 Signal(s) : FID1B.CH
 Acq On : 24 Mar 2021 9:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 25 01:09:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031621.M
 Quant Title :
 QLast Update : Wed Mar 17 09:27:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	7644823	19.892 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.791	186624	0.433 ug/ml
14) N-DOTRIACONTANE	18.623	205934	0.487 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032421\
Data File : FE033436.D
Signal(s) : FID1B.CH
Acq On : 24 Mar 2021 9:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 25 01:09:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031621.M
Quant Title :
QLast Update : Wed Mar 17 09:27:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

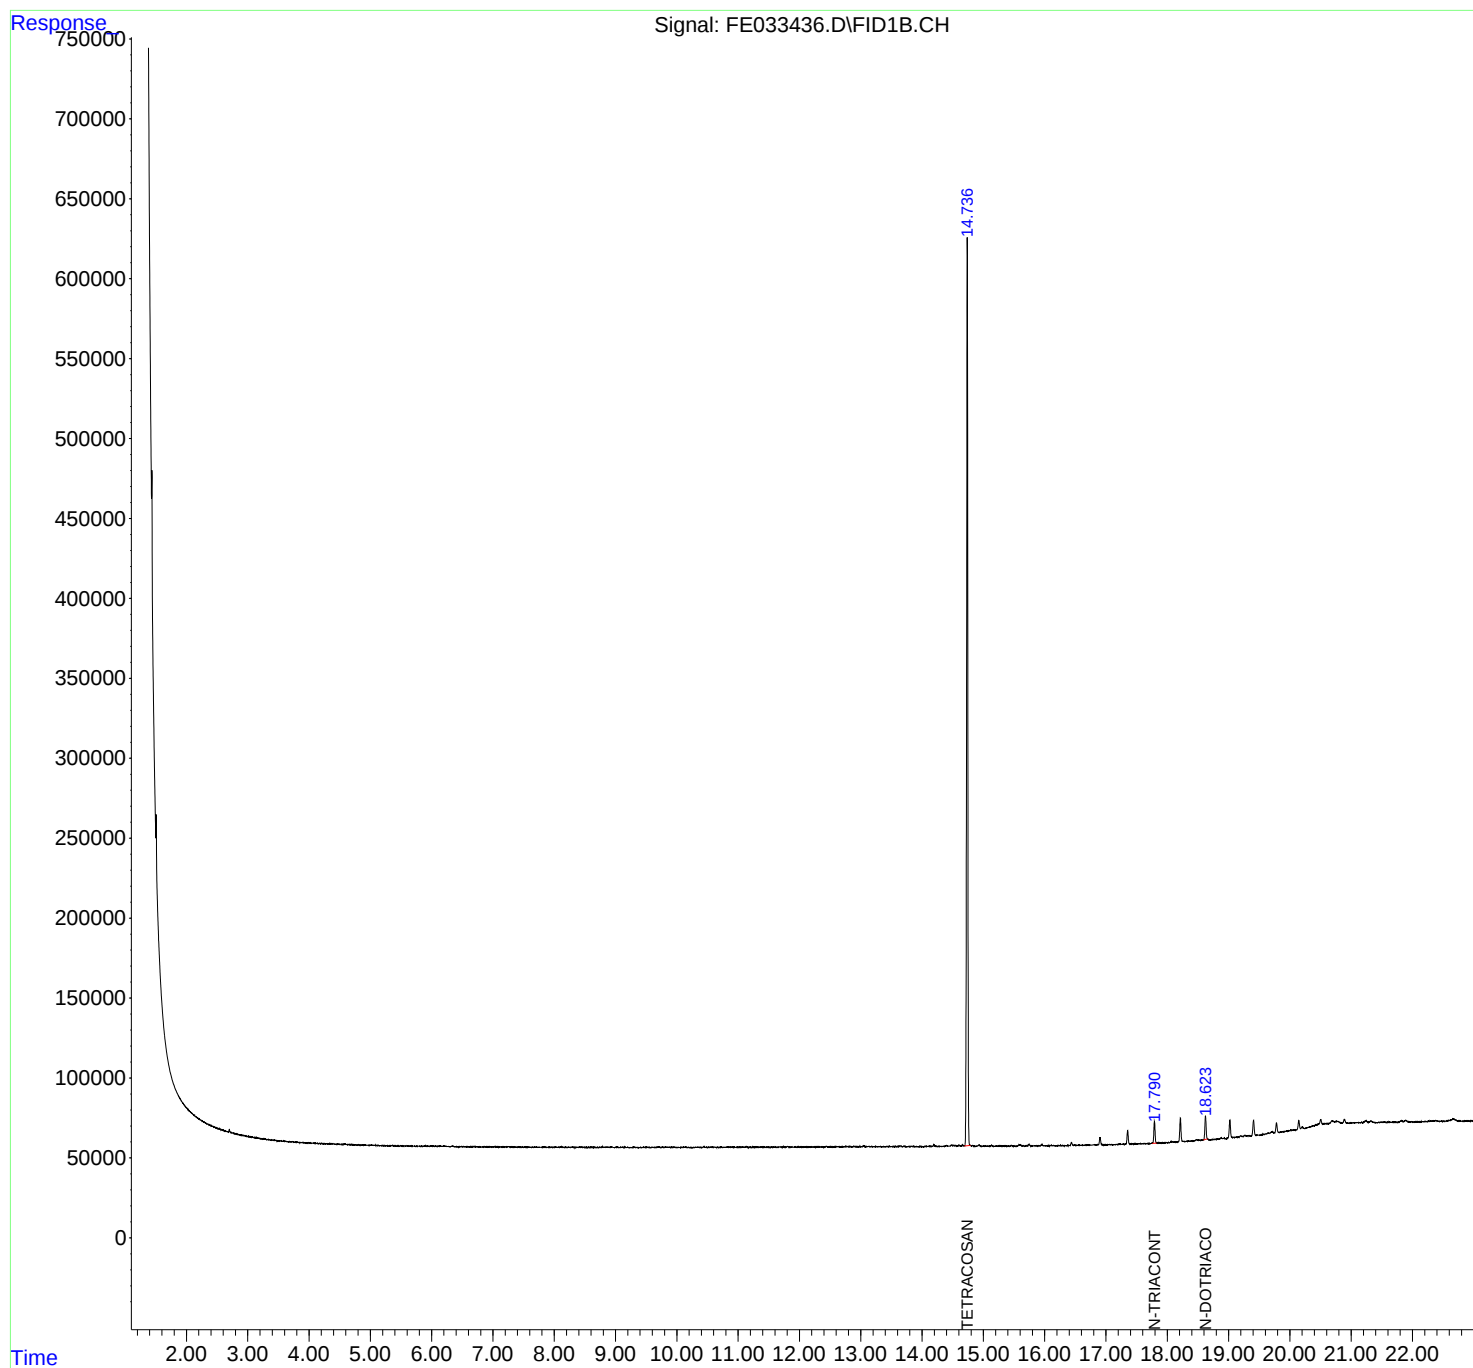


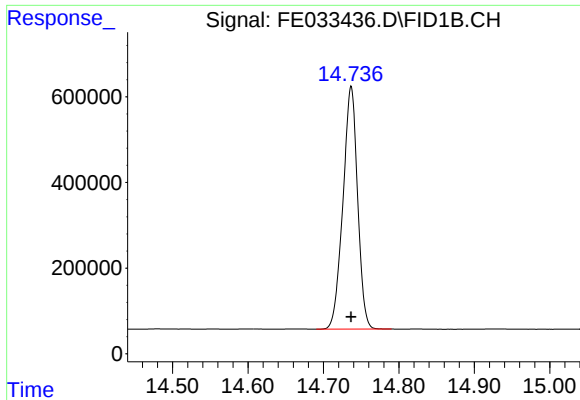

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.737 min
Delta R.T.: 0.000 min
Response: 7644823
Conc: 19.89 ug/ml

Instrument :
FID_E
ClientSampleId :

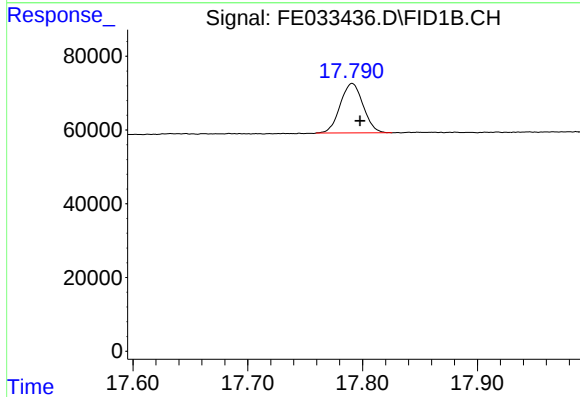

#13 N-TRIACONTANE

R.T.: 17.791 min
Delta R.T.: -0.007 min
Response: 186624
Conc: 0.43 ug/ml

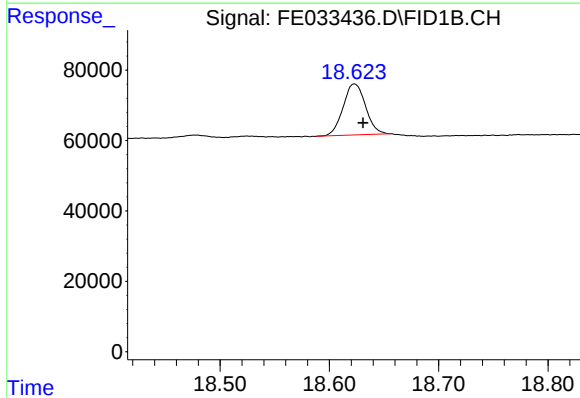

#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: -0.008 min
Response: 205934
Conc: 0.49 ug/ml