

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032523AL\
 Data File : FE041023.D
 Signal(s) : FID1B.ch
 Acq On : 25 Mar 2023 04:49
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 25 06:33:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.860	38301	0.245 ug/ml
19) T n-Tetratriacontane (C34)	19.643	20737	0.134 ug/ml
20) T n-Hexatriacontane (C36)	20.384	18267	0.120 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032523AL\
Data File : FE041023.D
Signal(s) : FID1B.ch
Acq On : 25 Mar 2023 04:49
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 25 06:33:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

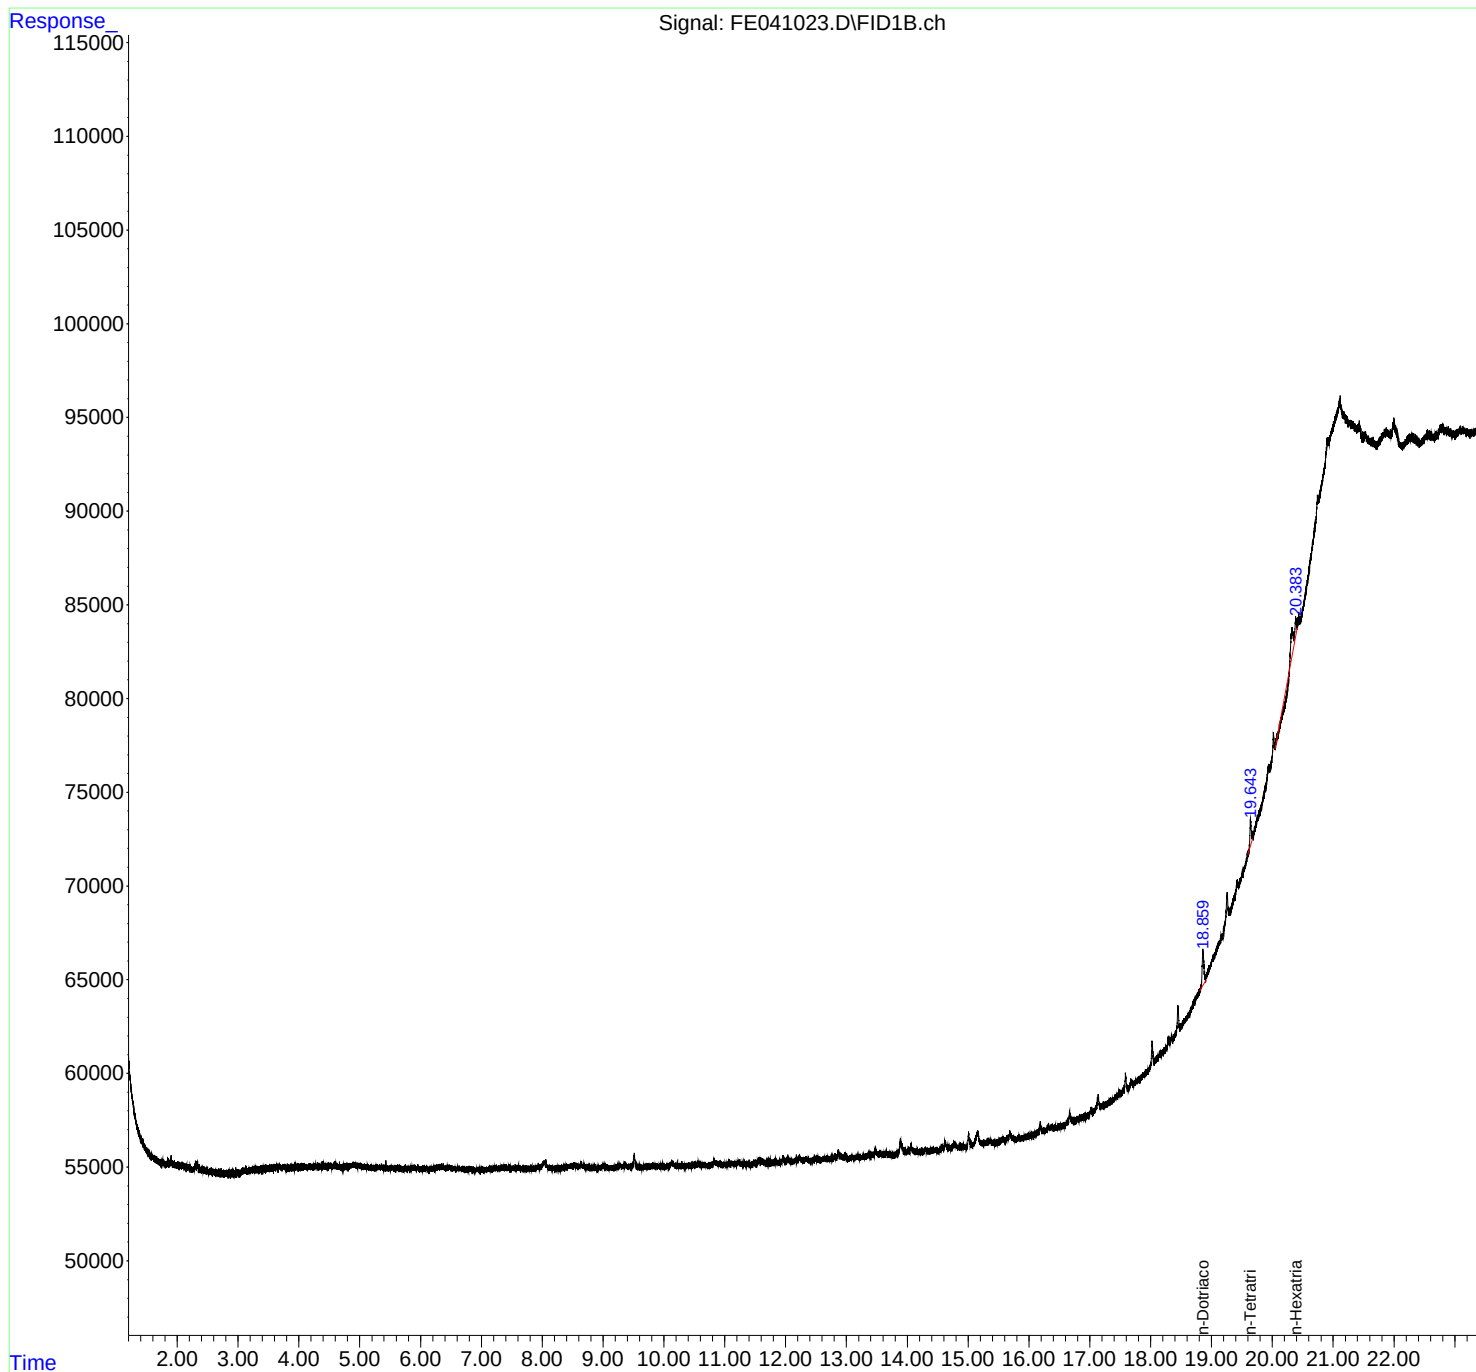


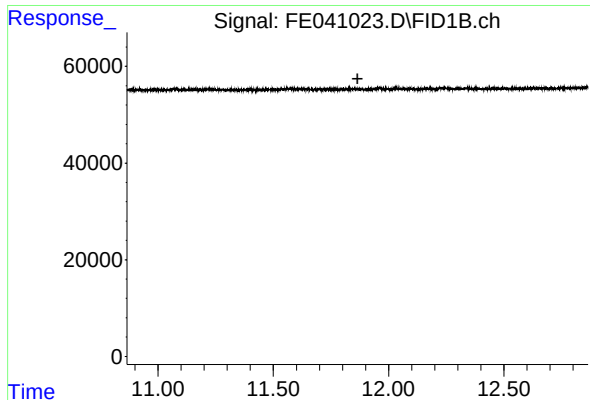

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

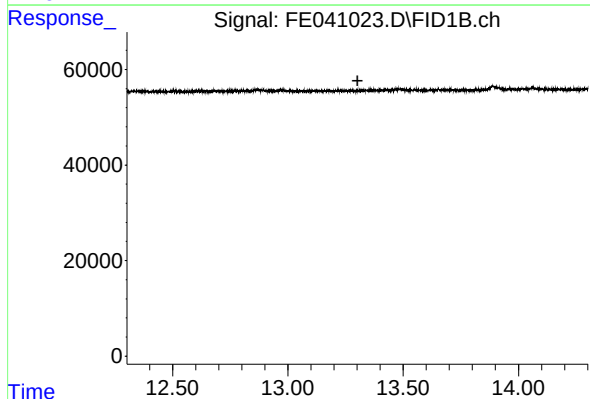


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

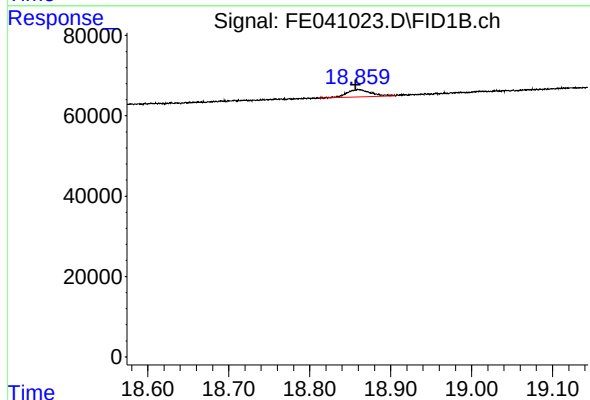


#18 n-Dotriacontane (C32)

R.T.: 18.860 min
Delta R.T.: 0.004 min
Response: 38301
Conc: 0.25 ug/ml

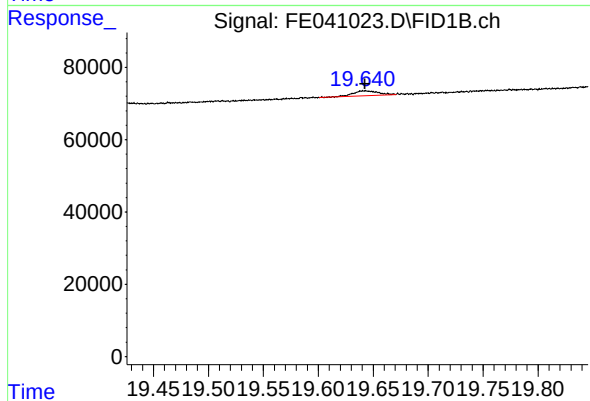

#19 n-Tetratriacontane (C34)

R.T.: 19.643 min
Delta R.T.: 0.000 min
Response: 20737
Conc: 0.13 ug/ml

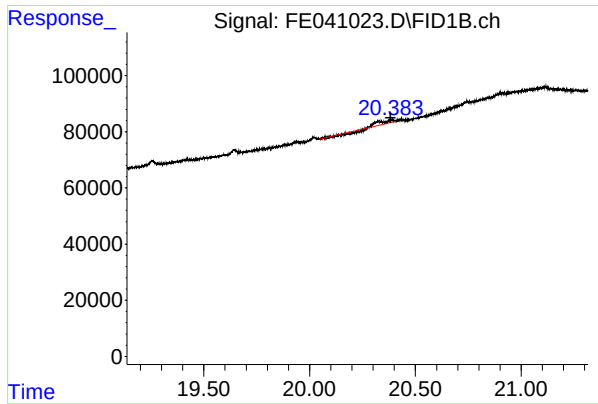

#20 n-Hexatriacontane (C36)

R.T.: 20.384 min
Delta R.T.: 0.000 min
Response: 18267
Conc: 0.12 ug/ml

Instrument :
FID_E
ClientSampleId :