

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032619\
 Data File : FE029767.D
 Signal(s) : FID1B.CH
 Acq On : 26 Mar 2019 11:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 26 14:55:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
 Quant Title :
 QLast Update : Wed Mar 20 08:08:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.648	3516994	21.205 ug/ml
Target Compounds				
11)	N-OCTACOSANE	16.820	57283	0.396 ug/ml
14)	N-HEXATRIACONTANE	20.070	23536	0.163 ug/ml
15)	N-TETRACONTANE	21.743	180080	1.446 ug/ml
16)	N-TETRTETRACOOCTANE	24.444	255718	2.615 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032619\
Data File : FE029767.D
Signal(s) : FID1B.CH
Acq On : 26 Mar 2019 11:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 26 14:55:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
Quant Title :
QLast Update : Wed Mar 20 08:08:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

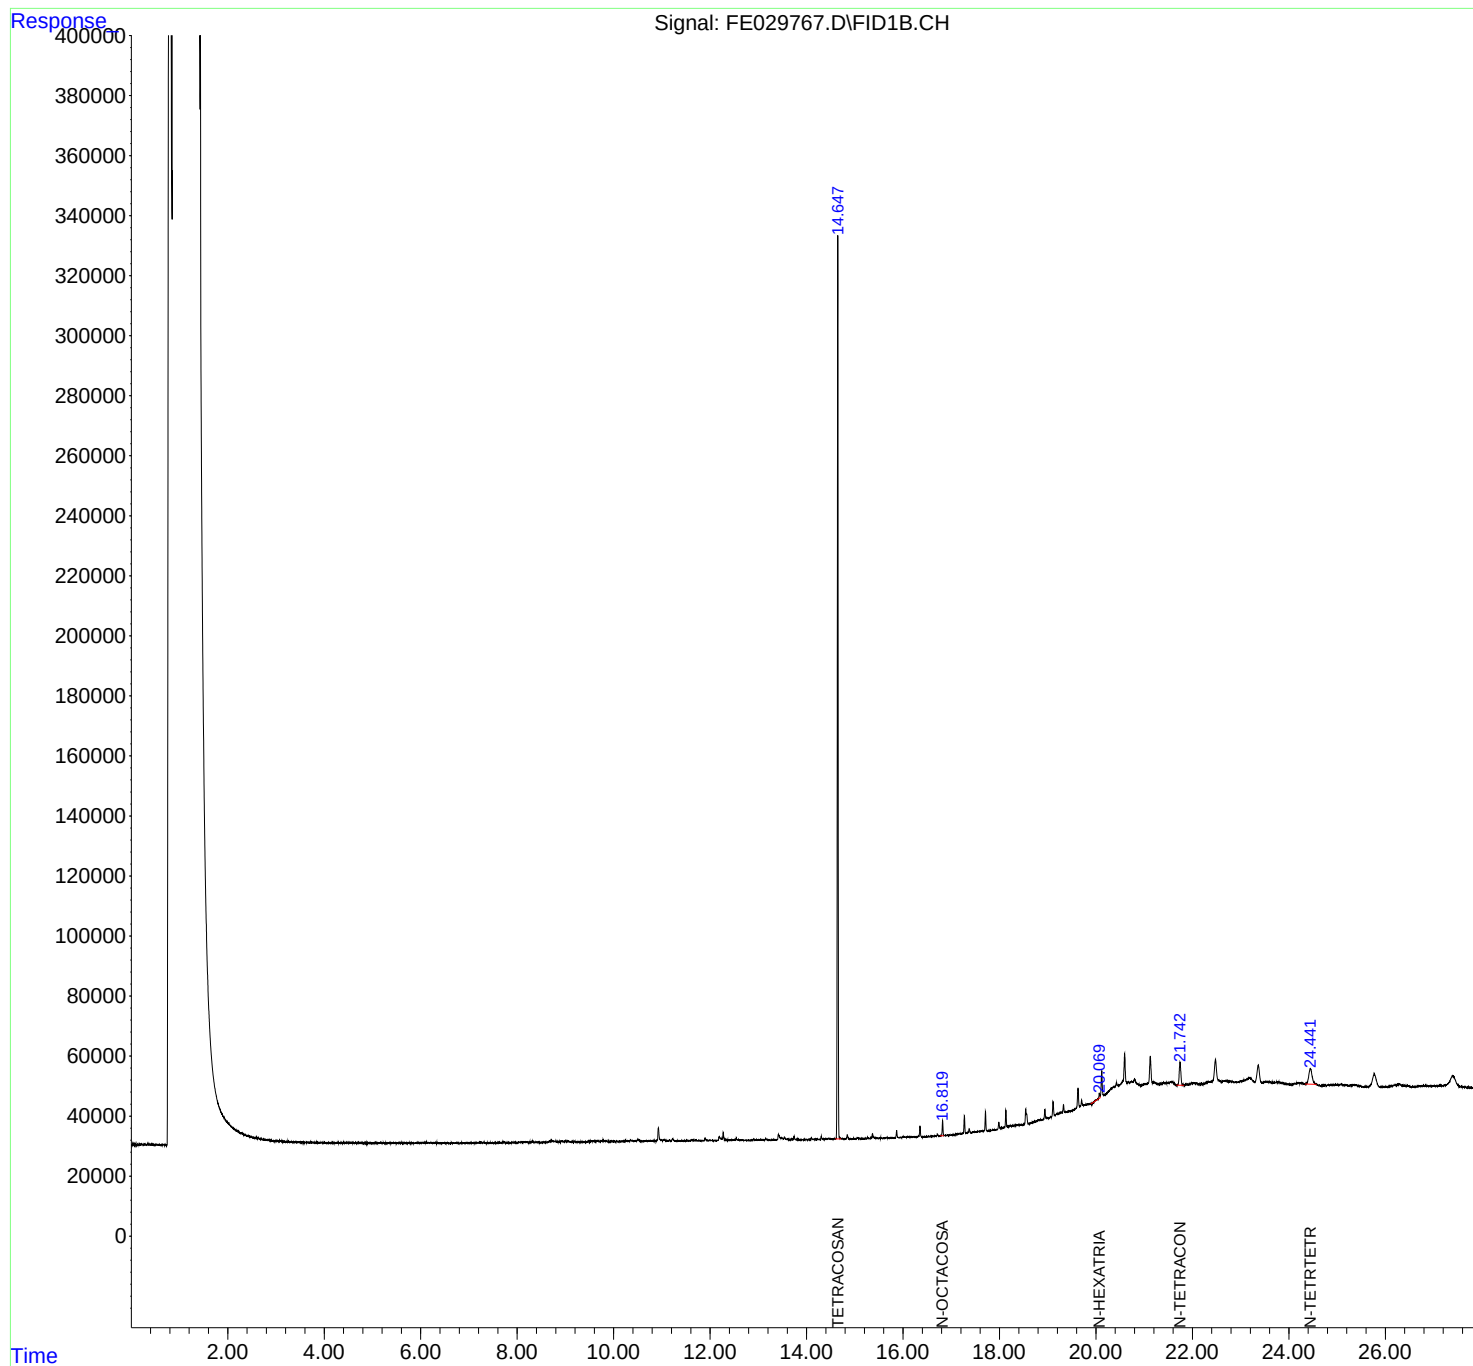

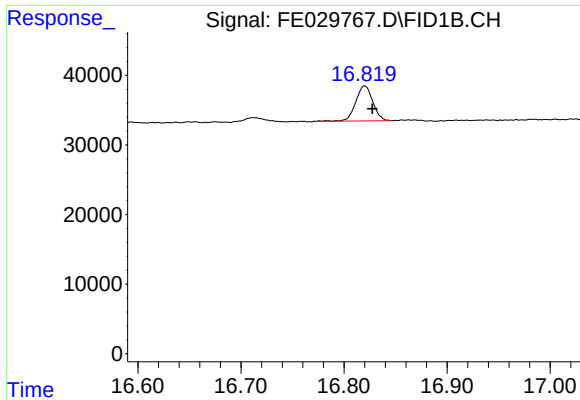


#11 N-OCTACOSANE

R.T.: 16.820 min
Delta R.T.: -0.007 min
Response: 57283
Conc: 0.40 ug/ml

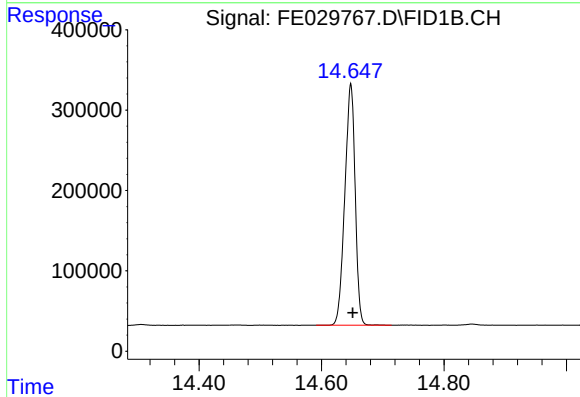


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: -0.003 min
Response: 3516994
Conc: 21.21 ug/ml

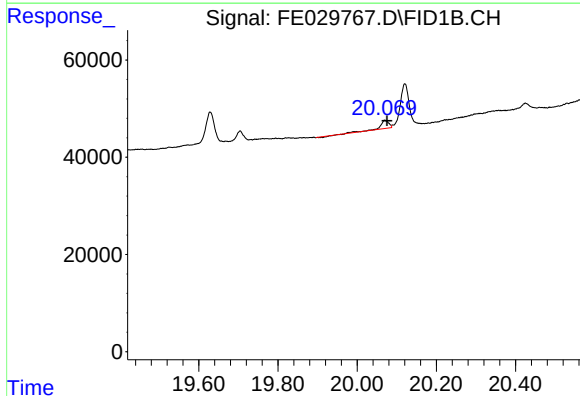


#14 N-HEXATRIACONTANE

R.T.: 20.070 min
Delta R.T.: -0.006 min
Response: 23536
Conc: 0.16 ug/ml

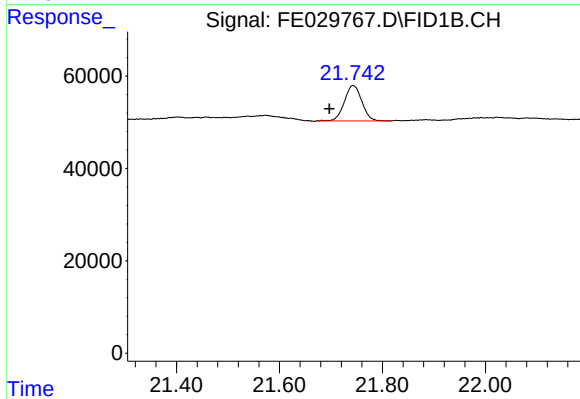

#15 N-TETRACONTANE

R.T.: 21.743 min
Delta R.T.: 0.046 min
Response: 180080
Conc: 1.45 ug/ml

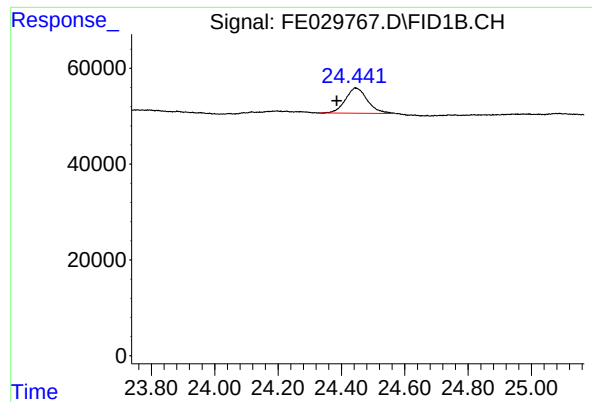

#16 N-TETRTETRACOCTANE

R.T.:	24.444 min
Delta R.T.:	0.059 min
Response:	255718
Conc:	2.62 ug/ml