

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
 Data File : FE031596.D
 Signal(s) : FID1B.CH
 Acq On : 26 Mar 2020 22:10
 Operator : DD\AJ
 Sample : L2013-08 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 04:42:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.388	614617	1.665 ug/ml
Target Compounds			
7) N-EICOSANE	12.349	698583	1.634 ug/ml
10) N-TETRACOSANE	14.577	438932	1.031 ug/ml
11) N-HEXACOSANE	15.615	363981	0.867 ug/ml
12) N-OCTACOSANE	16.563	475107	1.132 ug/ml
13) N-TRIACONTANE	17.450	782810	1.873 ug/ml
14) N-DOTRIACONTANE	18.283	472631	1.193 ug/ml
15) N-TETRATRIACONTANE	19.066	207304	0.600 ug/ml
16) N-HEXATRIACONTANE	19.840	522011	1.869 ug/ml
17) N-OCTATRIACONTANE	20.508	339844	1.501 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
Data File : FE031596.D
Signal(s) : FID1B.CH
Acq On : 26 Mar 2020 22:10
Operator : DD\AJ
Sample : L2013-08 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 04:42:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

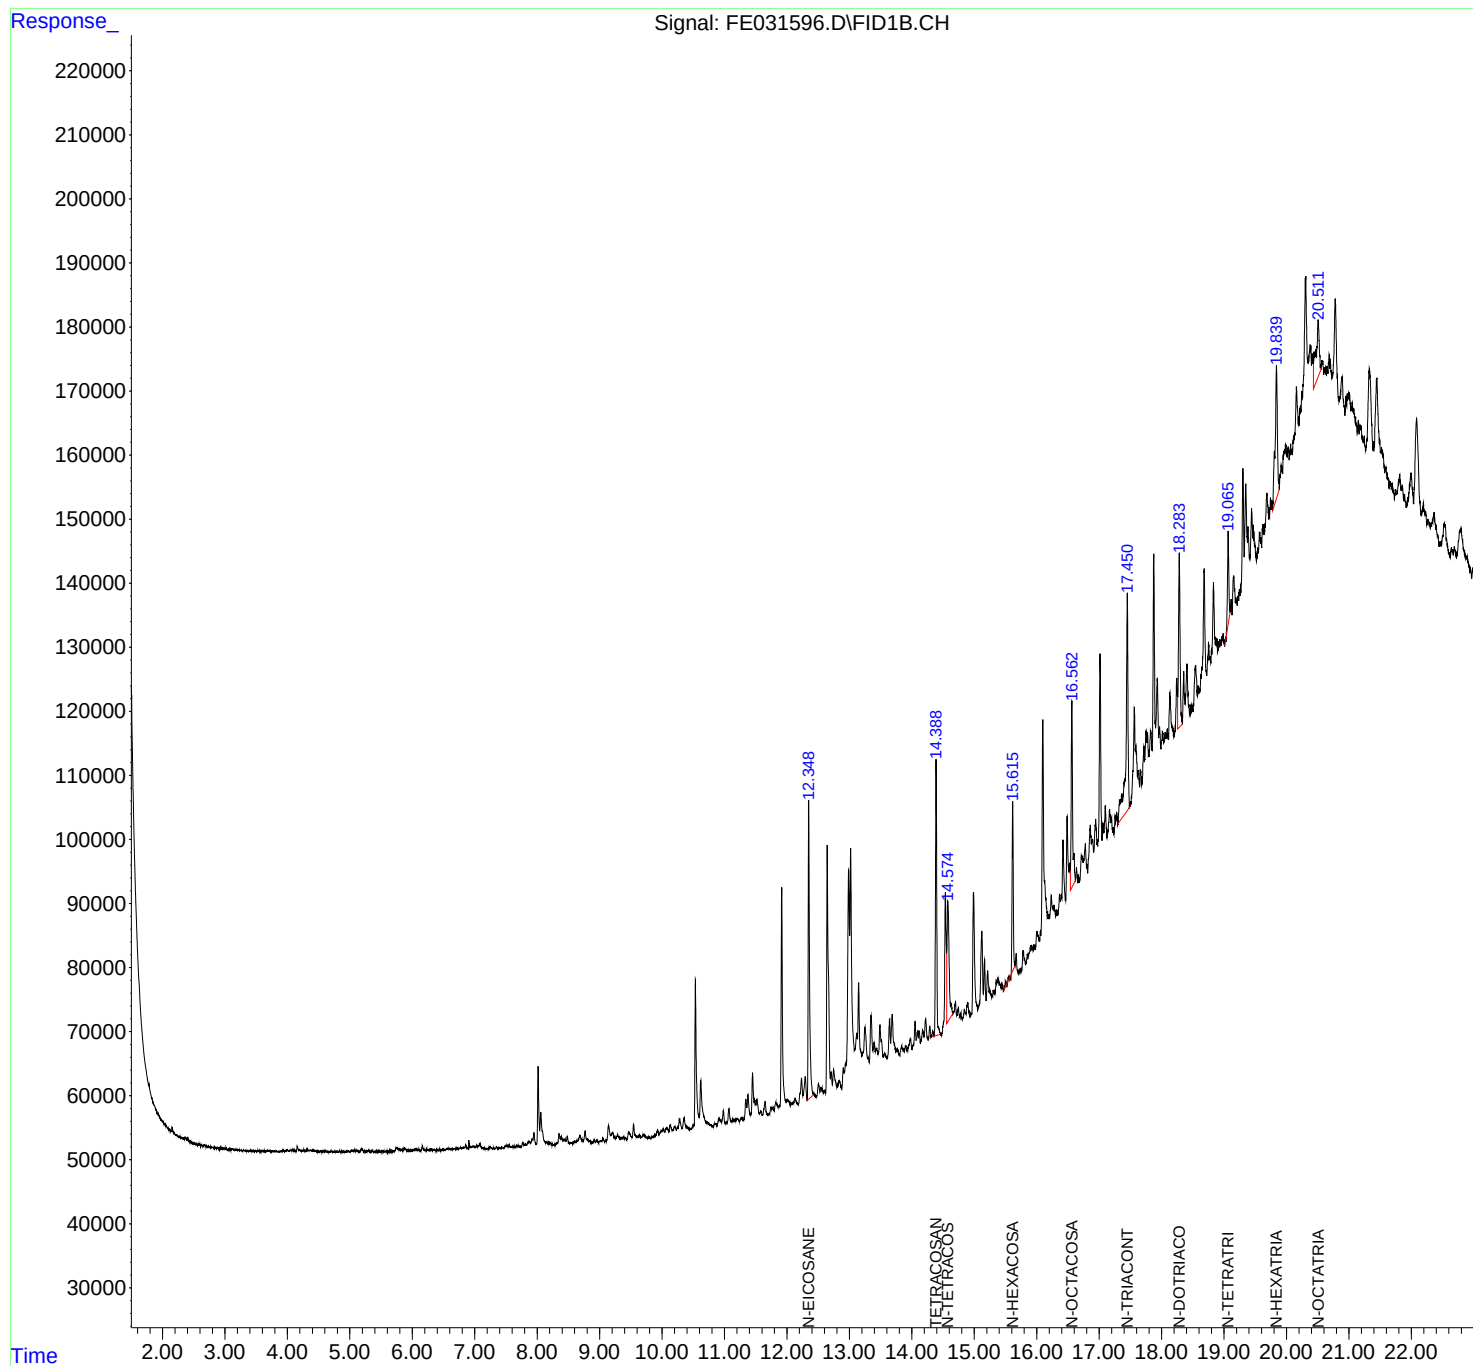


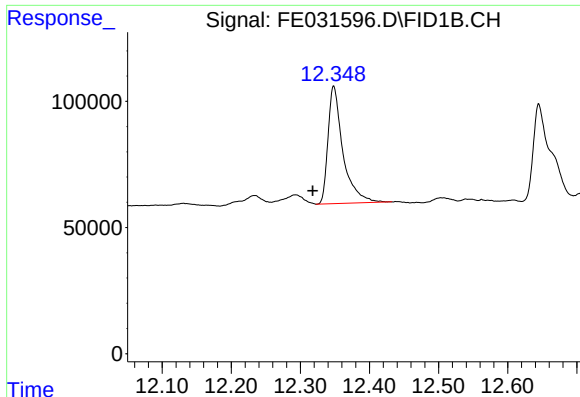

#7 N-EICOSANE


R.T.: 12.349 min
Delta R.T.: 0.031 min
Response: 698583
Conc: 1.63 ug/ml

Instrument :
FID_E
ClientSampleId :

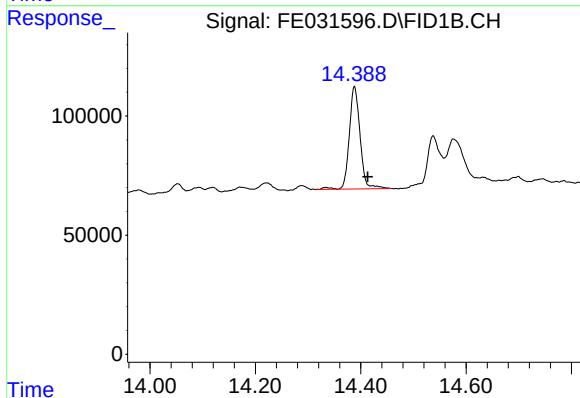


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.388 min
Delta R.T.: -0.025 min
Response: 614617
Conc: 1.67 ug/ml

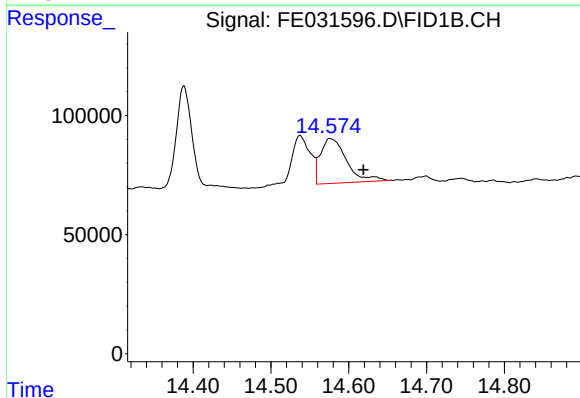


#10 N-TETRACOSANE

R.T.: 14.577 min
Delta R.T.: -0.042 min
Response: 438932
Conc: 1.03 ug/ml

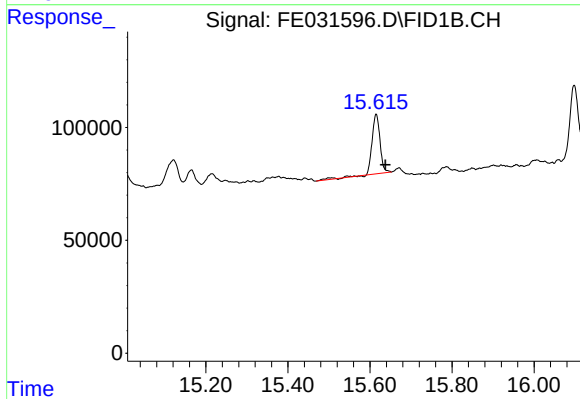

#11 N-HEXACOSANE


R.T.: 15.615 min
Delta R.T.: -0.023 min
Response: 363981
Conc: 0.87 ug/ml

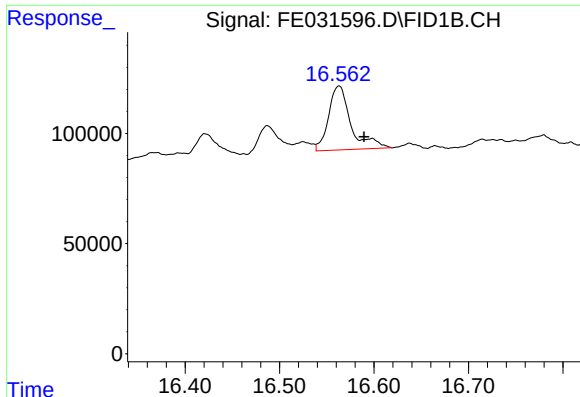

#12 N-OCTACOSANE


R.T.: 16.563 min
Delta R.T.: -0.027 min
Response: 475107
Conc: 1.13 ug/ml

Instrument :
FID_E
ClientSampleId :

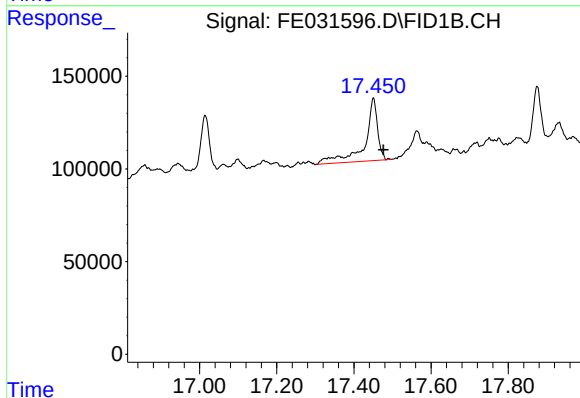


#13 N-TRIACONTANE

R.T.: 17.450 min
Delta R.T.: -0.026 min
Response: 782810
Conc: 1.87 ug/ml

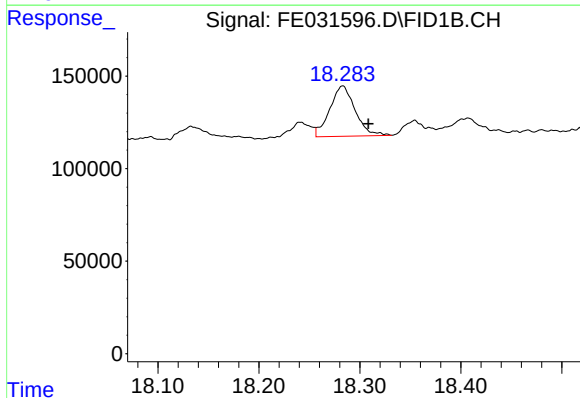


#14 N-DOTRIACONTANE

R.T.: 18.283 min
Delta R.T.: -0.026 min
Response: 472631
Conc: 1.19 ug/ml

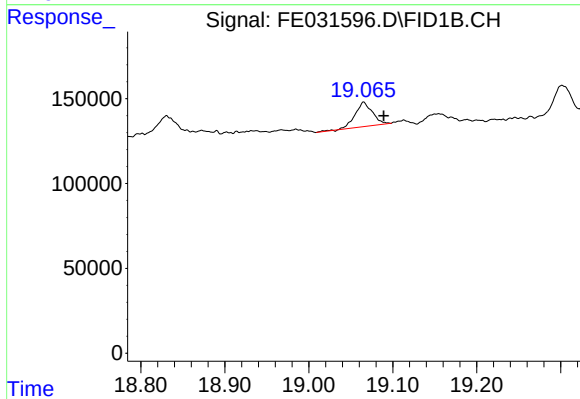

#15 N-TETRATRIACONTANE


R.T.: 19.066 min
Delta R.T.: -0.024 min
Response: 207304
Conc: 0.60 ug/ml

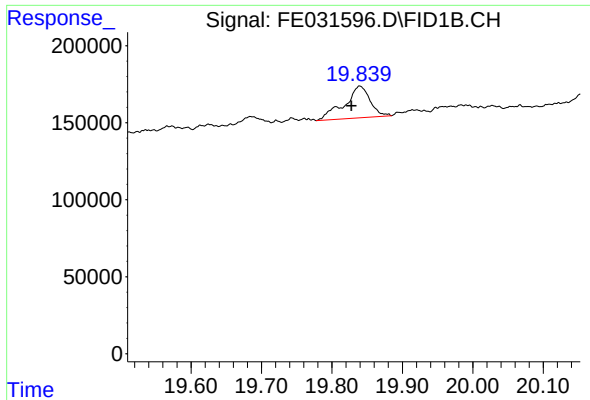

#16 N-HEXATRIACONTANE

R.T.: 19.840 min
Delta R.T.: 0.012 min
Response: 522011
Conc: 1.87 ug/ml

Instrument :
FID_E
ClientSampleId :

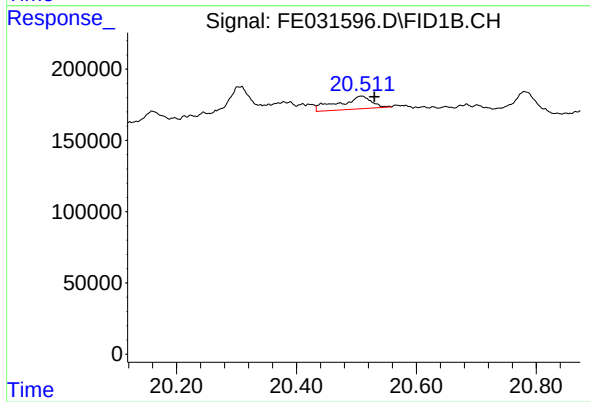

#17 N-OCTATRIACONTANE

R.T.: 20.508 min
Delta R.T.: -0.022 min
Response: 339844
Conc: 1.50 ug/ml