

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
 Data File : FE031597.D
 Signal(s) : FID1B.CH
 Acq On : 26 Mar 2020 22:44
 Operator : DD\AJ
 Sample : L2013-09 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 04:42:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.389	652284	1.767 ug/ml
Target Compounds			
7) N-EICOSANE	12.348	1168348	2.733 ug/ml
10) N-TETRACOSANE	14.574	703737	1.653 ug/ml
11) N-HEXACOSANE	15.614	240691	0.573 ug/ml
12) N-OCTACOSANE	16.562	384612	0.916 ug/ml
13) N-TRIACONTANE	17.449	495215	1.185 ug/ml
14) N-DOTRIACONTANE	18.279	391279	0.987 ug/ml
16) N-HEXATRIACONTANE	19.803	154489	0.553 ug/ml
17) N-OCTATRIACONTANE	20.504	664047	2.933 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
Data File : FE031597.D
Signal(s) : FID1B.CH
Acq On : 26 Mar 2020 22:44
Operator : DD\AJ
Sample : L2013-09 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 04:42:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

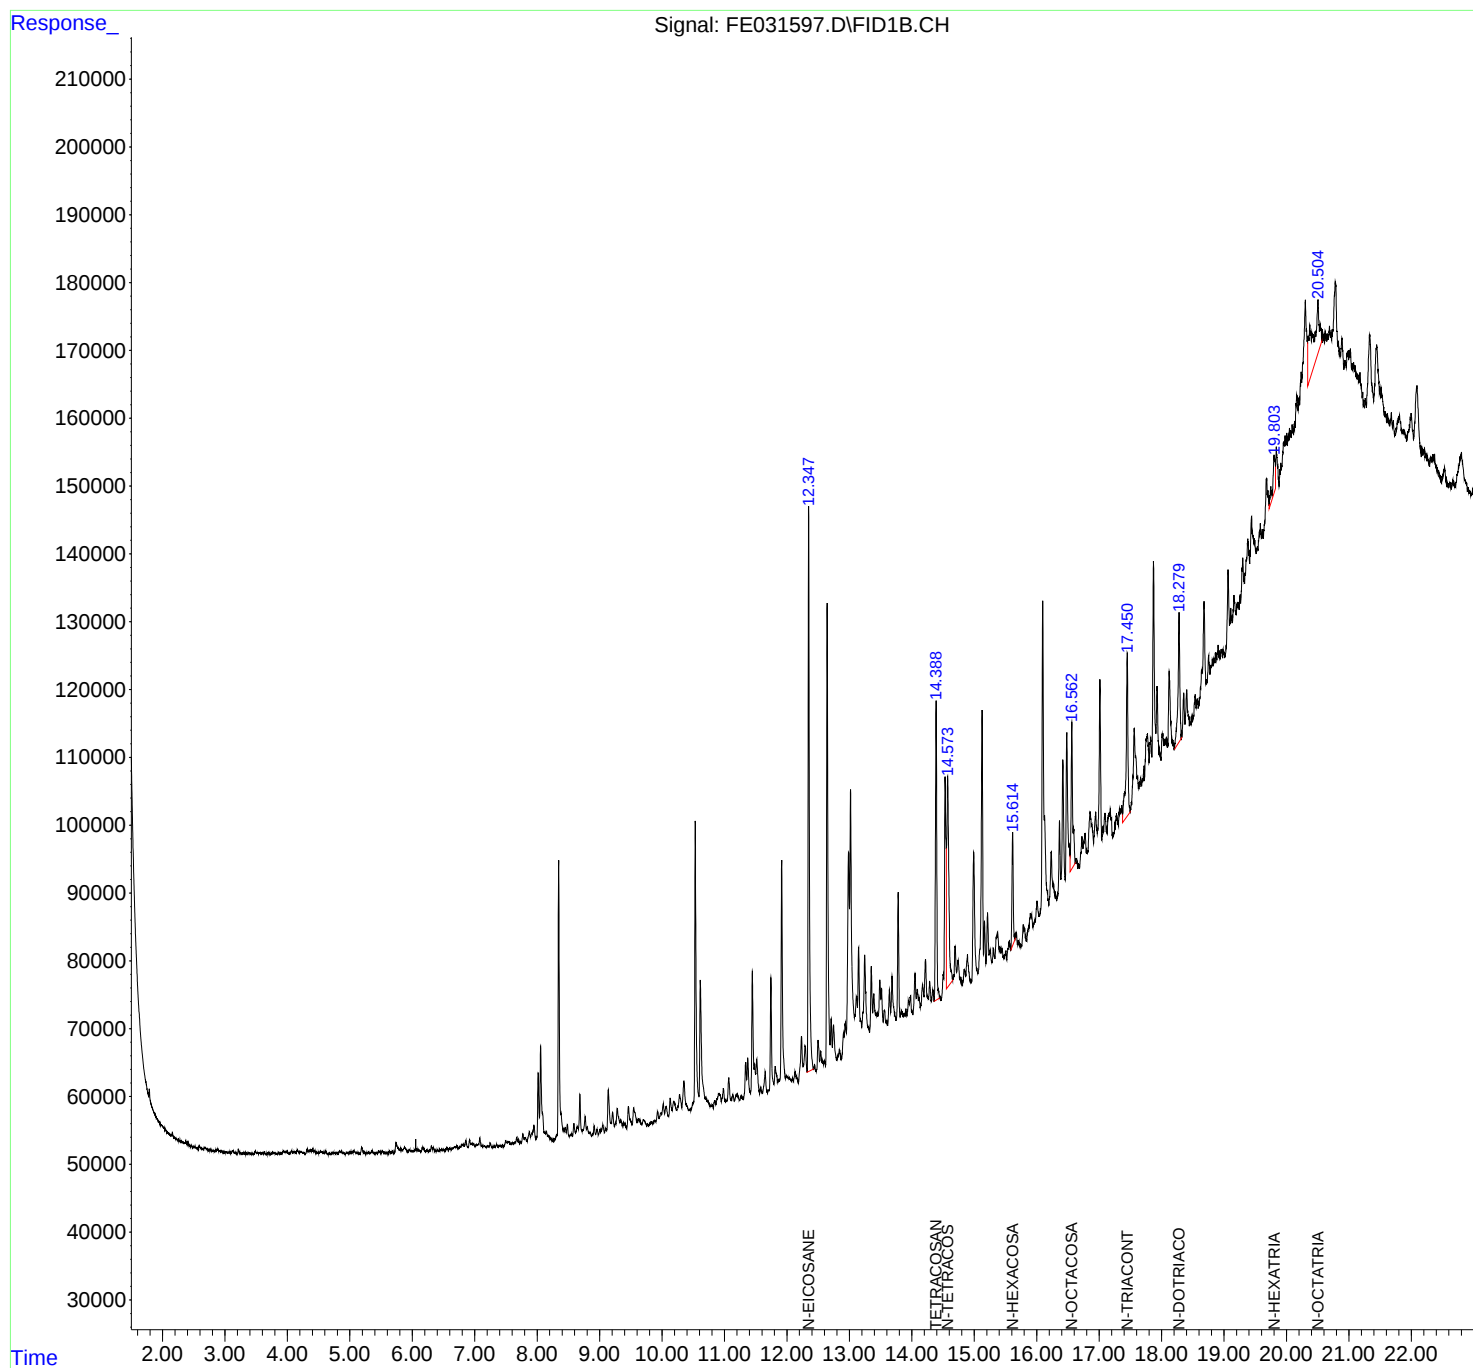


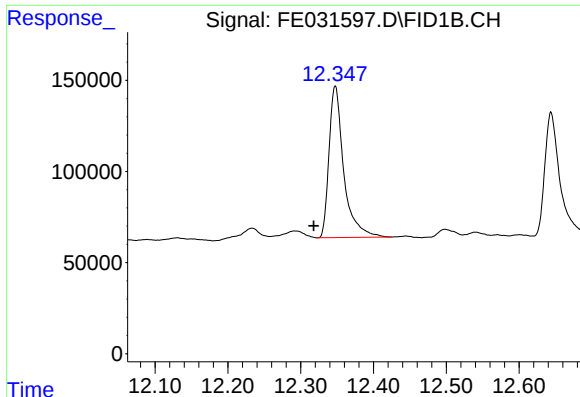

#7 N-EICOSANE


R.T.: 12.348 min
Delta R.T.: 0.030 min
Response: 1168348
Conc: 2.73 ug/ml

Instrument :
FID_E
ClientSampleId :

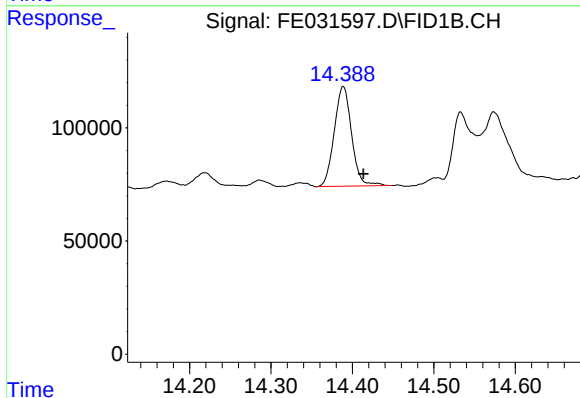


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.389 min
Delta R.T.: -0.025 min
Response: 652284
Conc: 1.77 ug/ml

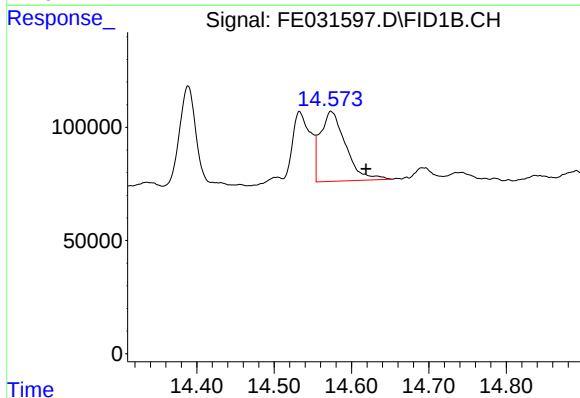


#10 N-TETRACOSANE

R.T.: 14.574 min
Delta R.T.: -0.045 min
Response: 703737
Conc: 1.65 ug/ml

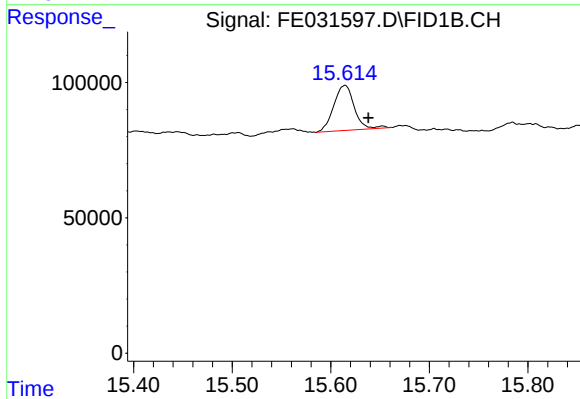

#11 N-HEXACOSANE


R.T.: 15.614 min
Delta R.T.: -0.024 min
Response: 240691
Conc: 0.57 ug/ml

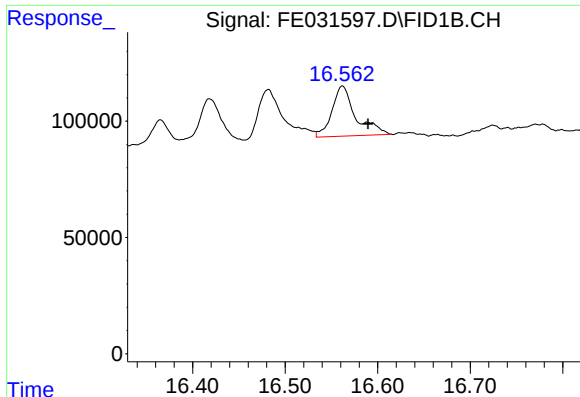

#12 N-OCTACOSANE


R.T.: 16.562 min
Delta R.T.: -0.028 min
Response: 384612
Conc: 0.92 ug/ml

Instrument :
FID_E
ClientSampleId :

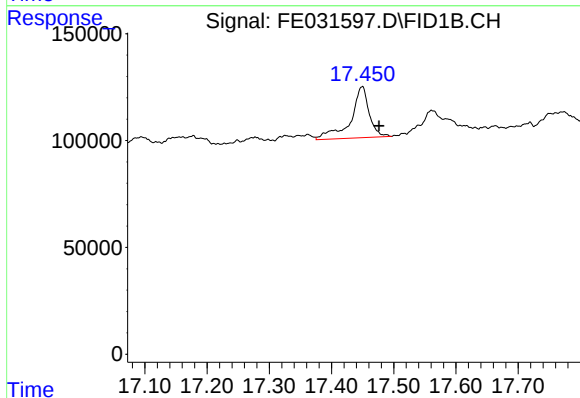


#13 N-TRIACONTANE

R.T.: 17.449 min
Delta R.T.: -0.028 min
Response: 495215
Conc: 1.19 ug/ml

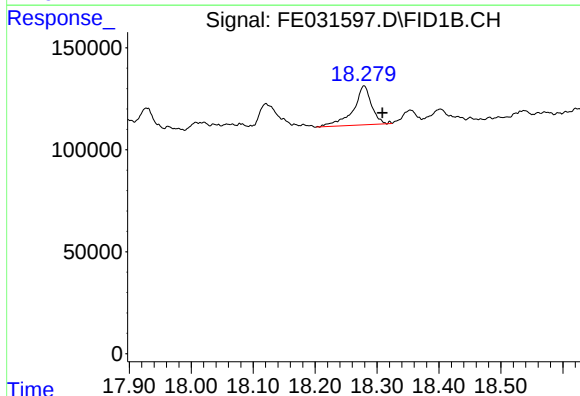


#14 N-DOTRIACONTANE

R.T.: 18.279 min
Delta R.T.: -0.030 min
Response: 391279
Conc: 0.99 ug/ml

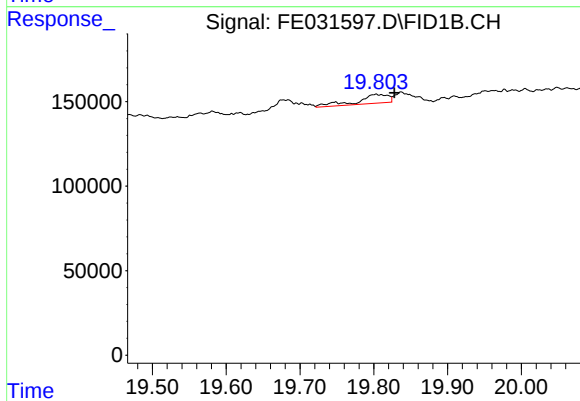

#16 N-HEXATRIACONTANE

R.T.: 19.803 min
Delta R.T.: -0.025 min
Response: 154489
Conc: 0.55 ug/ml

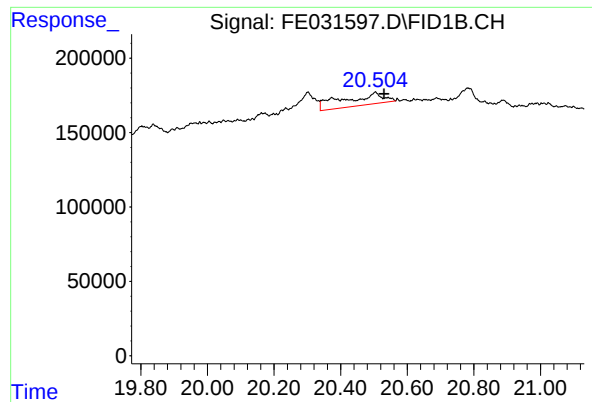

#17 N-OCTATRIACONTANE

R.T.: 20.504 min
Delta R.T.: -0.026 min
Response: 664047
Conc: 2.93 ug/ml

Instrument :
FID_E
ClientSampleId :