

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
 Data File : FE031600.D
 Signal(s) : FID1B.CH
 Acq On : 27 Mar 2020 00:23
 Operator : DD\AJ
 Sample : L2011-06 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 04:43:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.387	579357	1.570 ug/ml
Target Compounds			
7) N-EICOSANE	12.347	2408942	5.635 ug/ml
10) N-TETRACOSANE	14.570	1332271	3.128 ug/ml
11) N-HEXACOSANE	15.616	467409	1.113 ug/ml
12) N-OCTACOSANE	16.562	762307	1.816 ug/ml
13) N-TRIACONTANE	17.449	561440	1.344 ug/ml
14) N-DOTRIACONTANE	18.278	570458	1.440 ug/ml
15) N-TETRATRIACONTANE	19.066	519089	1.502 ug/ml
16) N-HEXATRIACONTANE	19.809	401255	1.436 ug/ml
17) N-OCTATRIACONTANE	20.502	1192569	5.268 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032620\
Data File : FE031600.D
Signal(s) : FID1B.CH
Acq On : 27 Mar 2020 00:23
Operator : DD\AJ
Sample : L2011-06 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 27 04:43:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

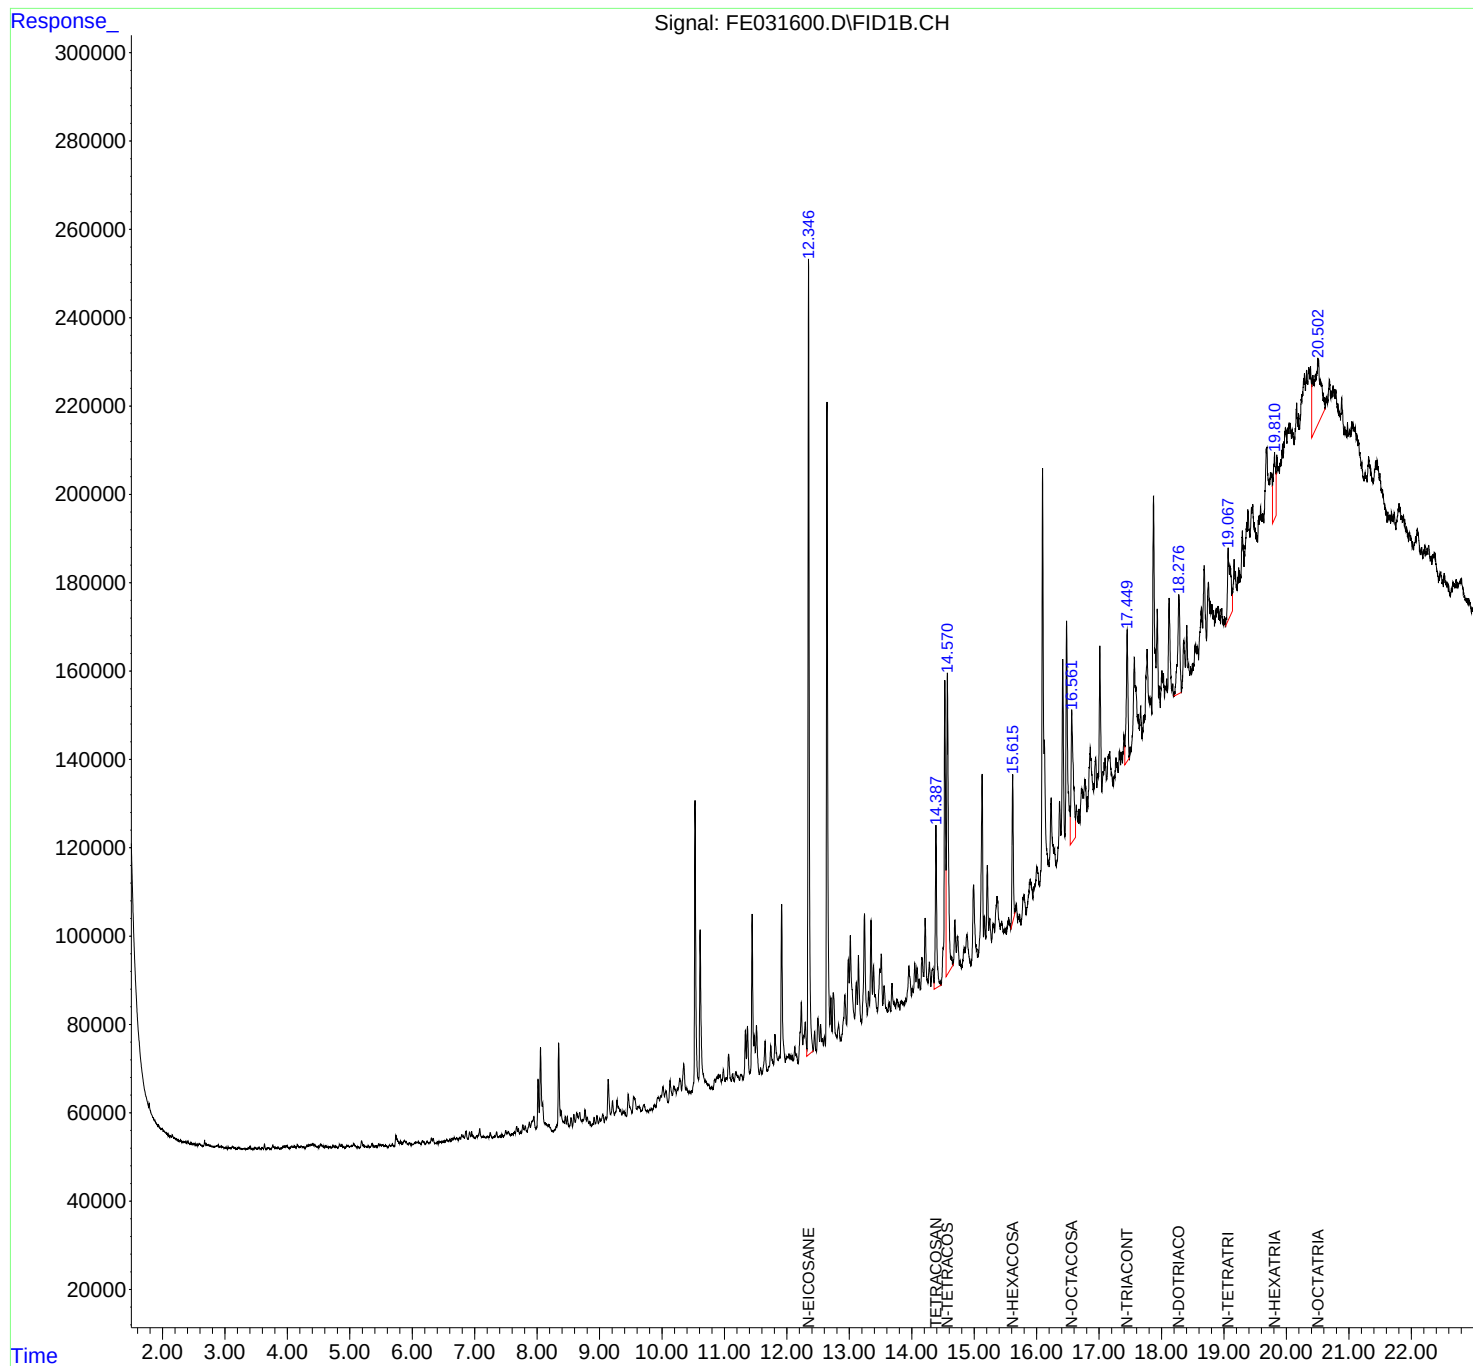


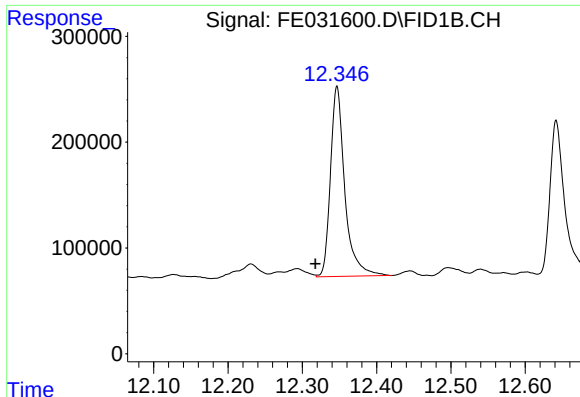

#7 N-EICOSANE


R.T.: 12.347 min
Delta R.T.: 0.029 min
Response: 2408942
Conc: 5.64 ug/ml

Instrument :
FID_E
ClientSampleId :

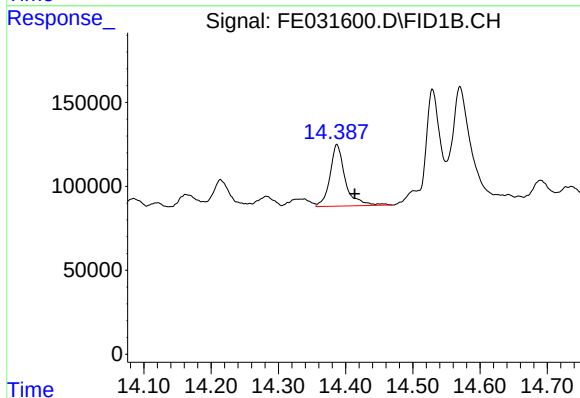


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.387 min
Delta R.T.: -0.026 min
Response: 579357
Conc: 1.57 ug/ml

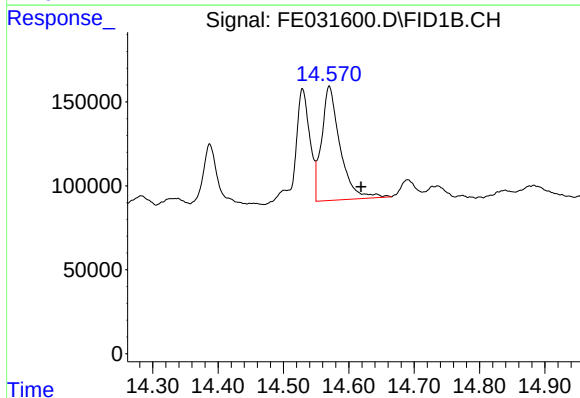


#10 N-TETRACOSANE

R.T.: 14.570 min
Delta R.T.: -0.049 min
Response: 1332271
Conc: 3.13 ug/ml

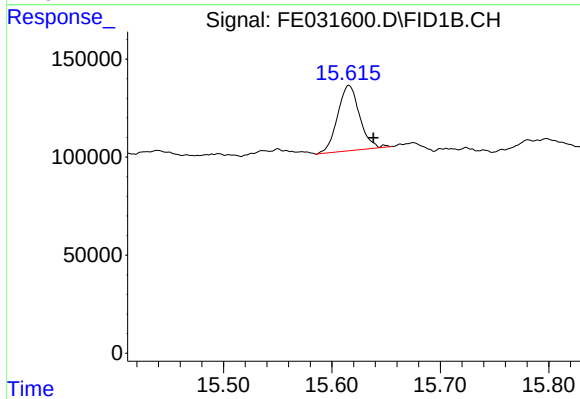

#11 N-HEXACOSANE


R.T.: 15.616 min
Delta R.T.: -0.022 min
Response: 467409
Conc: 1.11 ug/ml

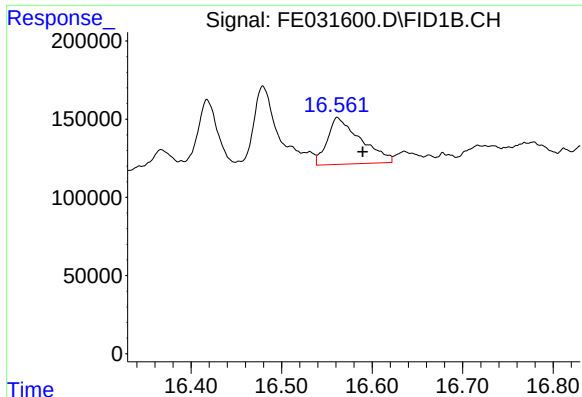

#12 N-OCTACOSANE


R.T.: 16.562 min
Delta R.T.: -0.027 min
Response: 762307
Conc: 1.82 ug/ml

Instrument :
FID_E
ClientSampleId :

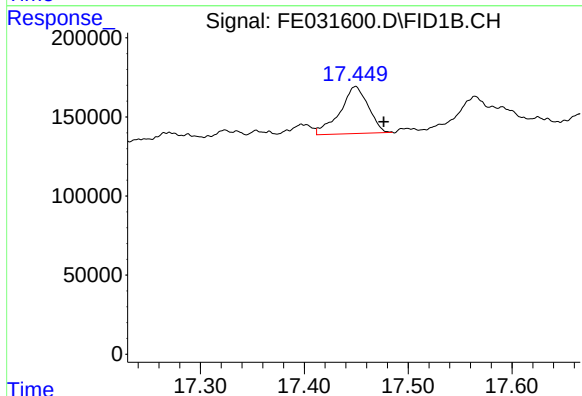


#13 N-TRIACONTANE

R.T.: 17.449 min
Delta R.T.: -0.027 min
Response: 561440
Conc: 1.34 ug/ml

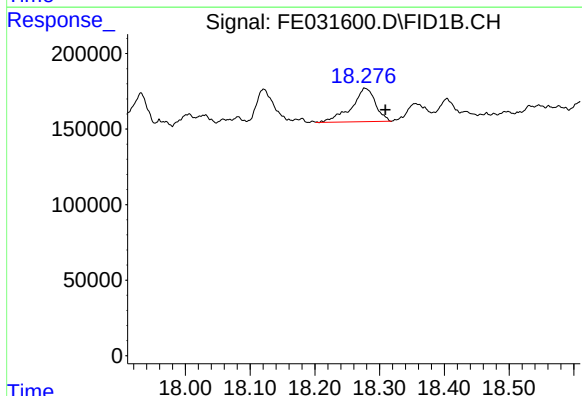


#14 N-DOTRIACONTANE

R.T.: 18.278 min
Delta R.T.: -0.030 min
Response: 570458
Conc: 1.44 ug/ml

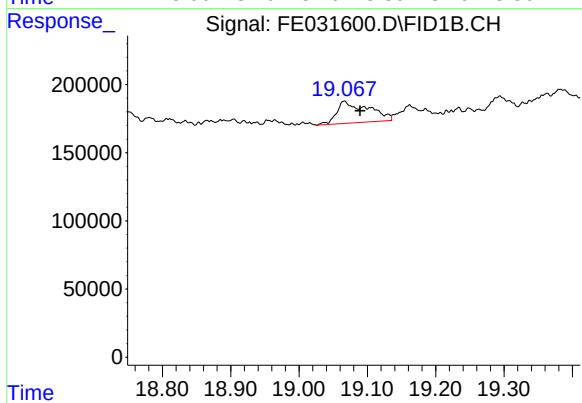

#15 N-TETRATRIACONTANE


R.T.: 19.066 min
Delta R.T.: -0.023 min
Response: 519089
Conc: 1.50 ug/ml

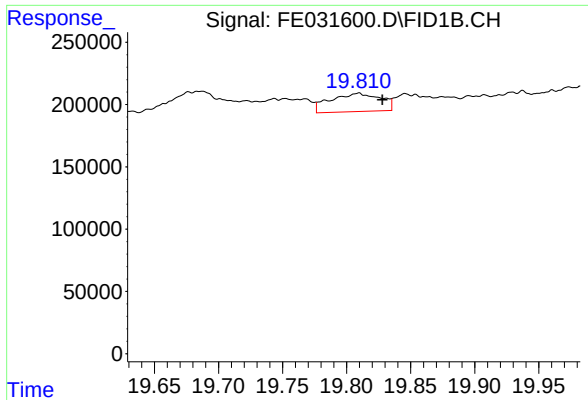

#16 N-HEXATRIACONTANE

R.T.: 19.809 min
Delta R.T.: -0.019 min
Response: 401255
Conc: 1.44 ug/ml

Instrument :
FID_E
ClientSampleId :

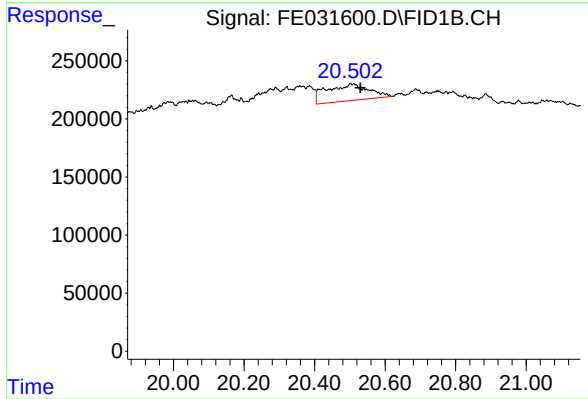

#17 N-OCTATRIACONTANE

R.T.: 20.502 min
Delta R.T.: -0.027 min
Response: 1192569
Conc: 5.27 ug/ml