

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032723AL\
 Data File : FE041026.D
 Signal(s) : FID1B.ch
 Acq On : 27 Mar 2023 09:17
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 28 03:23:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.030	17796	0.116 ug/ml
18) T n-Dotriacontane (C32)	18.869	27045	0.173 ug/ml
19) T n-Tetratriacontane (C34)	19.643	42649	0.275 ug/ml
20) T n-Hexatriacontane (C36)	20.366	17523	0.115 ug/ml
21) T n-Octatriacontane (C38)	21.111	40110	0.257 ug/ml
22) T n-Tetracontane (C40)	21.993	76865	0.482 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032723AL\
Data File : FE041026.D
Signal(s) : FID1B.ch
Acq On : 27 Mar 2023 09:17
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 28 03:23:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

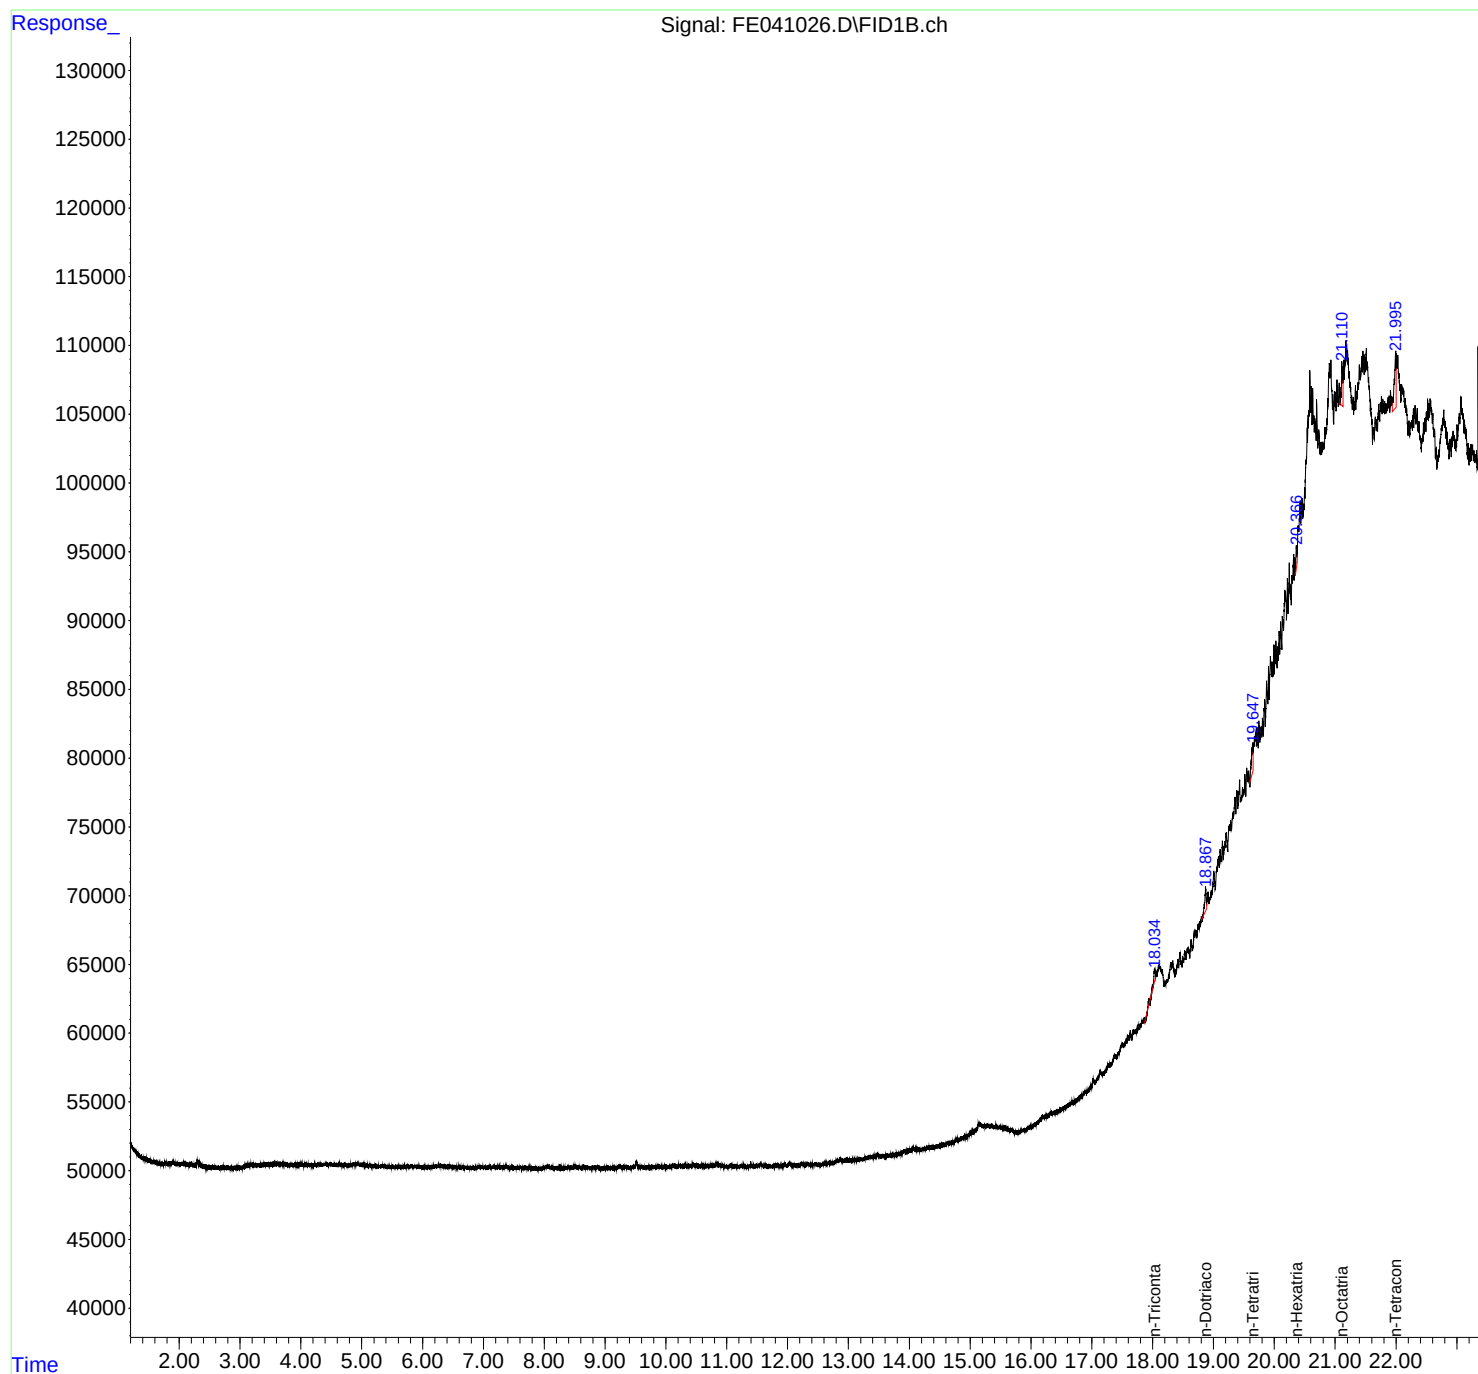


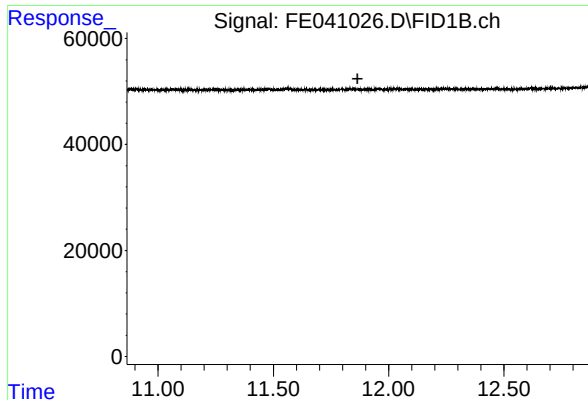

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

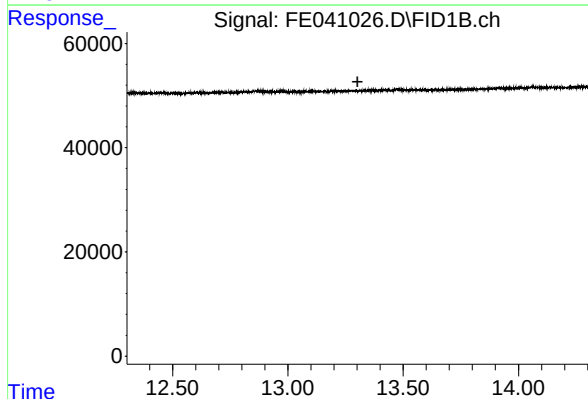


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

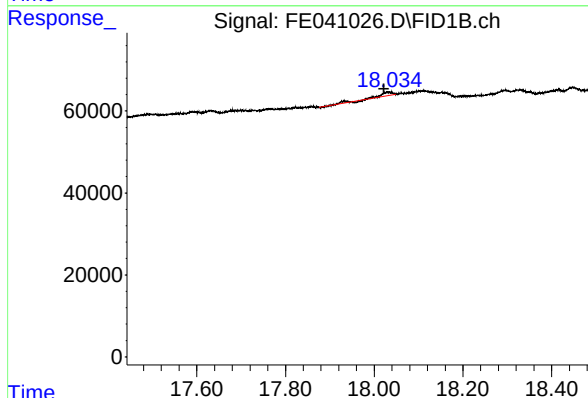


#17 n-Tricontane (C30)

R.T.: 18.030 min
Delta R.T.: 0.008 min
Response: 17796
Conc: 0.12 ug/ml

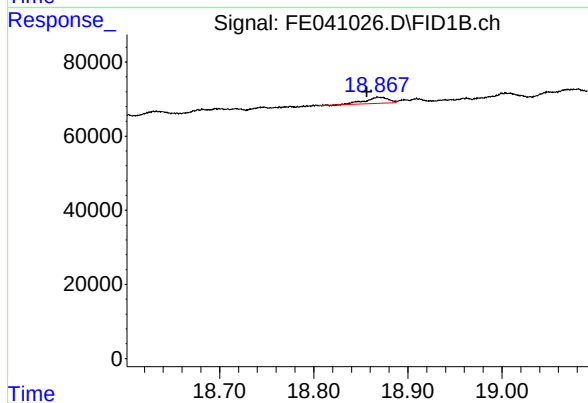

#18 n-Dotriacontane (C32)

R.T.: 18.869 min
Delta R.T.: 0.012 min
Response: 27045
Conc: 0.17 ug/ml

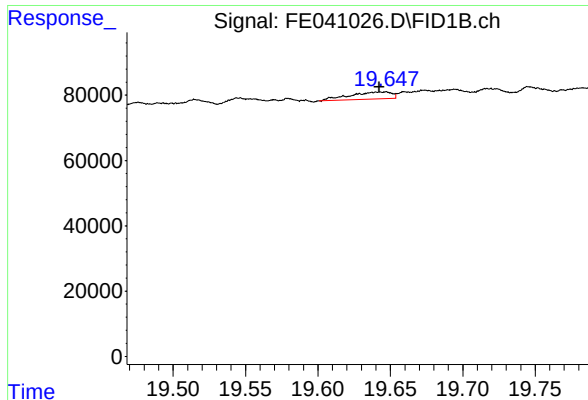


#19 n-Tetratriacontane (C34)

R.T.: 19.643 min
Delta R.T.: 0.000 min
Response: 42649
Conc: 0.28 ug/ml

Instrument :


FID_E

ClientSampleId :

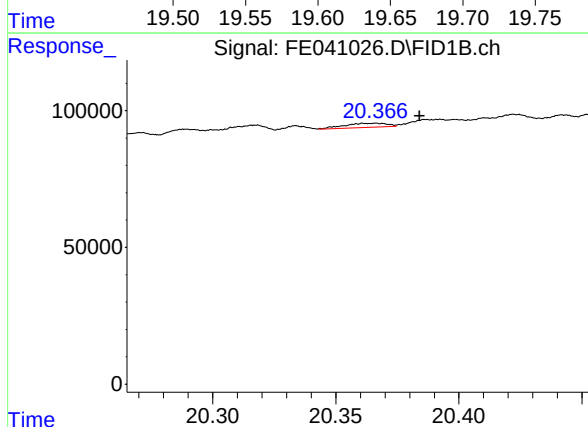


#20 n-Hexatriacontane (C36)

R.T.: 20.366 min
Delta R.T.: -0.018 min
Response: 17523
Conc: 0.12 ug/ml

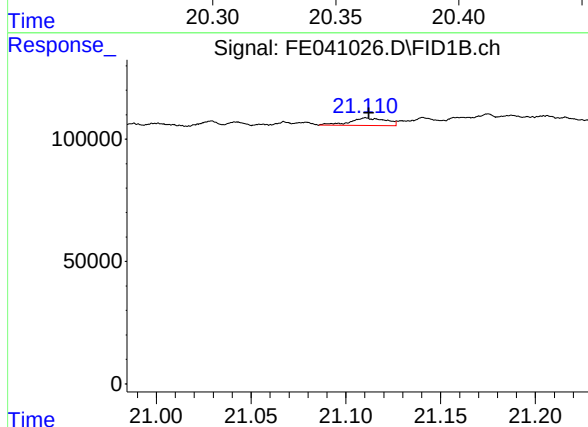

#21 n-Octatriacontane (C38)

R.T.: 21.111 min
Delta R.T.: -0.002 min
Response: 40110
Conc: 0.26 ug/ml

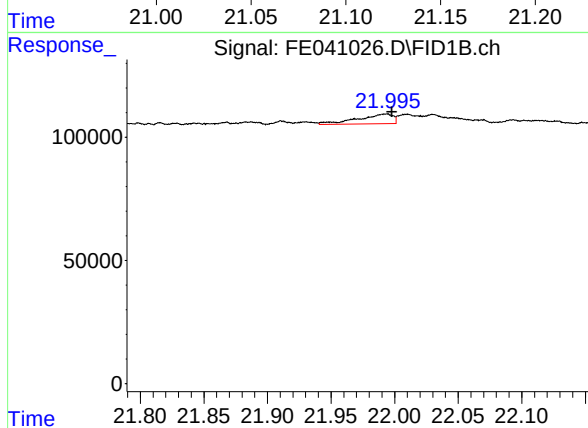

#22 n-Tetracontane (C40)

R.T.: 21.993 min
Delta R.T.: -0.005 min
Response: 76865
Conc: 0.48 ug/ml