

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032919\
Data File : FE029812.D
Signal(s) : FID1B.CH
Acq On : 29 Mar 2019 10:00
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 29 16:18:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
Quant Title :
QLast Update : Wed Mar 20 08:08:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
12)	N-DOTRIACONTANE	18.557	117744	0.719 ug/ml
14)	N-HEXATRIACONTANE	20.113	282966	1.958 ug/ml
15)	N-TETRACONTANE	21.732	485109	3.896 ug/ml
16)	N-TETRTETRACOOCTANE	24.423	509554	5.211 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032919\
Data File : FE029812.D
Signal(s) : FID1B.CH
Acq On : 29 Mar 2019 10:00
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 29 16:18:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
Quant Title :
QLast Update : Wed Mar 20 08:08:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

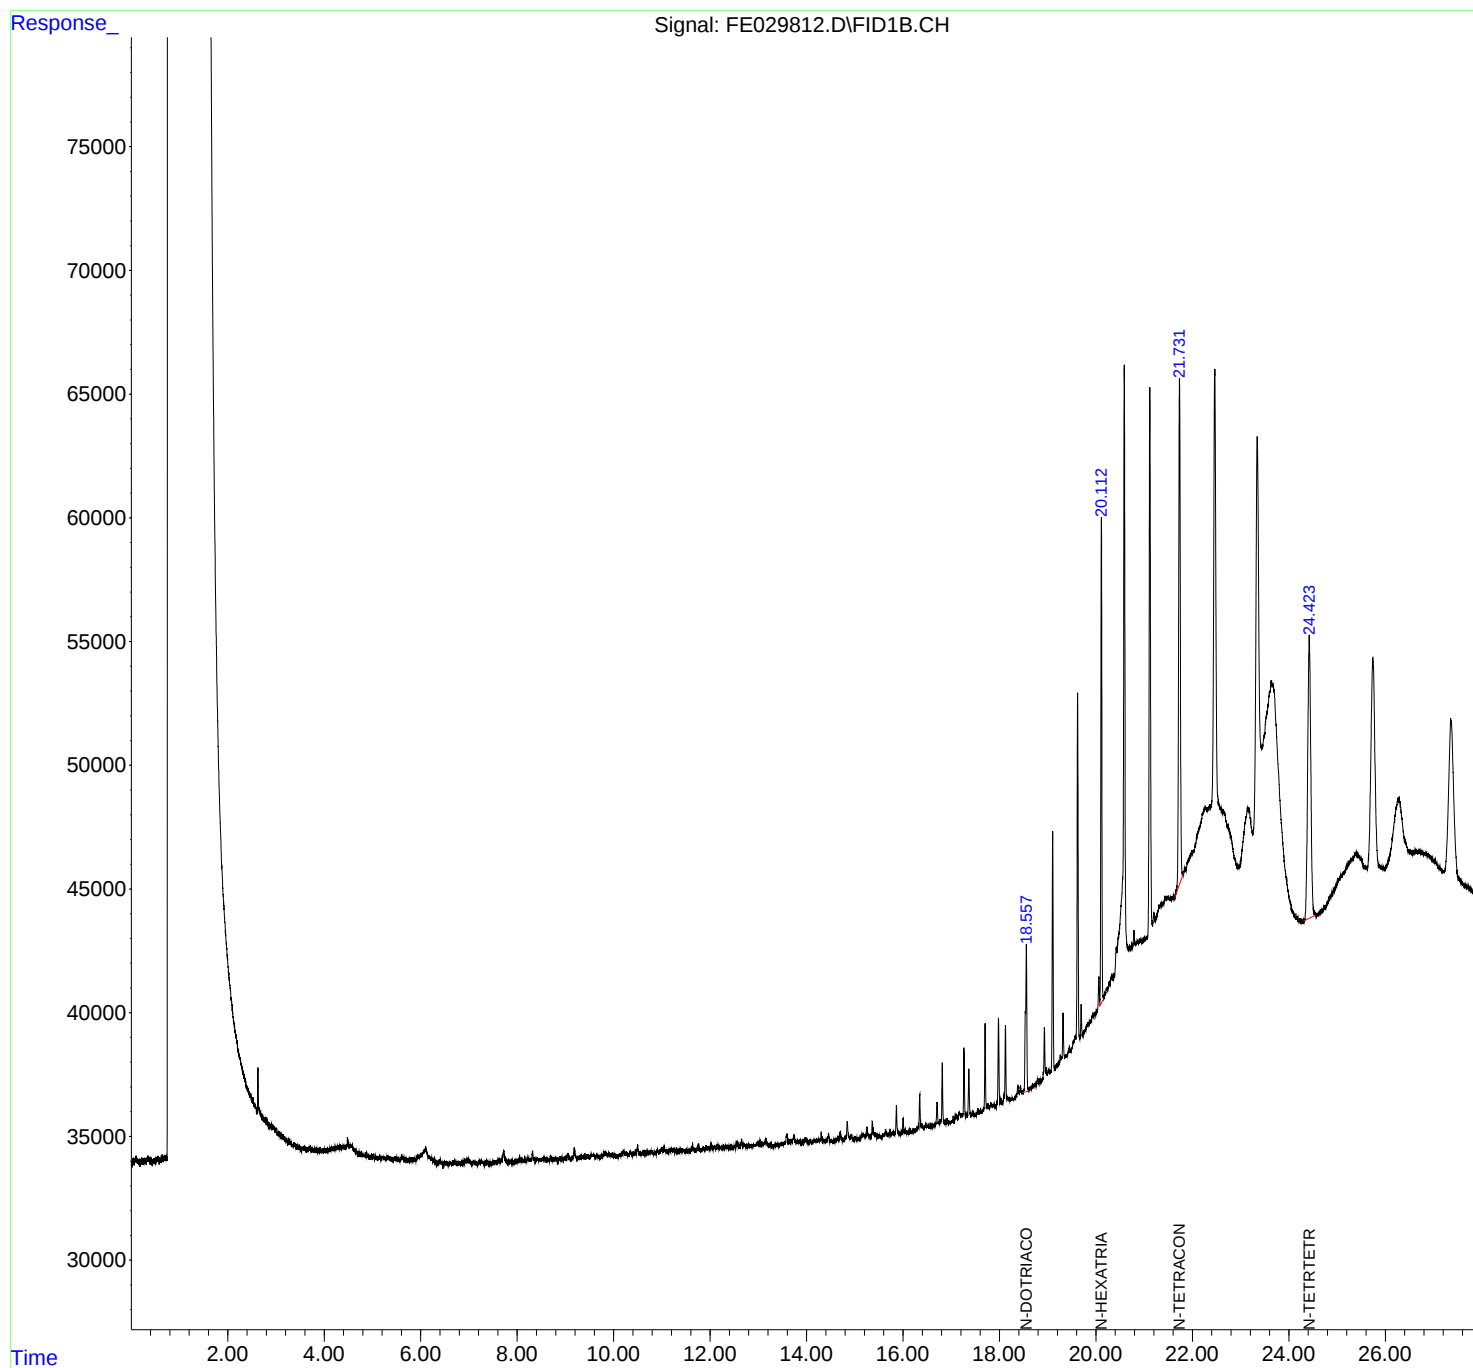

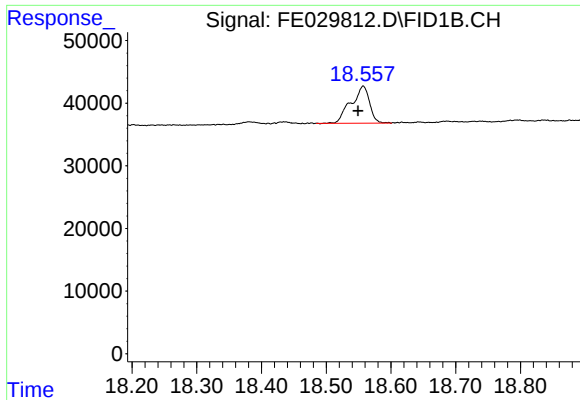


#12 N-DOTRIACONTANE

R.T.: 18.557 min
Delta R.T.: 0.008 min
Response: 117744
Conc: 0.72 ug/ml

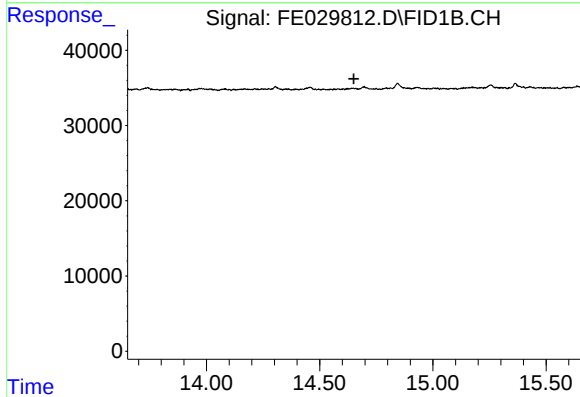


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.651 min
Response: 0
Conc: N.D.

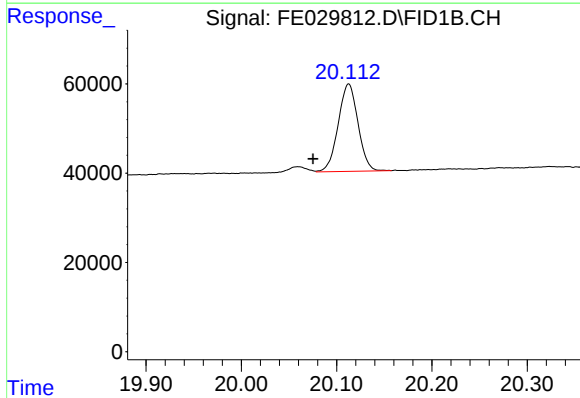


#14 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: 0.037 min
Response: 282966
Conc: 1.96 ug/ml

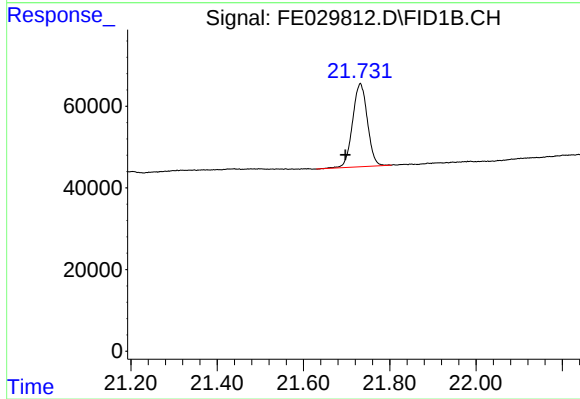

#15 N-TETRACONTANE

R.T.: 21.732 min
Delta R.T.: 0.035 min
Response: 485109
Conc: 3.90 ug/ml

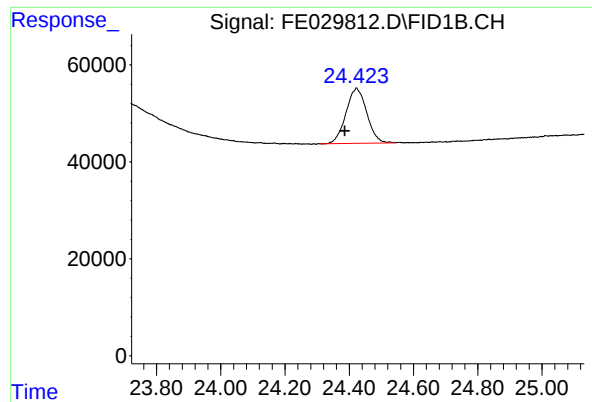

#16 N-TETRTETRACOCTANE

R.T.:	24.423 min
Delta R.T.:	0.037 min
Response:	509554
Conc:	5.21 ug/ml