

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032919\
 Data File : FE029815.D
 Signal(s) : FID1B.CH
 Acq On : 29 Mar 2019 12:04
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 29 16:18:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
 Quant Title :
 QLast Update : Wed Mar 20 08:08:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
5) N-DODECANE	6.391	4430592	27.392 ug/ml
11) N-OCTACOSANE	16.818	4185862	28.962 ug/ml
12) N-DOTRIACONTANE	18.535	215496	1.315 ug/ml
14) N-HEXATRIACONTANE	20.060	88273	0.611 ug/ml
15) N-TETRACONTANE	21.671	51765	0.416 ug/ml
16) N-TETRTETRACOOCTANE	24.334	417783	4.273 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE032919\
Data File : FE029815.D
Signal(s) : FID1B.CH
Acq On : 29 Mar 2019 12:04
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 29 16:18:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE031919.M
Quant Title :
QLast Update : Wed Mar 20 08:08:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

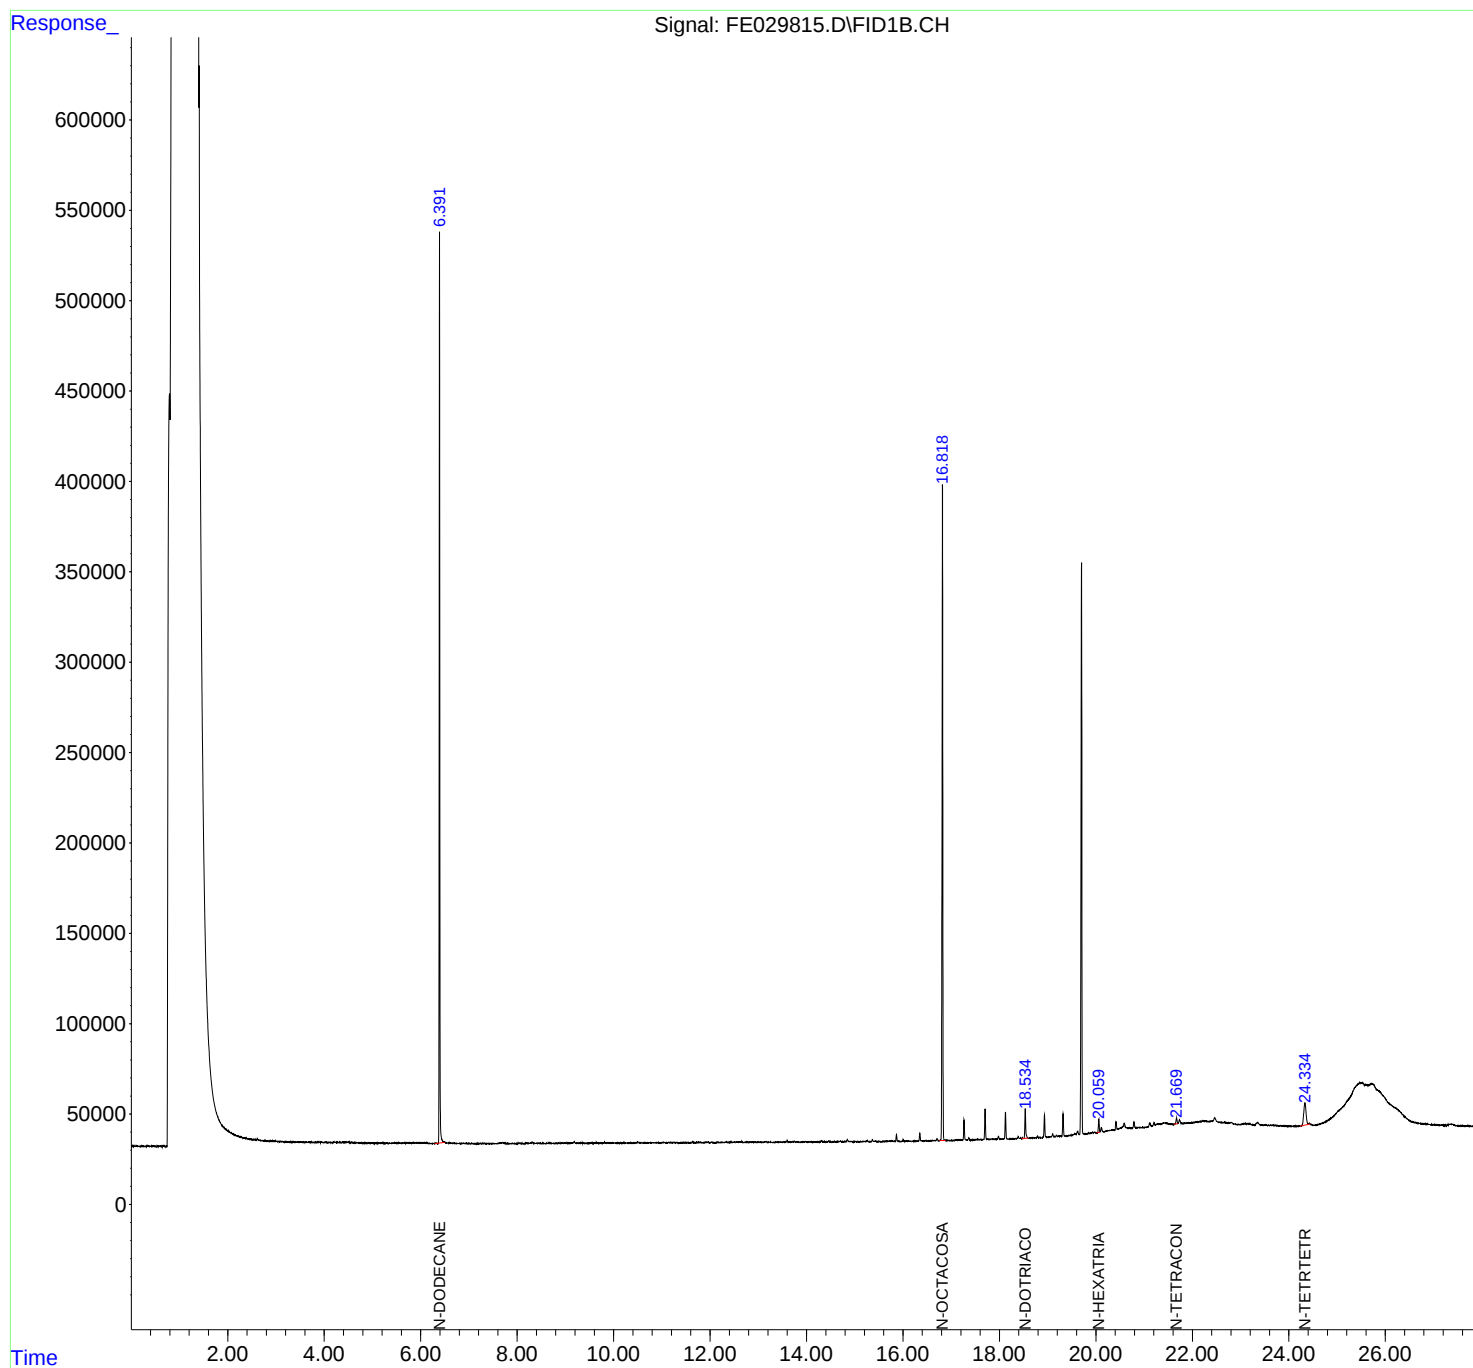

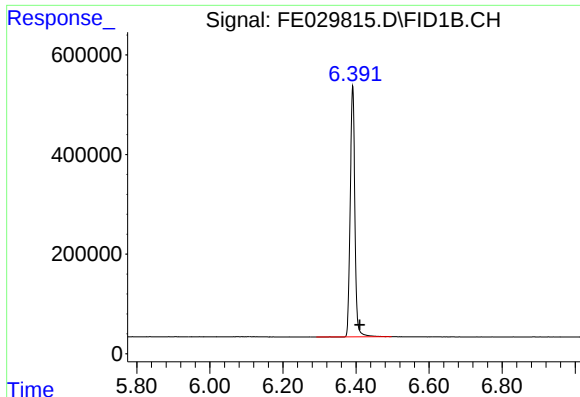


#5 N-DODECANE

R.T.: 6.391 min
Delta R.T.: -0.020 min
Response: 4430592
Conc: 27.39 ug/ml

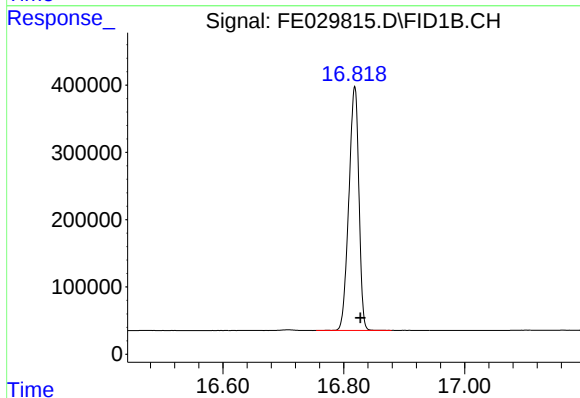


#11 N-OCTACOSANE

R.T.: 16.818 min
Delta R.T.: -0.009 min
Response: 4185862
Conc: 28.96 ug/ml

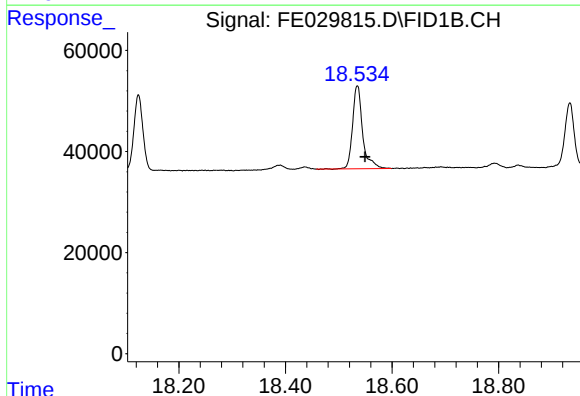


#12 N-DOTRIACONTANE

R.T.: 18.535 min
Delta R.T.: -0.014 min
Response: 215496
Conc: 1.32 ug/ml

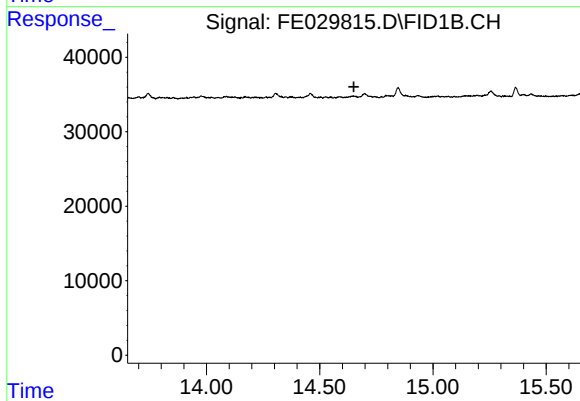


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.651 min
Response: 0
Conc: N.D.

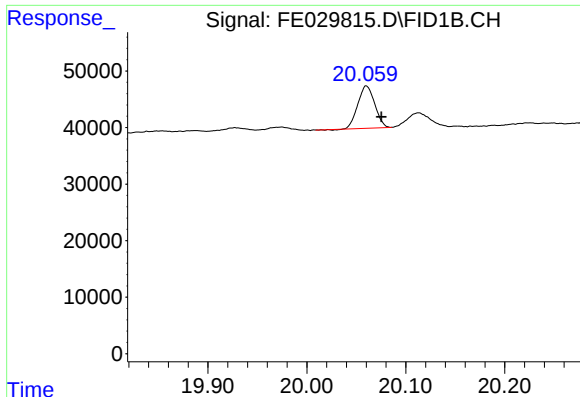


#14 N-HEXATRIACONTANE

R.T.: 20.060 min
Delta R.T.: -0.015 min
Response: 88273
Conc: 0.61 ug/ml

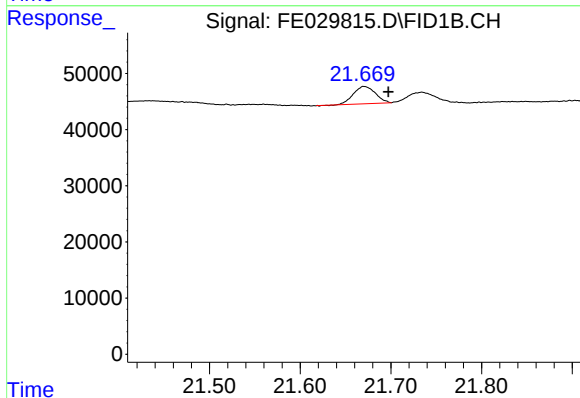

#15 N-TETRACONTANE

R.T.: 21.671 min
Delta R.T.: -0.027 min
Response: 51765
Conc: 0.42 ug/ml

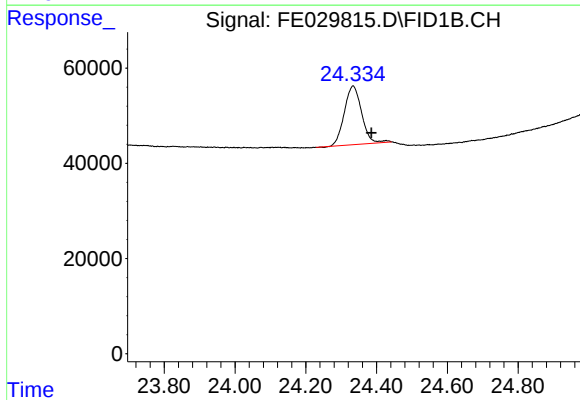

#16 N-TETRTETRACOCOCTANE

R.T.: 24.334 min
Delta R.T.: -0.052 min
Response: 417783
Conc: 4.27 ug/ml