

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE033023AL\
 Data File : FE041088.D
 Signal(s) : FID1B.ch
 Acq On : 30 Mar 2023 07:50
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 30 14:49:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.832	134079	0.786 ug/ml
11) T n-Heneicosane (C21)	13.450	135234	0.799 ug/ml
13) T n-Docosane (C22)	14.040	153453	0.927 ug/ml
14) T n-Tetracosane (C24)	15.146	87503	0.541 ug/ml
15) T n-Hexacosane (C26)	16.169	96474	0.622 ug/ml
16) T n-Octacosane (C28)	17.120	101825	0.665 ug/ml
17) T n-Tricontane (C30)	18.008	77525	0.507 ug/ml
18) T n-Dotriacontane (C32)	18.842	164818	1.056 ug/ml
19) T n-Tetratriacontane (C34)	19.626	37358	0.241 ug/ml
20) T n-Hexatriacontane (C36)	20.371	37188	0.245 ug/ml
22) T n-Tetracontane (C40)	22.031	162530	1.018 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE033023AL\
Data File : FE041088.D
Signal(s) : FID1B.ch
Acq On : 30 Mar 2023 07:50
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 30 14:49:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

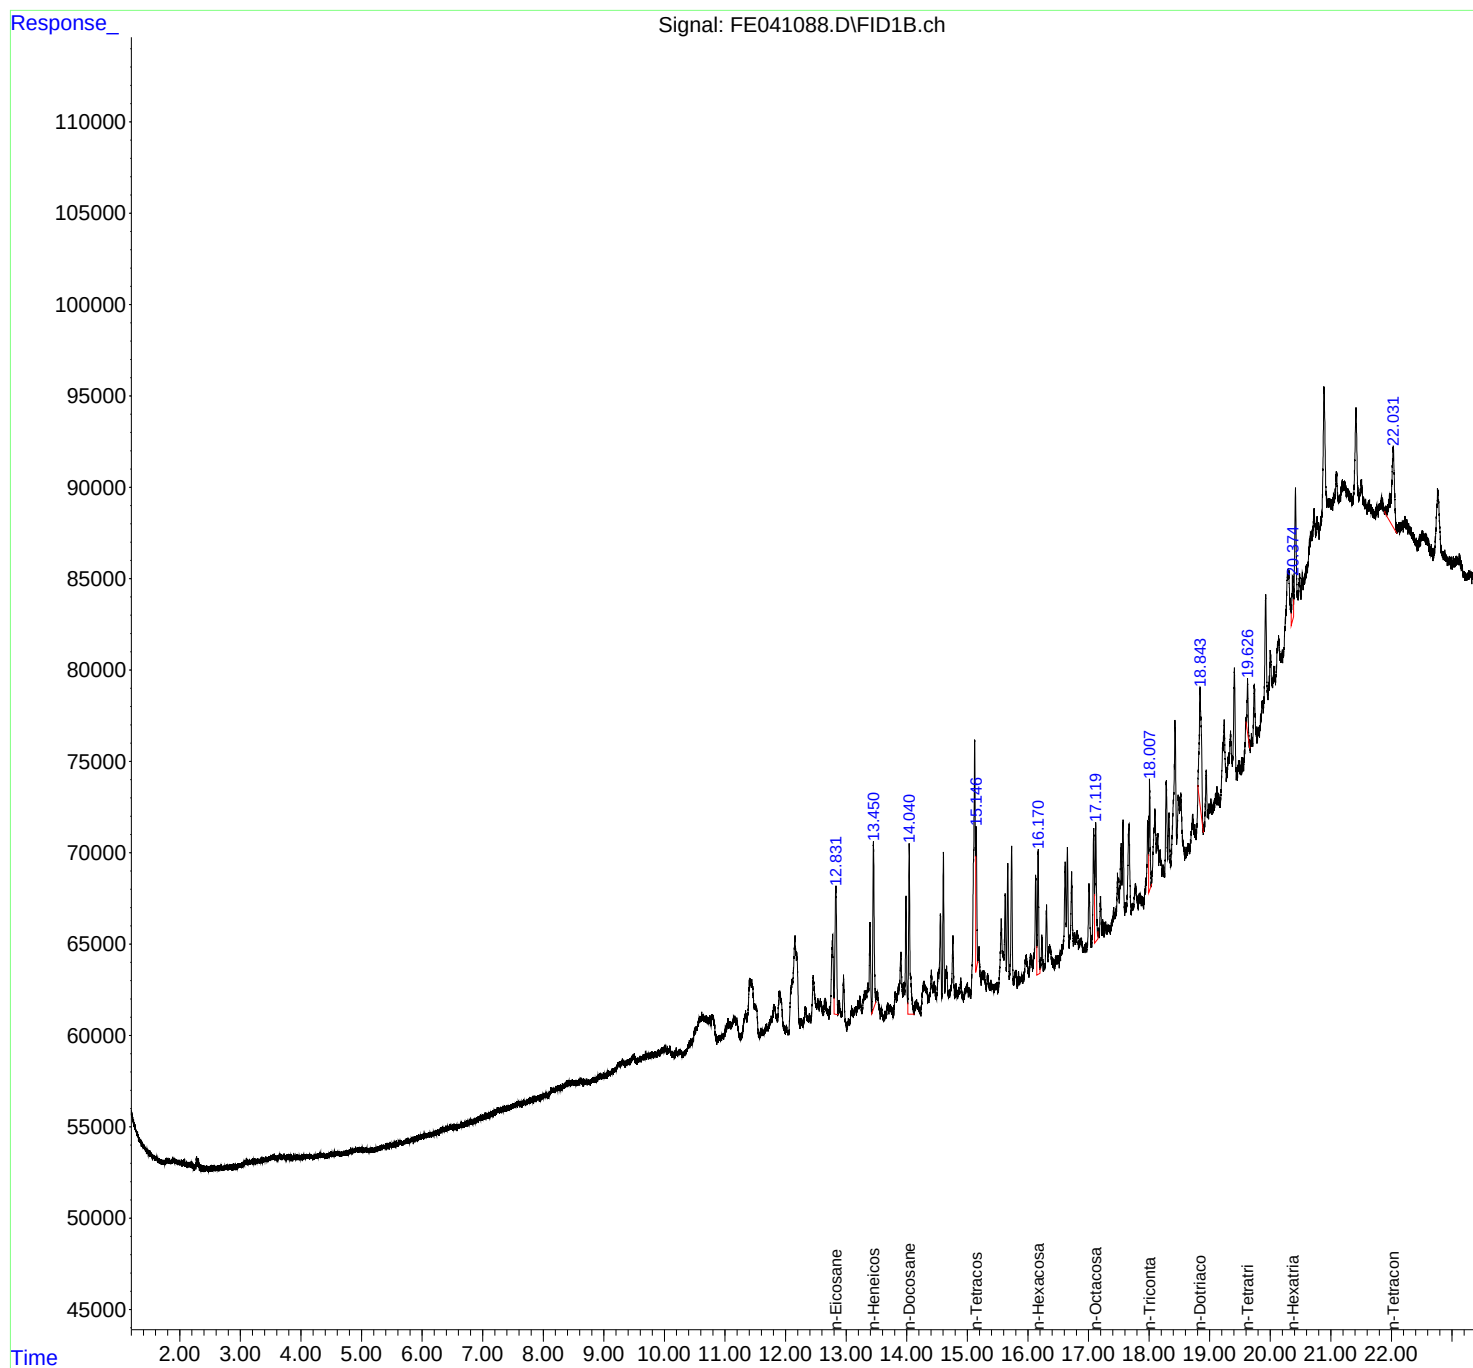


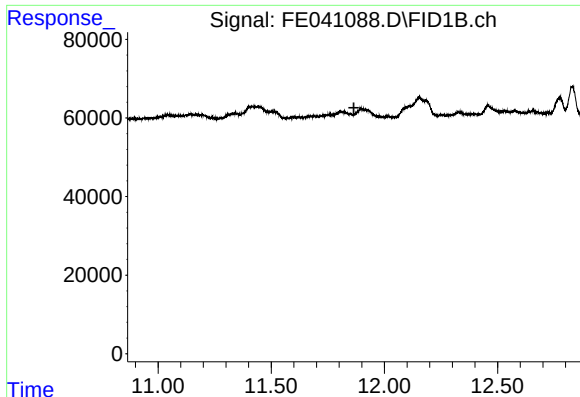

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

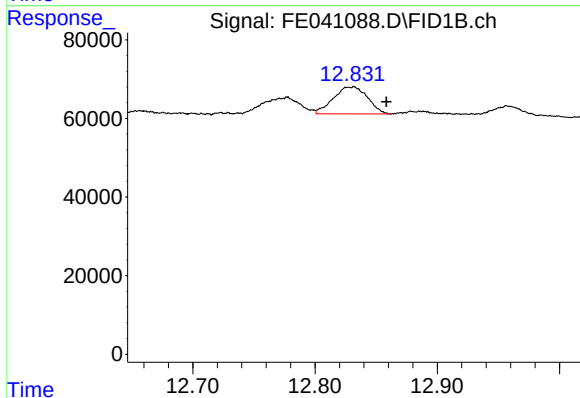


#10 n-Eicosane (C20)

R.T.: 12.832 min
Delta R.T.: -0.027 min
Response: 134079
Conc: 0.79 ug/ml

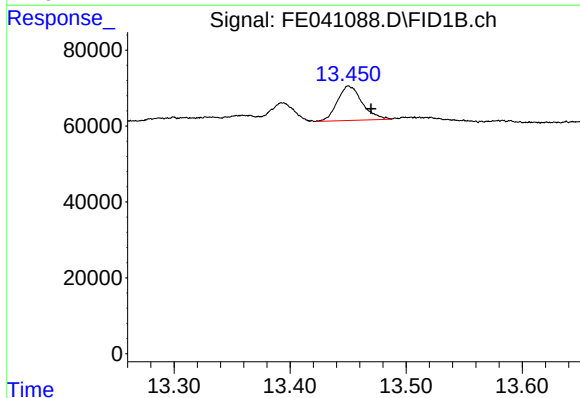


#11 n-Heneicosane (C21)

R.T.: 13.450 min
Delta R.T.: -0.020 min
Response: 135234
Conc: 0.80 ug/ml

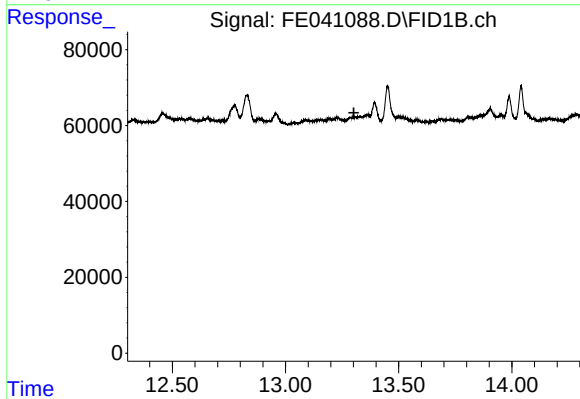

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

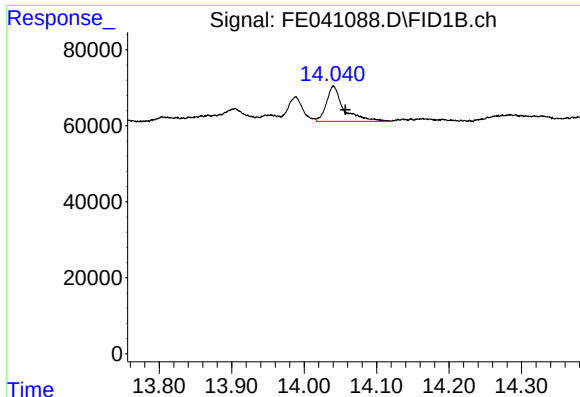

#13 n-Docosane (C22)


R.T.: 14.040 min
Delta R.T.: -0.017 min
Response: 153453
Conc: 0.93 ug/ml

Instrument :
FID_E
ClientSampleId :

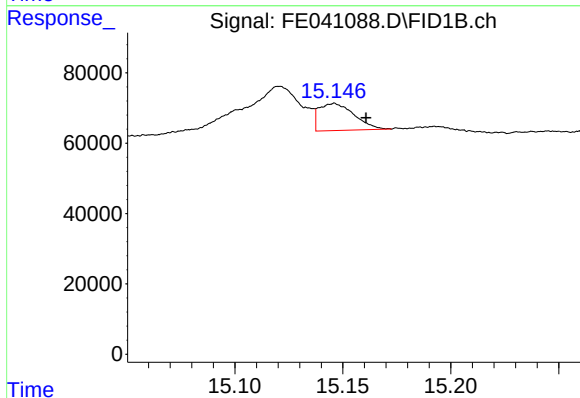


#14 n-Tetracosane (C24)

R.T.: 15.146 min
Delta R.T.: -0.015 min
Response: 87503
Conc: 0.54 ug/ml

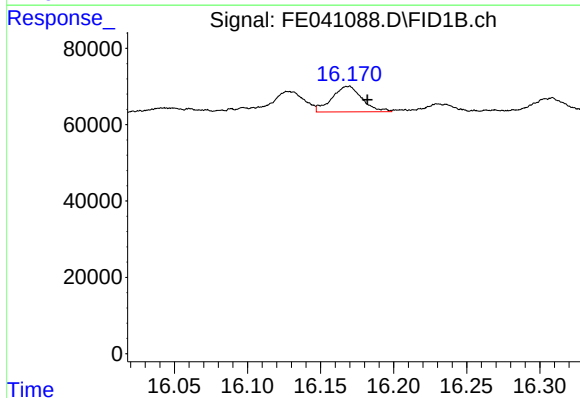


#15 n-Hexacosane (C26)

R.T.: 16.169 min
Delta R.T.: -0.013 min
Response: 96474
Conc: 0.62 ug/ml

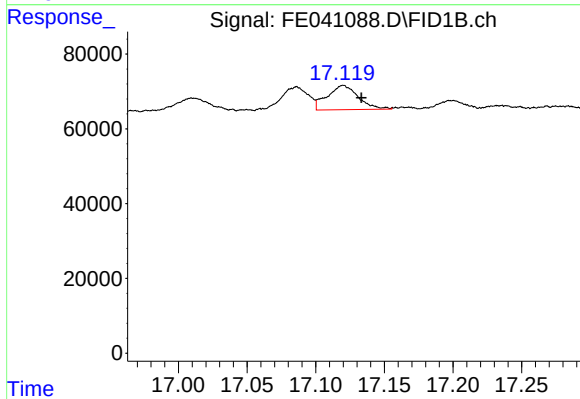

#16 n-Octacosane (C28)


R.T.: 17.120 min
Delta R.T.: -0.013 min
Response: 101825
Conc: 0.66 ug/ml

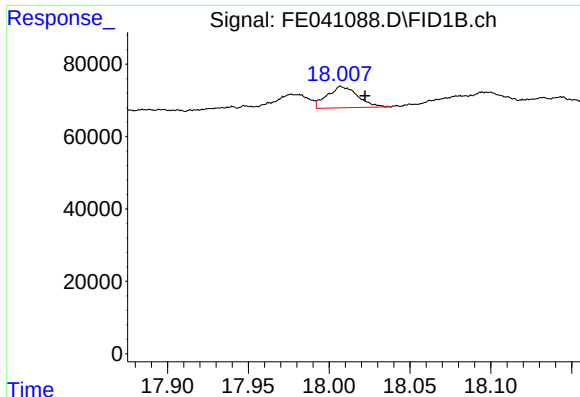

#17 n-Tricontane (C30)


R.T.: 18.008 min
Delta R.T.: -0.015 min
Response: 77525
Conc: 0.51 ug/ml

Instrument :
FID_E
ClientSampleId :

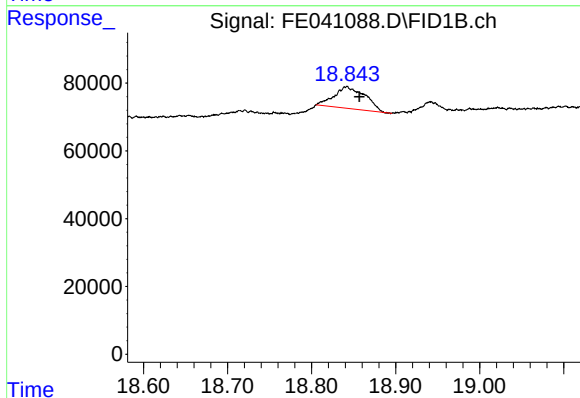


#18 n-Dotriacontane (C32)

R.T.: 18.842 min
Delta R.T.: -0.015 min
Response: 164818
Conc: 1.06 ug/ml

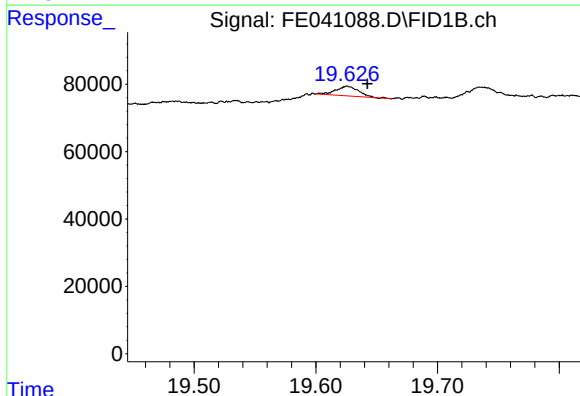


#19 n-Tetratriacontane (C34)

R.T.: 19.626 min
Delta R.T.: -0.017 min
Response: 37358
Conc: 0.24 ug/ml

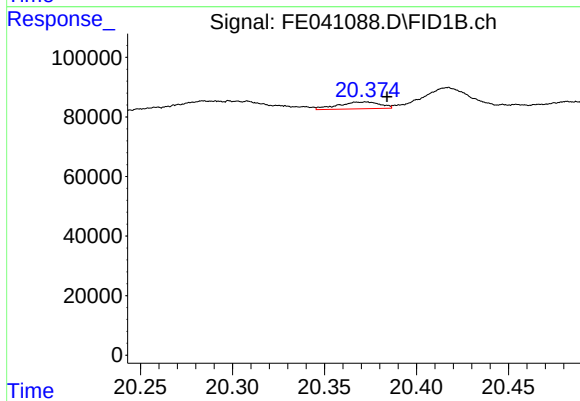

#20 n-Hexatriacontane (C36)

R.T.: 20.371 min
Delta R.T.: -0.013 min
Response: 37188
Conc: 0.24 ug/ml

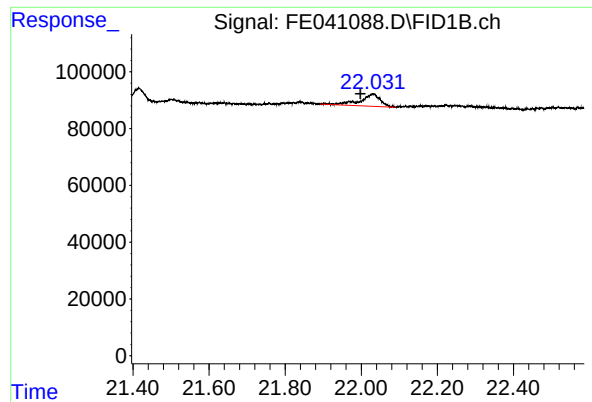

#22 n-Tetracontane (C40)

R.T.: 22.031 min
Delta R.T.: 0.033 min
Response: 162530
Conc: 1.02 ug/ml

Instrument :

FID_E

ClientSampleId :