

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE033123AL\
 Data File : FE041113.D
 Signal(s) : FID1B.ch
 Acq On : 31 Mar 2023 20:58
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 01 01:21:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) T n-Hexacosane (C26)	16.179	411	0.003 ug/ml
17) T n-Tricontane (C30)	18.018	40754	0.267 ug/ml
18) T n-Dotriacontane (C32)	18.852	137094	0.878 ug/ml
19) T n-Tetratriacontane (C34)	19.636	53530	0.345 ug/ml
20) T n-Hexatriacontane (C36)	20.374	252252	1.661 ug/ml
22) T n-Tetracontane (C40)	21.969	572600	3.588 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE033123AL\
Data File : FE041113.D
Signal(s) : FID1B.ch
Acq On : 31 Mar 2023 20:58
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 01 01:21:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

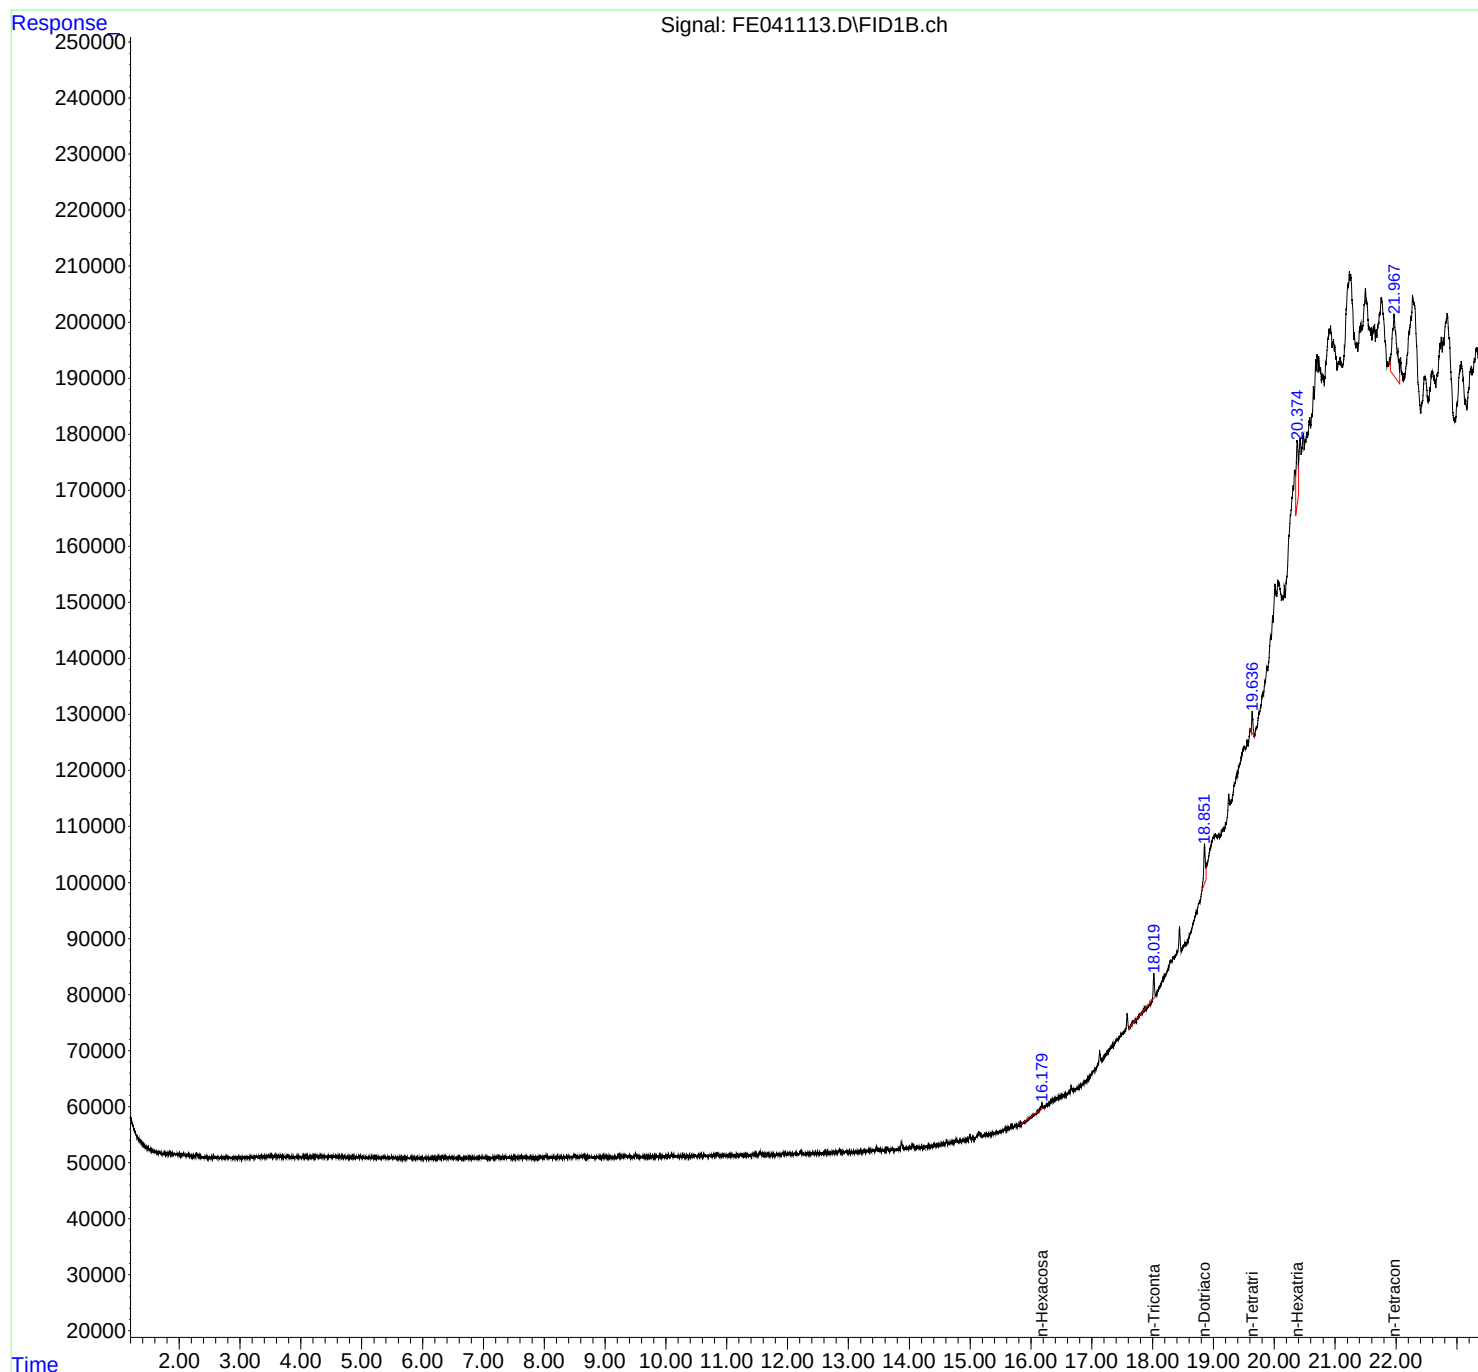


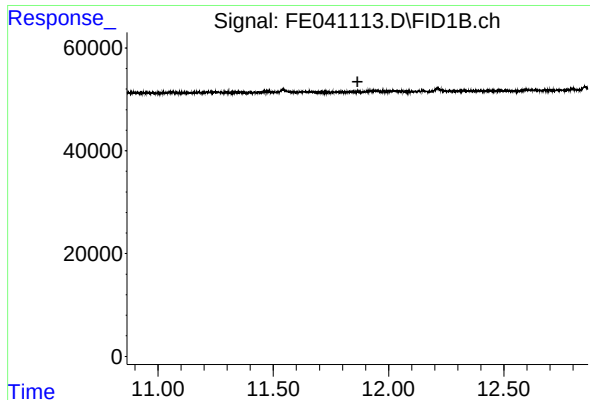

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

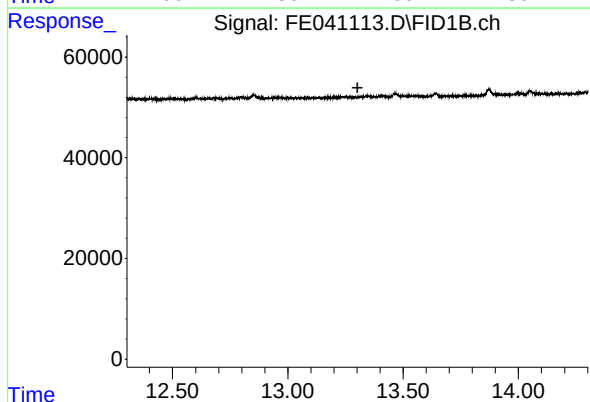


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

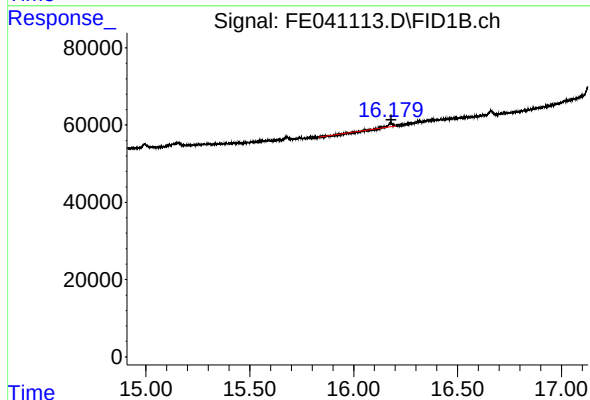


#15 n-Hexacosane (C26)

R.T.: 16.179 min
Delta R.T.: -0.003 min
Response: 411
Conc: 0.00 ug/ml

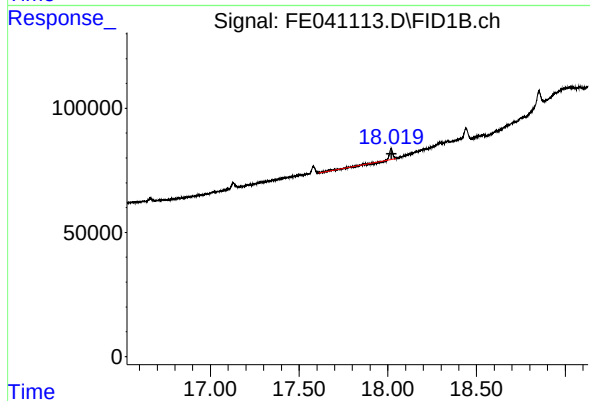

#17 n-Tricontane (C30)


R.T.: 18.018 min
Delta R.T.: -0.004 min
Response: 40754
Conc: 0.27 ug/ml

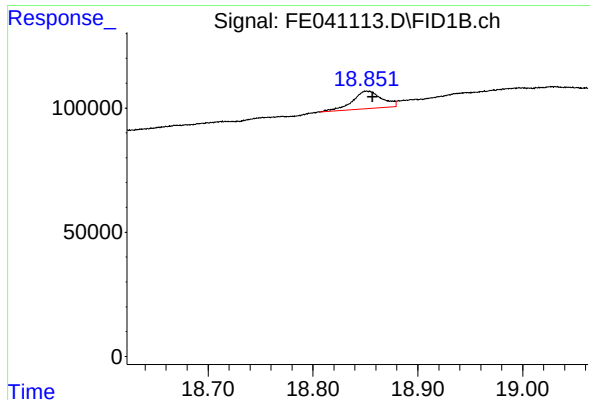

#18 n-Dotriacontane (C32)


R.T.: 18.852 min
Delta R.T.: -0.005 min
Response: 137094
Conc: 0.88 ug/ml

Instrument :
FID_E
ClientSampleId :

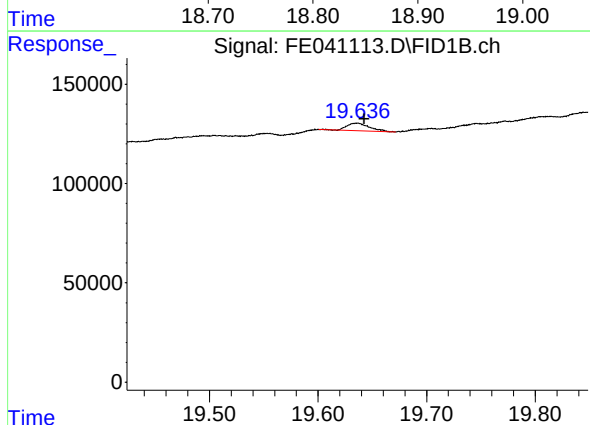


#19 n-Tetratriacontane (C34)

R.T.: 19.636 min
Delta R.T.: -0.006 min
Response: 53530
Conc: 0.35 ug/ml

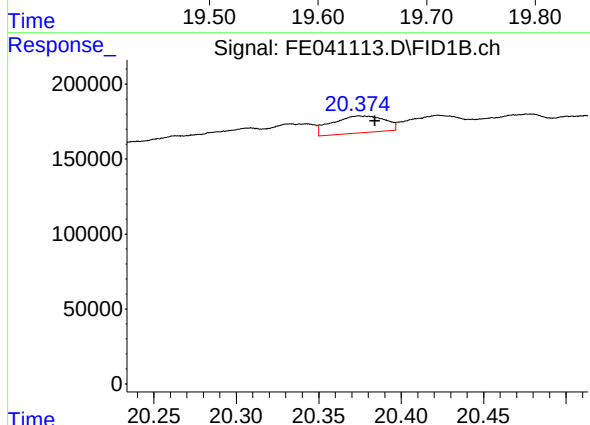

#20 n-Hexatriacontane (C36)

R.T.: 20.374 min
Delta R.T.: -0.010 min
Response: 252252
Conc: 1.66 ug/ml

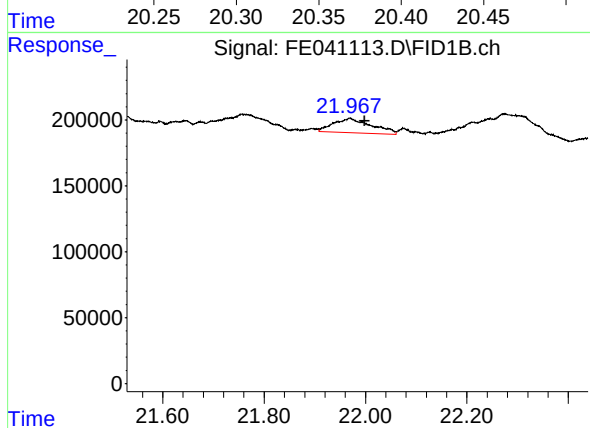

#22 n-Tetracontane (C40)

R.T.: 21.969 min
Delta R.T.: -0.029 min
Response: 572600
Conc: 3.59 ug/ml