

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031616.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 16:00
 Operator : DD\AJ
 Sample : L2089-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:32:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.389	7905456	21.419 ug/ml
Target Compounds			
4) N-TETRADECANE	8.008	2251556	5.414 ug/ml
7) N-EICOSANE	12.350	366795	0.858 ug/ml
11) N-HEXACOSANE	15.607	285241	0.679 ug/ml
12) N-OCTACOSANE	16.558	814607	1.941 ug/ml
13) N-TRIACONTANE	17.443	918757	2.199 ug/ml
14) N-DOTRIACONTANE	18.276	519134	1.310 ug/ml
17) N-OCTATRIACONTANE	20.503	333557	1.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031616.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 16:00
Operator : DD\AJ
Sample : L2089-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:32:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

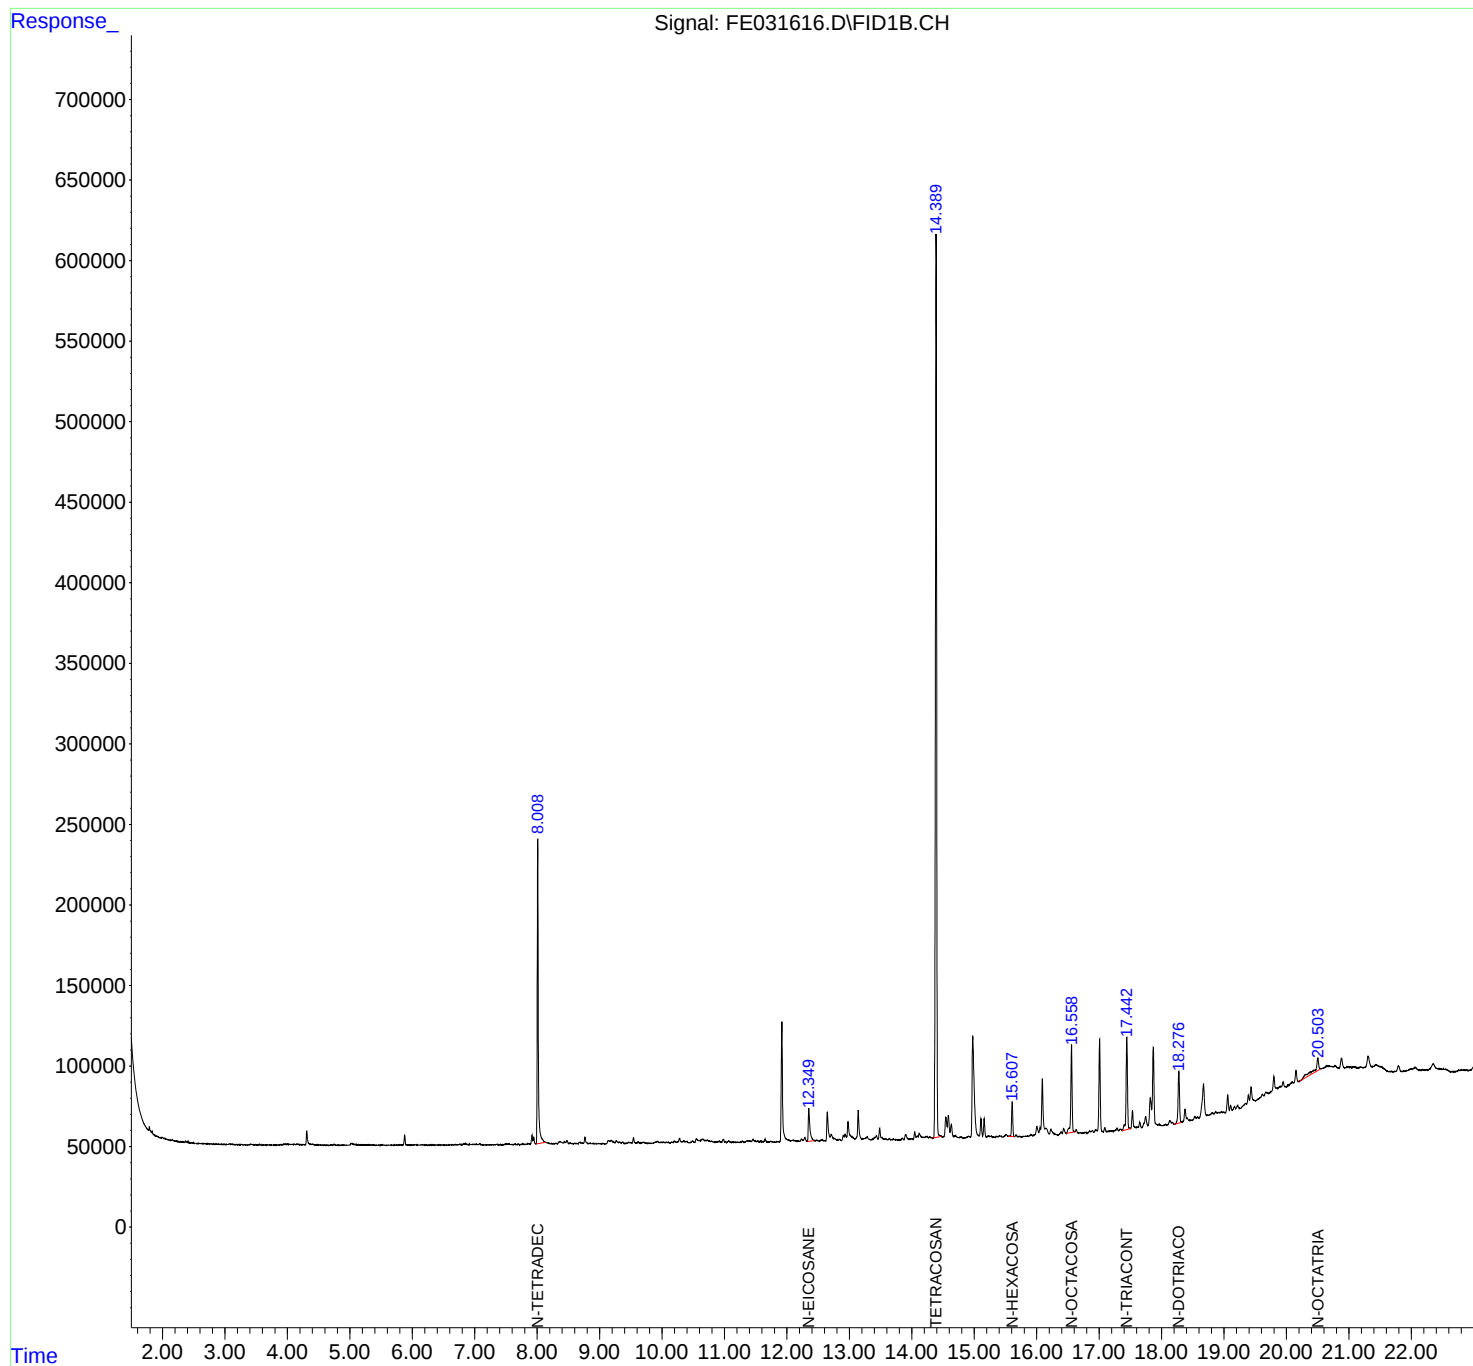


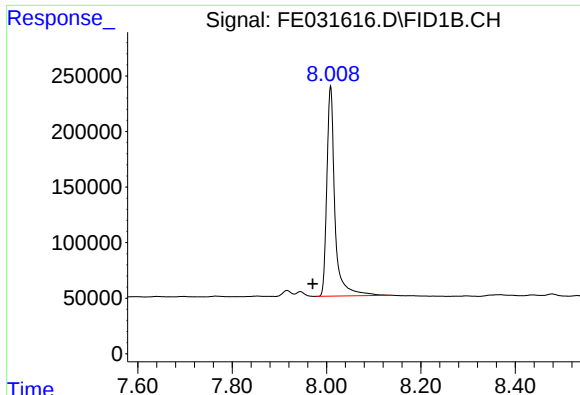

#4 N-TETRADECANE


R.T.: 8.008 min
Delta R.T.: 0.038 min
Response: 2251556
Conc: 5.41 ug/ml

Instrument :
FID_E
ClientSampleId :

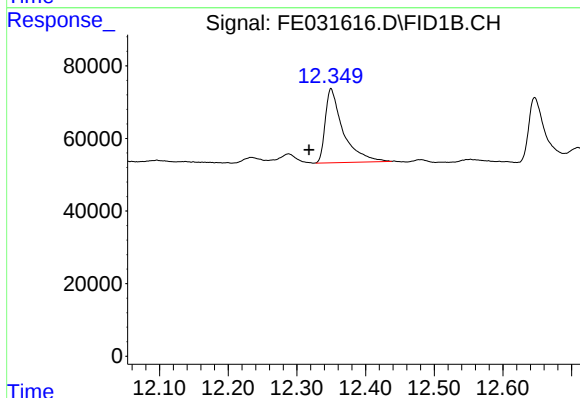


#7 N-EICOSANE

R.T.: 12.350 min
Delta R.T.: 0.033 min
Response: 366795
Conc: 0.86 ug/ml

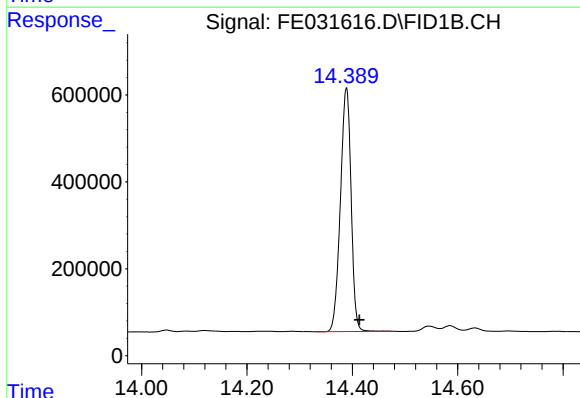


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.389 min
Delta R.T.: -0.025 min
Response: 7905456
Conc: 21.42 ug/ml

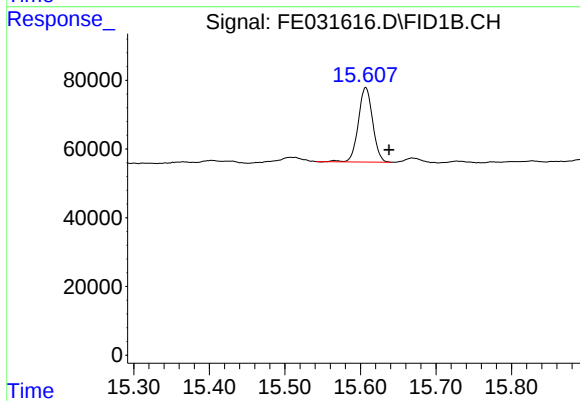

#11 N-HEXACOSANE


R.T.: 15.607 min
Delta R.T.: -0.031 min
Response: 285241
Conc: 0.68 ug/ml

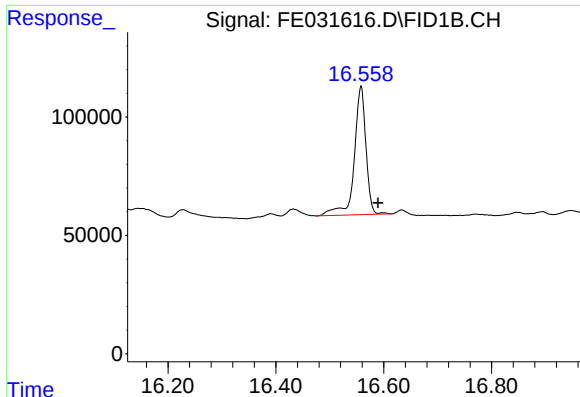

#12 N-OCTACOSANE


R.T.: 16.558 min
Delta R.T.: -0.032 min
Response: 814607
Conc: 1.94 ug/ml

Instrument :
FID_E
ClientSampleId :

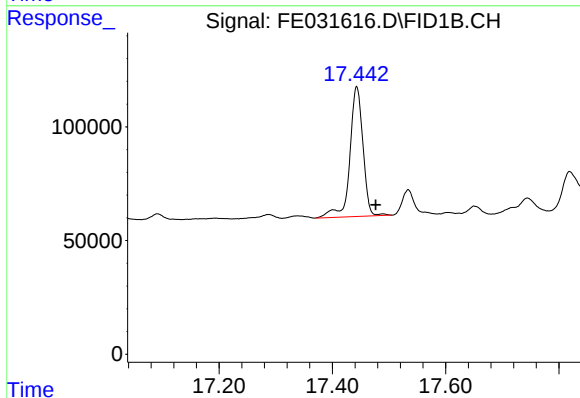


#13 N-TRIACONTANE

R.T.: 17.443 min
Delta R.T.: -0.033 min
Response: 918757
Conc: 2.20 ug/ml

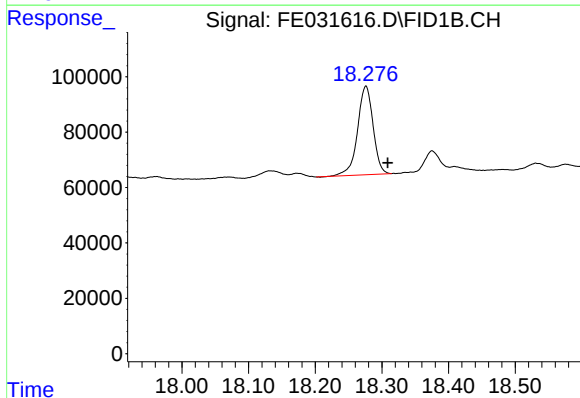

#14 N-DOTRIACONTANE

R.T.: 18.276 min
Delta R.T.: -0.033 min
Response: 519134
Conc: 1.31 ug/ml

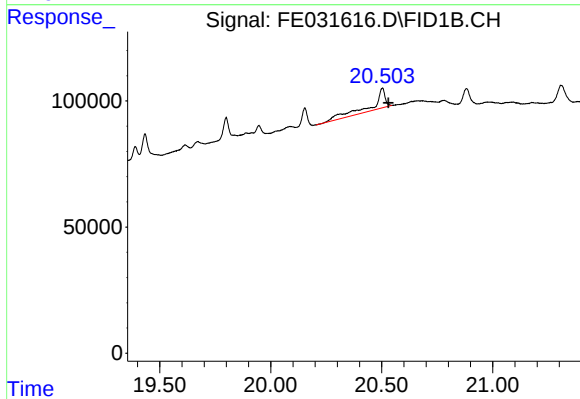

#17 N-OCTATRIACONTANE

R.T.: 20.503 min
Delta R.T.: -0.027 min
Response: 333557
Conc: 1.47 ug/ml