

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031620.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 18:13
 Operator : DD\AJ
 Sample : L2100-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:33:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.389	6290440	17.044 ug/ml
Target Compounds			
4) N-TETRADECANE	8.010	2756223	6.627 ug/ml
7) N-EICOSANE	12.347	770648	1.803 ug/ml
10) N-TETRACOSANE	14.577	432159	1.015 ug/ml
11) N-HEXACOSANE	15.607	256075	0.610 ug/ml
12) N-OCTACOSANE	16.595	285787	0.681 ug/ml
13) N-TRIACONTANE	17.442	700742	1.677 ug/ml
14) N-DOTRIACONTANE	18.273	667392	1.684 ug/ml
15) N-TETRATRIACONTANE	19.097	235711	0.682 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031620.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 18:13
Operator : DD\AJ
Sample : L2100-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:33:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

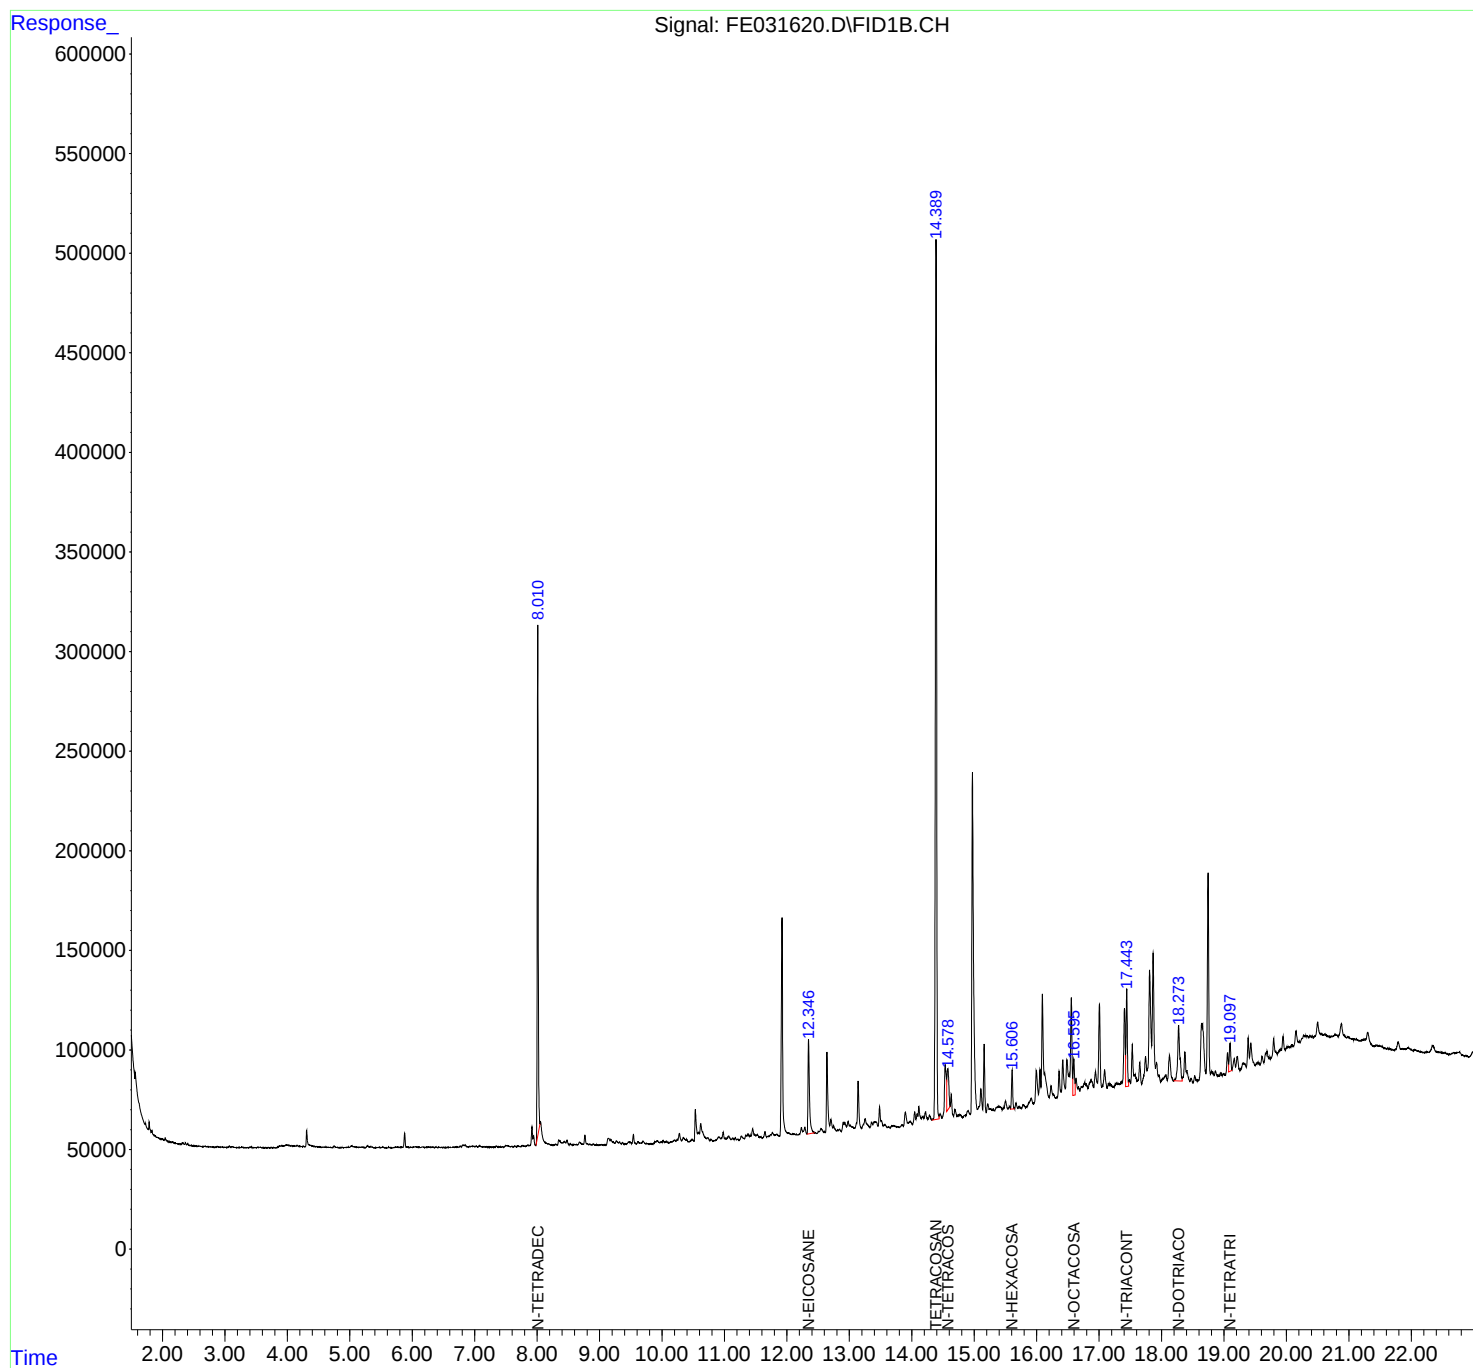


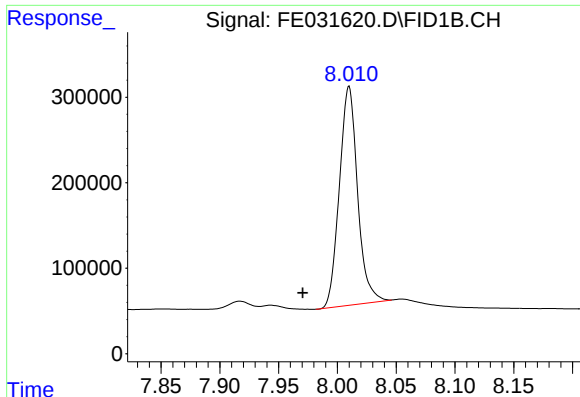

#4 N-TETRADECANE


R.T.: 8.010 min
Delta R.T.: 0.039 min
Response: 2756223
Conc: 6.63 ug/ml

Instrument :
FID_E
ClientSampleId :

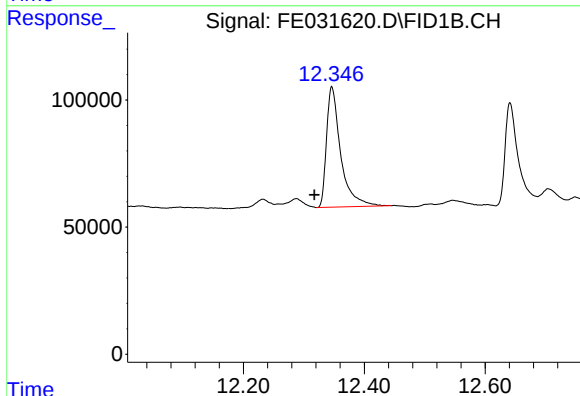


#7 N-EICOSANE

R.T.: 12.347 min
Delta R.T.: 0.029 min
Response: 770648
Conc: 1.80 ug/ml

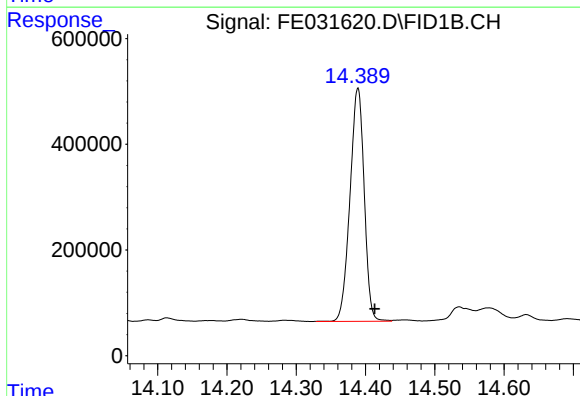


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.389 min
Delta R.T.: -0.025 min
Response: 6290440
Conc: 17.04 ug/ml

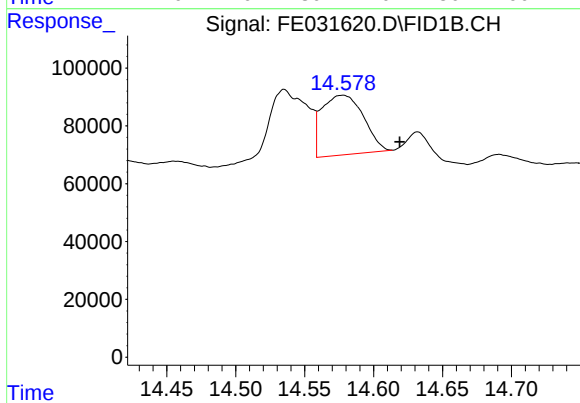

#10 N-TETRACOSANE


R.T.: 14.577 min
Delta R.T.: -0.042 min
Response: 432159
Conc: 1.01 ug/ml

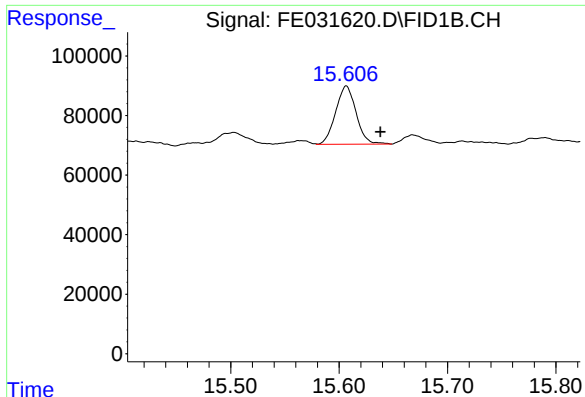

#11 N-HEXACOSANE


R.T.: 15.607 min
Delta R.T.: -0.031 min
Response: 256075
Conc: 0.61 ug/ml

Instrument :
FID_E
ClientSampleId :

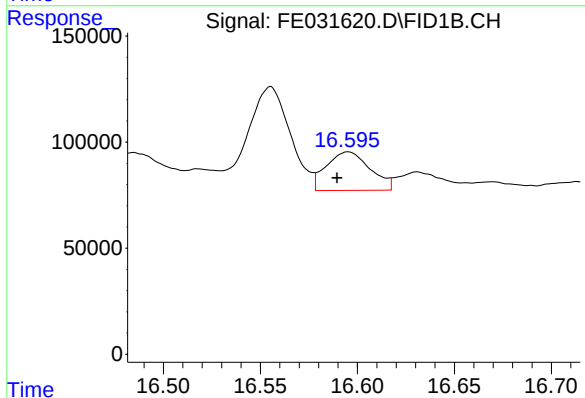


#12 N-OCTACOSANE

R.T.: 16.595 min
Delta R.T.: 0.006 min
Response: 285787
Conc: 0.68 ug/ml

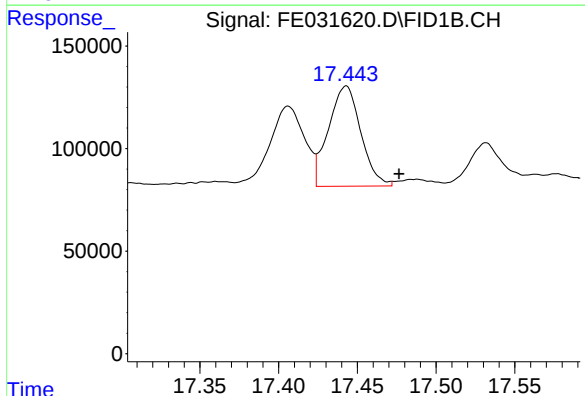


#13 N-TRIACONTANE

R.T.: 17.442 min
Delta R.T.: -0.034 min
Response: 700742
Conc: 1.68 ug/ml

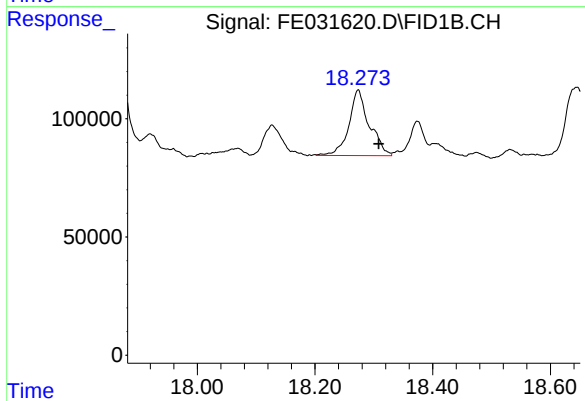

#14 N-DOTRIACONTANE

R.T.: 18.273 min
Delta R.T.: -0.035 min
Response: 667392
Conc: 1.68 ug/ml

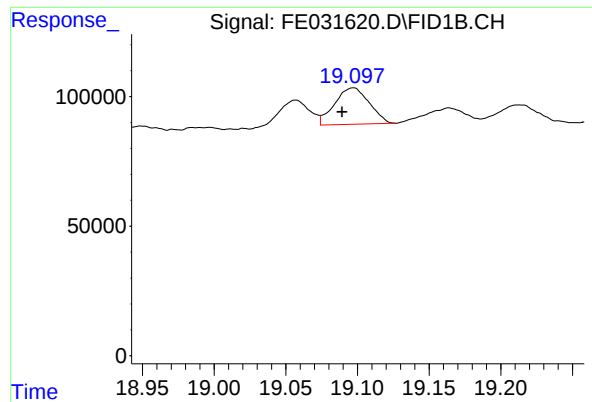

#15 N-TETRATRIACONTANE

R.T.: 19.097 min

Delta R.T.: 0.007 min

Response: 235711

Conc: 0.68 ug/ml

Instrument :
FID_E
ClientSampleId :