

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031621.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 18:46
 Operator : DD\AJ
 Sample : L2100-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:33:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.388	5528069	14.978 ug/ml
Target Compounds			
4) N-TETRADECANE	8.009	2079557	5.000 ug/ml
7) N-EICOSANE	12.346	742483	1.737 ug/ml
10) N-TETRACOSANE	14.576	415159	0.975 ug/ml
11) N-HEXACOSANE	15.606	196865	0.469 ug/ml
12) N-OCTACOSANE	16.558	1019649	2.430 ug/ml
13) N-TRIACONTANE	17.441	531331	1.271 ug/ml
14) N-DOTRIACONTANE	18.273	556631	1.405 ug/ml
15) N-TETRATRIACONTANE	19.098	201597	0.583 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031621.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 18:46
Operator : DD\AJ
Sample : L2100-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:33:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

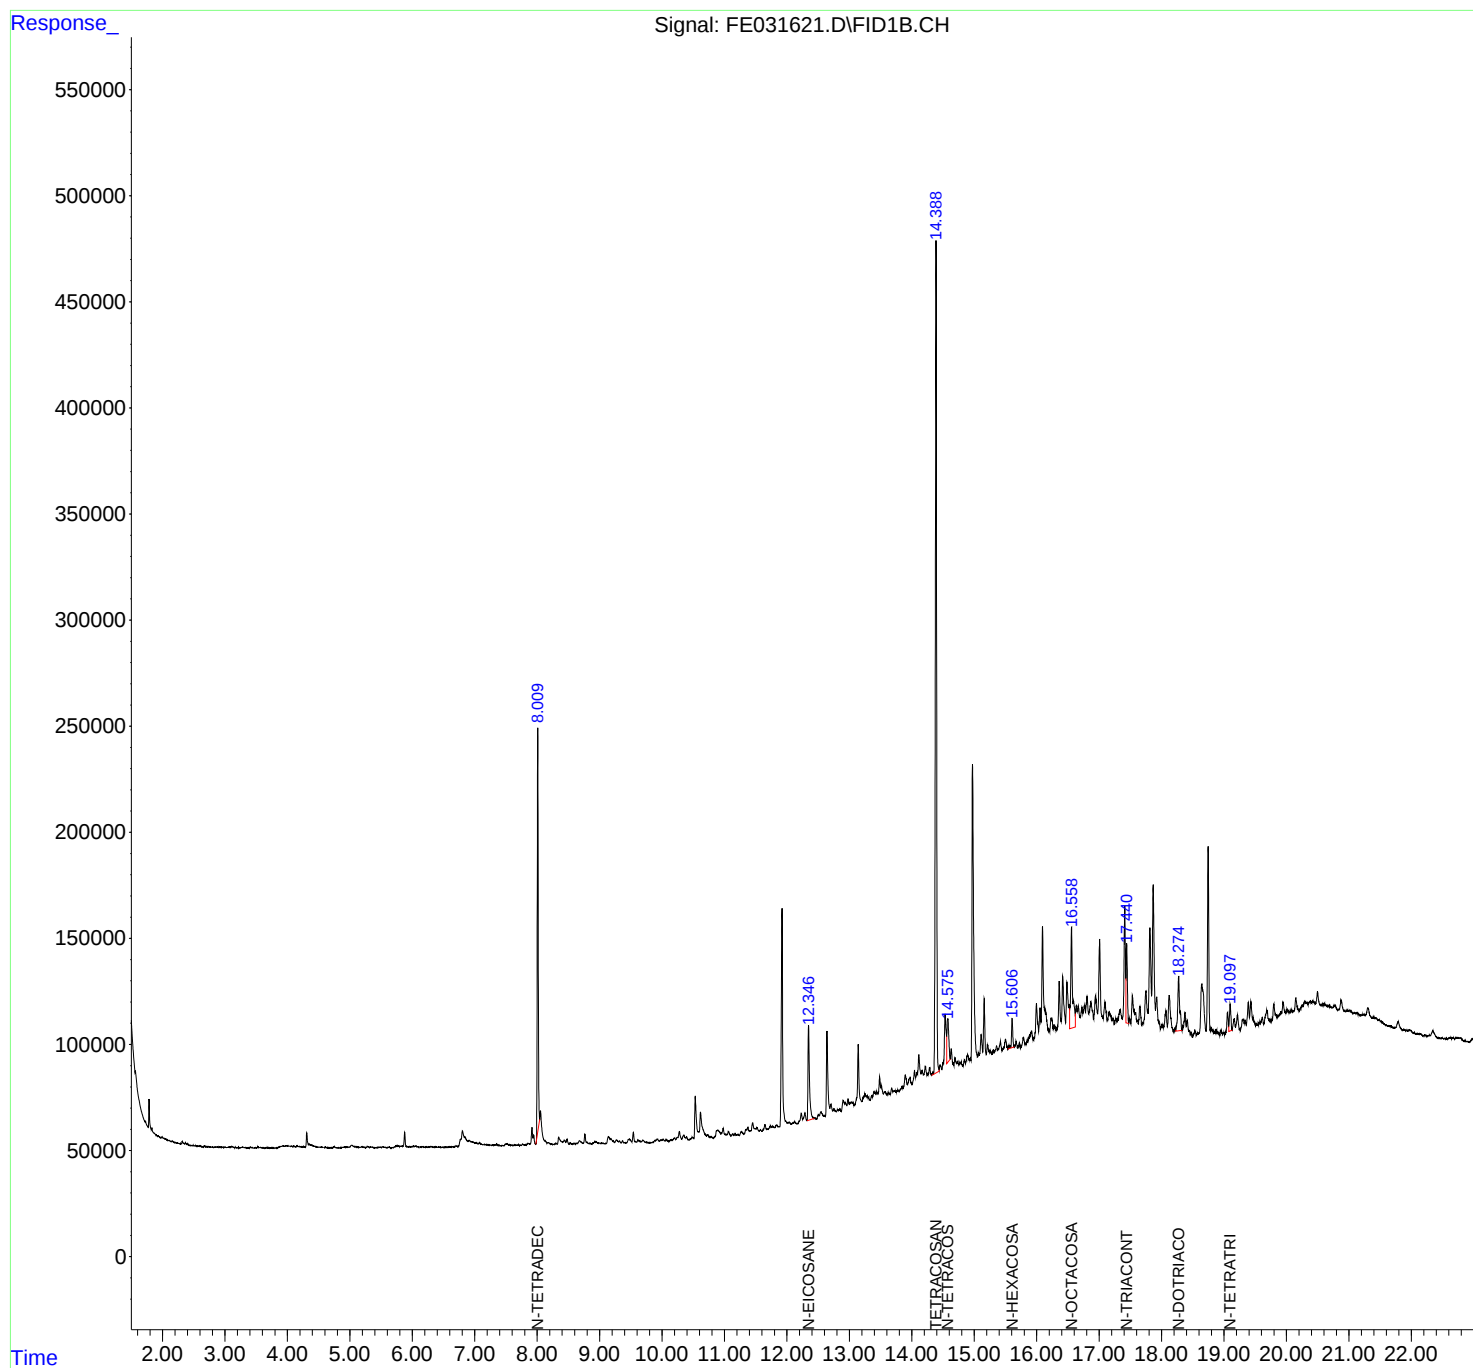


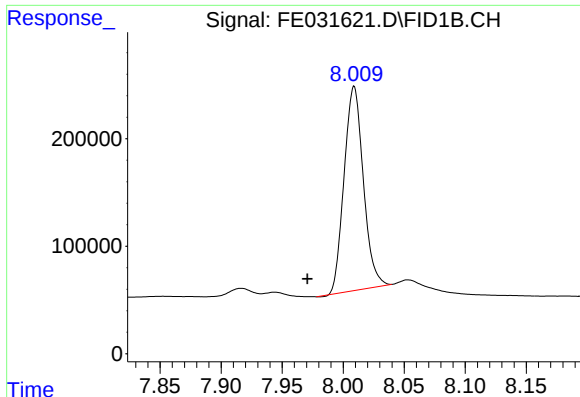

#4 N-TETRADECANE


R.T.: 8.009 min
Delta R.T.: 0.038 min
Response: 2079557
Conc: 5.00 ug/ml

Instrument :
FID_E
ClientSampleId :

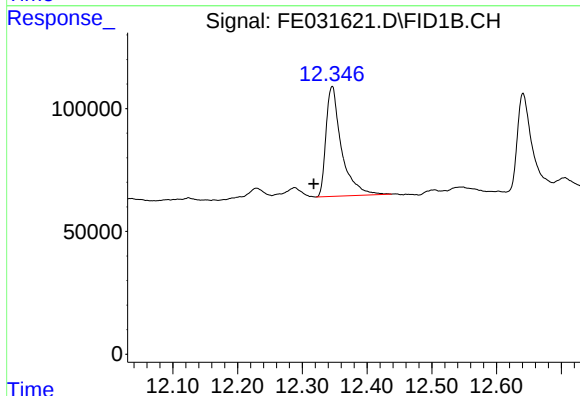


#7 N-EICOSANE

R.T.: 12.346 min
Delta R.T.: 0.028 min
Response: 742483
Conc: 1.74 ug/ml

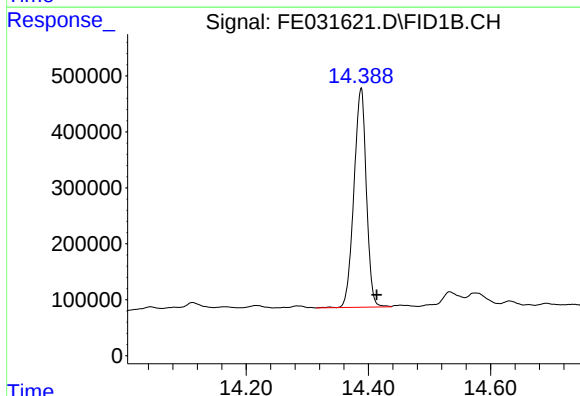


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.388 min
Delta R.T.: -0.026 min
Response: 5528069
Conc: 14.98 ug/ml

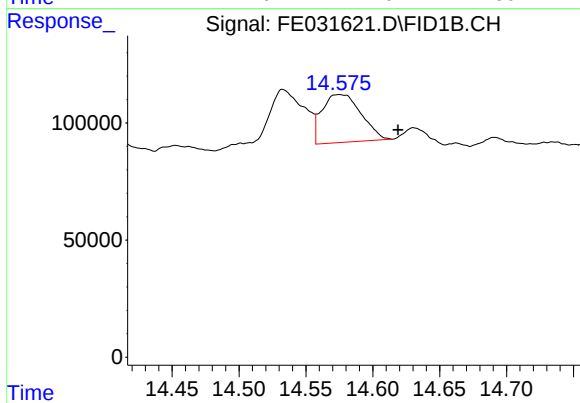

#10 N-TETRACOSANE


R.T.: 14.576 min
Delta R.T.: -0.043 min
Response: 415159
Conc: 0.97 ug/ml

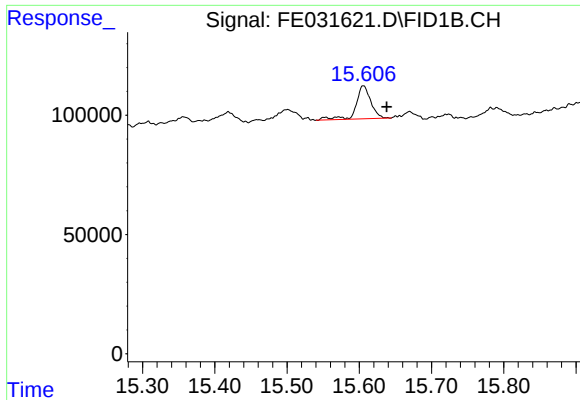

#11 N-HEXACOSANE


R.T.: 15.606 min
Delta R.T.: -0.032 min
Response: 196865
Conc: 0.47 ug/ml

Instrument :
FID_E
ClientSampleId :

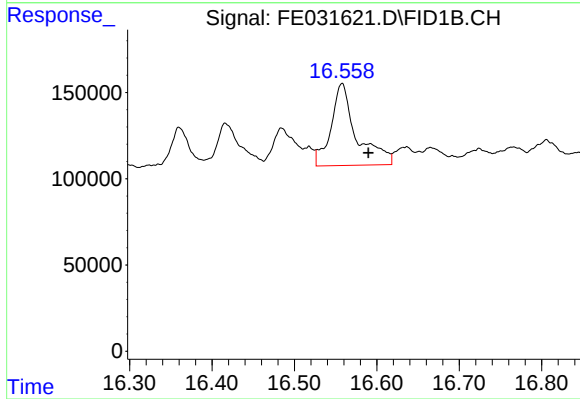


#12 N-OCTACOSANE

R.T.: 16.558 min
Delta R.T.: -0.032 min
Response: 1019649
Conc: 2.43 ug/ml

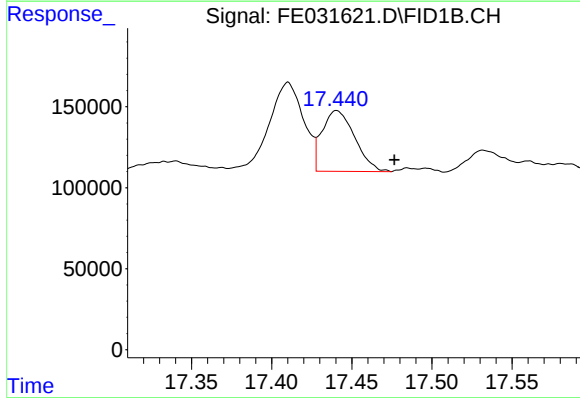


#13 N-TRIACONTANE

R.T.: 17.441 min
Delta R.T.: -0.036 min
Response: 531331
Conc: 1.27 ug/ml

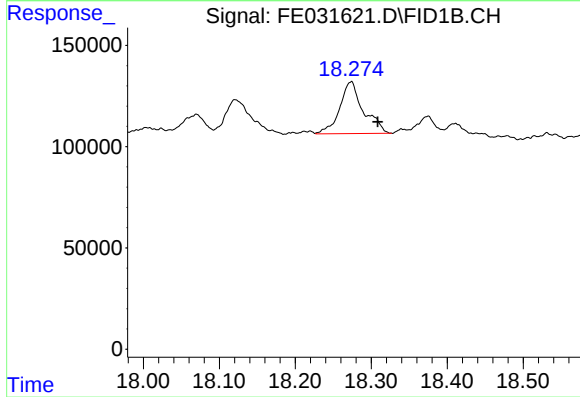

#14 N-DOTRIACONTANE

R.T.: 18.273 min
Delta R.T.: -0.036 min
Response: 556631
Conc: 1.40 ug/ml

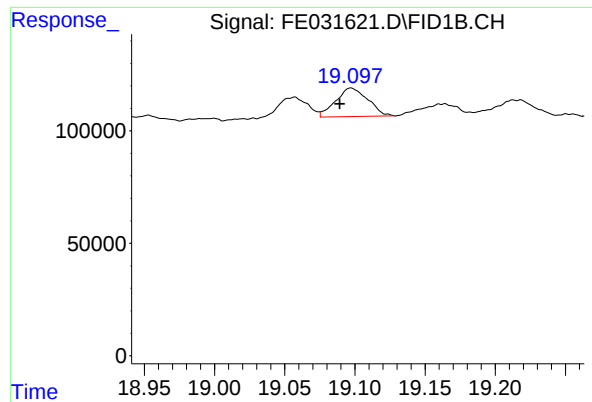

#15 N-TETRATRIACONTANE

R.T.: 19.098 min

Delta R.T.: 0.008 min

Response: 201597

Conc: 0.58 ug/ml

Instrument :
FID_E
ClientSampleId :