

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031622.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 19:20
 Operator : DD\AJ
 Sample : L2101-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:33:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.388	6102137	16.533 ug/ml
Target Compounds			
4) N-TETRADECANE	8.008	1759271	4.230 ug/ml
7) N-EICOSANE	12.342	2908407	6.804 ug/ml
10) N-TETRACOSANE	14.566f	1446536	3.397 ug/ml
11) N-HEXACOSANE	15.607	184737	0.440 ug/ml
12) N-OCTACOSANE	16.555	751890	1.792 ug/ml
13) N-TRIACONTANE	17.441	629681	1.507 ug/ml
14) N-DOTRIACONTANE	18.273	690945	1.744 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031622.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 19:20
Operator : DD\AJ
Sample : L2101-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:33:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

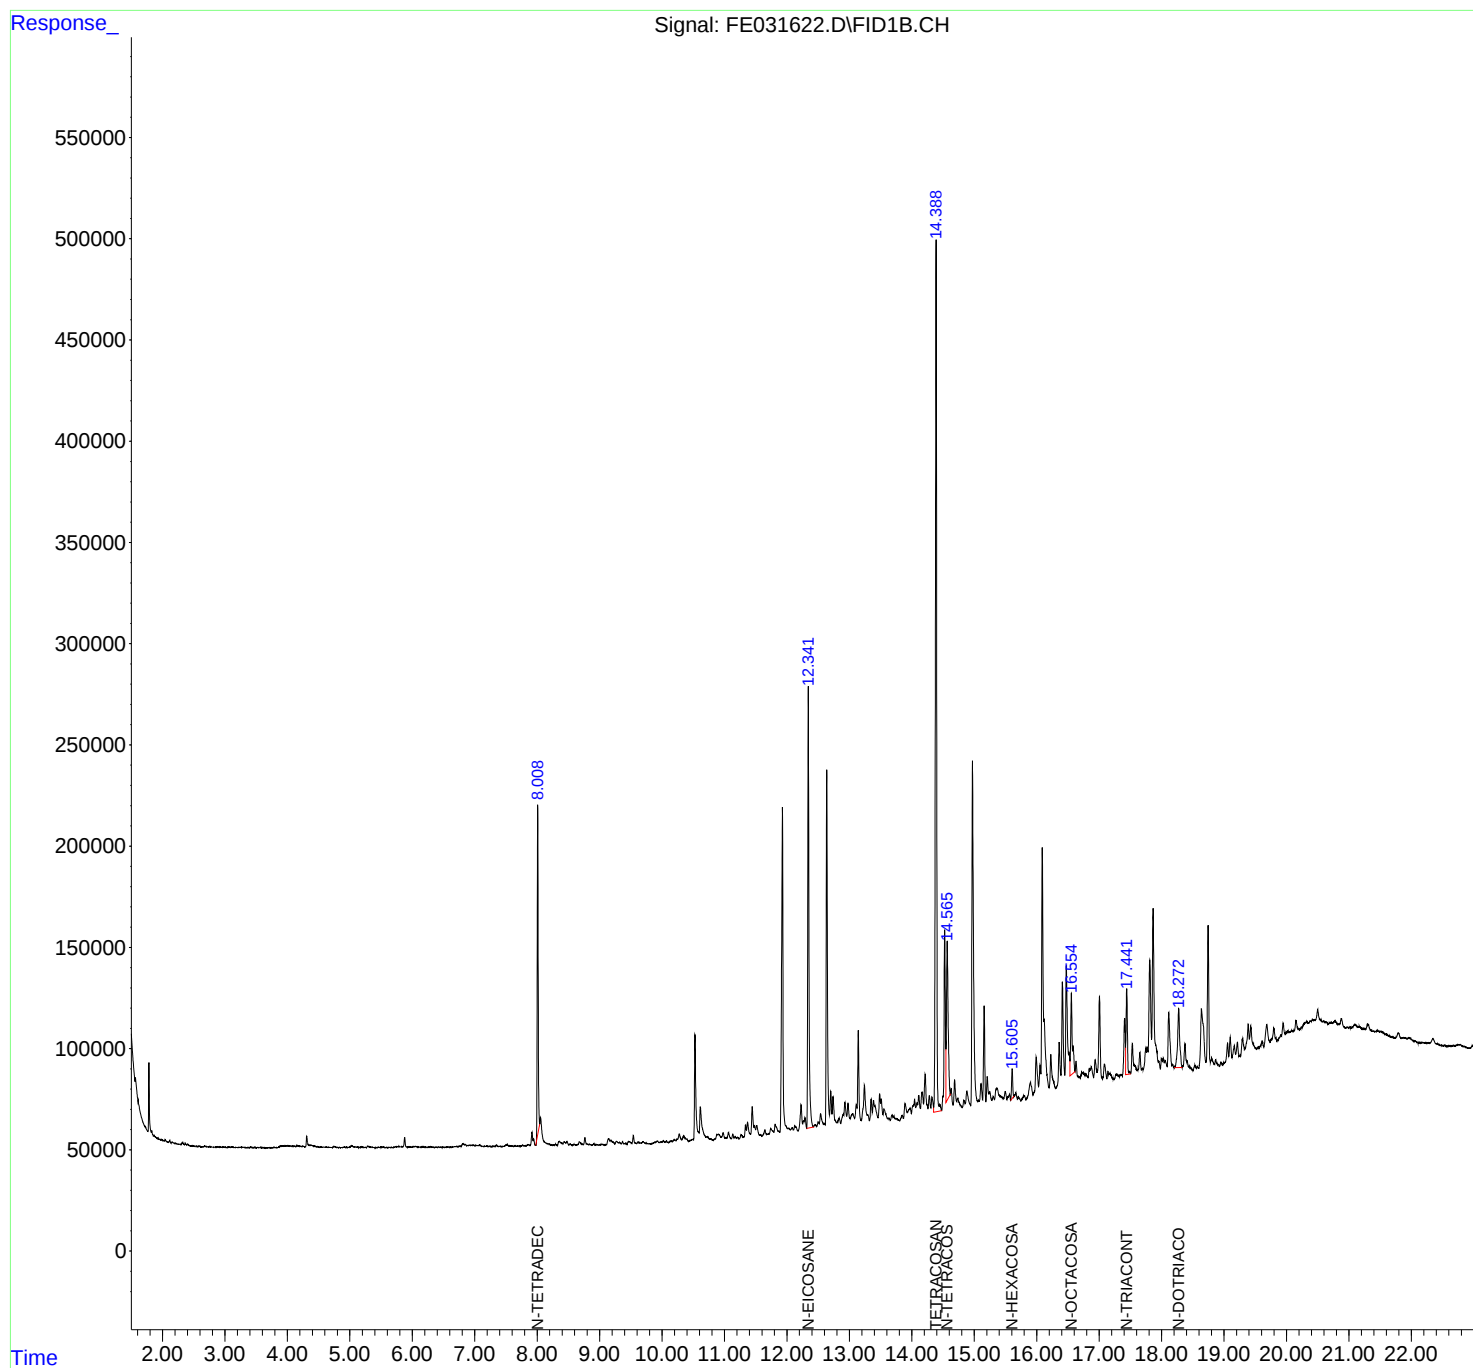


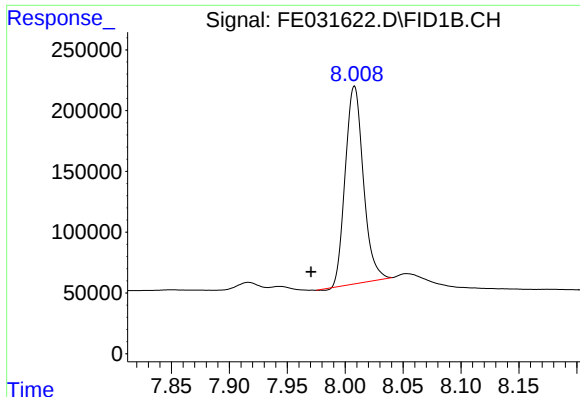

#4 N-TETRADECANE


R.T.: 8.008 min
Delta R.T.: 0.037 min
Response: 1759271
Conc: 4.23 ug/ml

Instrument :
FID_E
ClientSampleId :

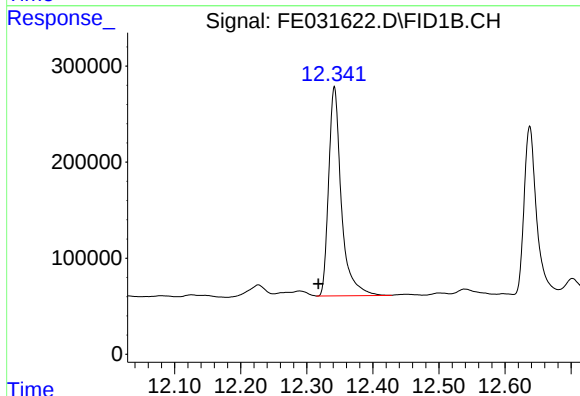


#7 N-EICOSANE

R.T.: 12.342 min
Delta R.T.: 0.024 min
Response: 2908407
Conc: 6.80 ug/ml

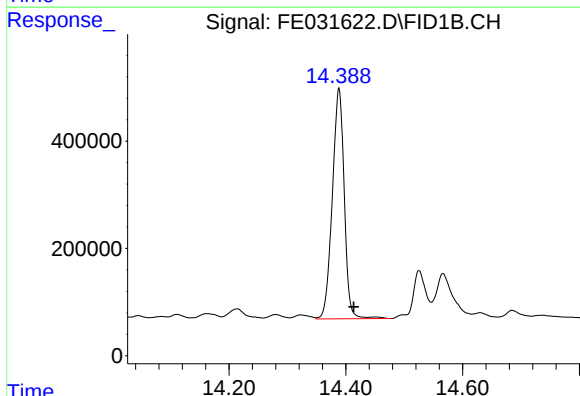


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.388 min
Delta R.T.: -0.025 min
Response: 6102137
Conc: 16.53 ug/ml

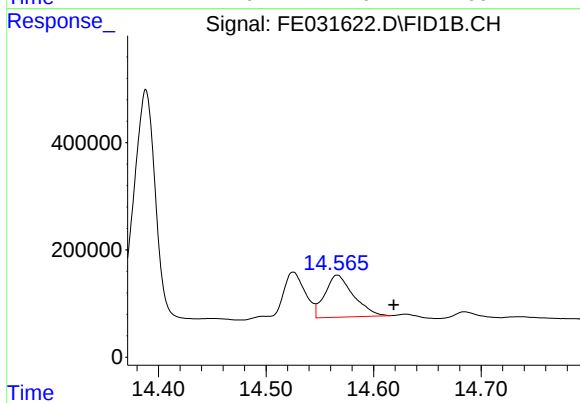

#10 N-TETRACOSANE


R.T.: 14.566 min
Delta R.T.: -0.052 min
Response: 1446536
Conc: 3.40 ug/ml

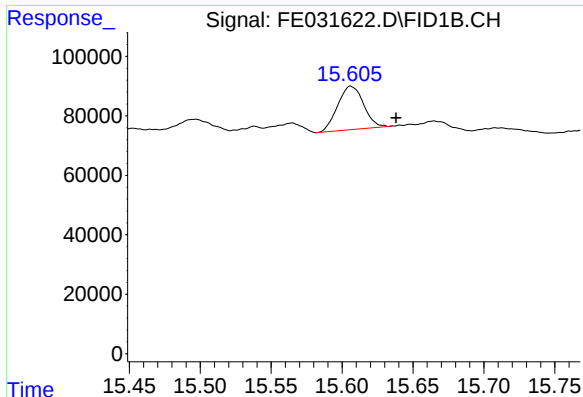

#11 N-HEXACOSANE


R.T.: 15.607 min
Delta R.T.: -0.032 min
Response: 184737
Conc: 0.44 ug/ml

Instrument :
FID_E
ClientSampleId :

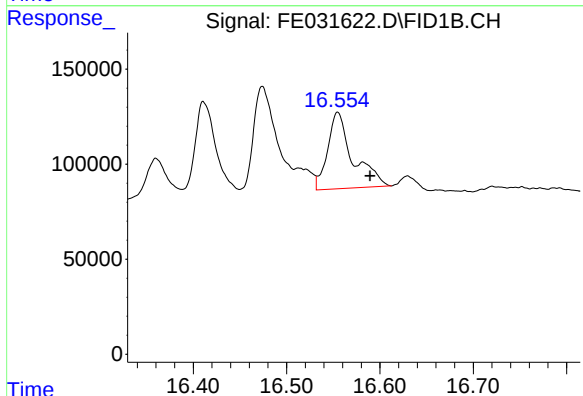


#12 N-OCTACOSANE

R.T.: 16.555 min
Delta R.T.: -0.035 min
Response: 751890
Conc: 1.79 ug/ml

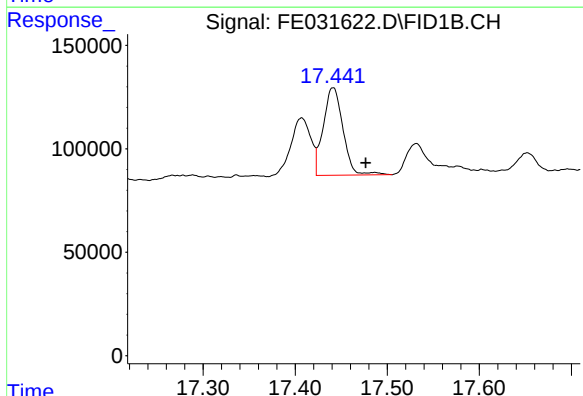

#13 N-TRIACONTANE

R.T.: 17.441 min
Delta R.T.: -0.035 min
Response: 629681
Conc: 1.51 ug/ml

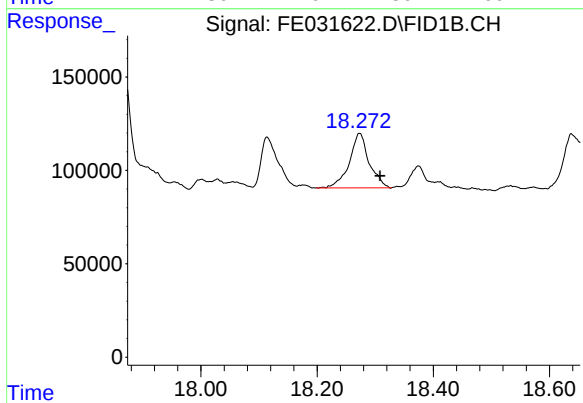

#14 N-DOTRIACONTANE

R.T.: 18.273 min
Delta R.T.: -0.035 min
Response: 690945
Conc: 1.74 ug/ml