

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031623.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 19:53
 Operator : DD\AJ
 Sample : L2101-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:33:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.389	6746453	18.279 ug/ml
Target Compounds			
4) N-TETRADECANE	8.007	1897077	4.562 ug/ml
7) N-EICOSANE	12.351	285219	0.667 ug/ml
8) N-DOCOSANE	13.484	224352	0.526 ug/ml
10) N-TETRACOSANE	14.585	349373	0.820 ug/ml
11) N-HEXACOSANE	15.608	403993	0.962 ug/ml
12) N-OCTACOSANE	16.556	810313	1.931 ug/ml
13) N-TRIACONTANE	17.443	742367	1.776 ug/ml
14) N-DOTRIACONTANE	18.272	657030	1.658 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031623.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 19:53
Operator : DD\AJ
Sample : L2101-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:33:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

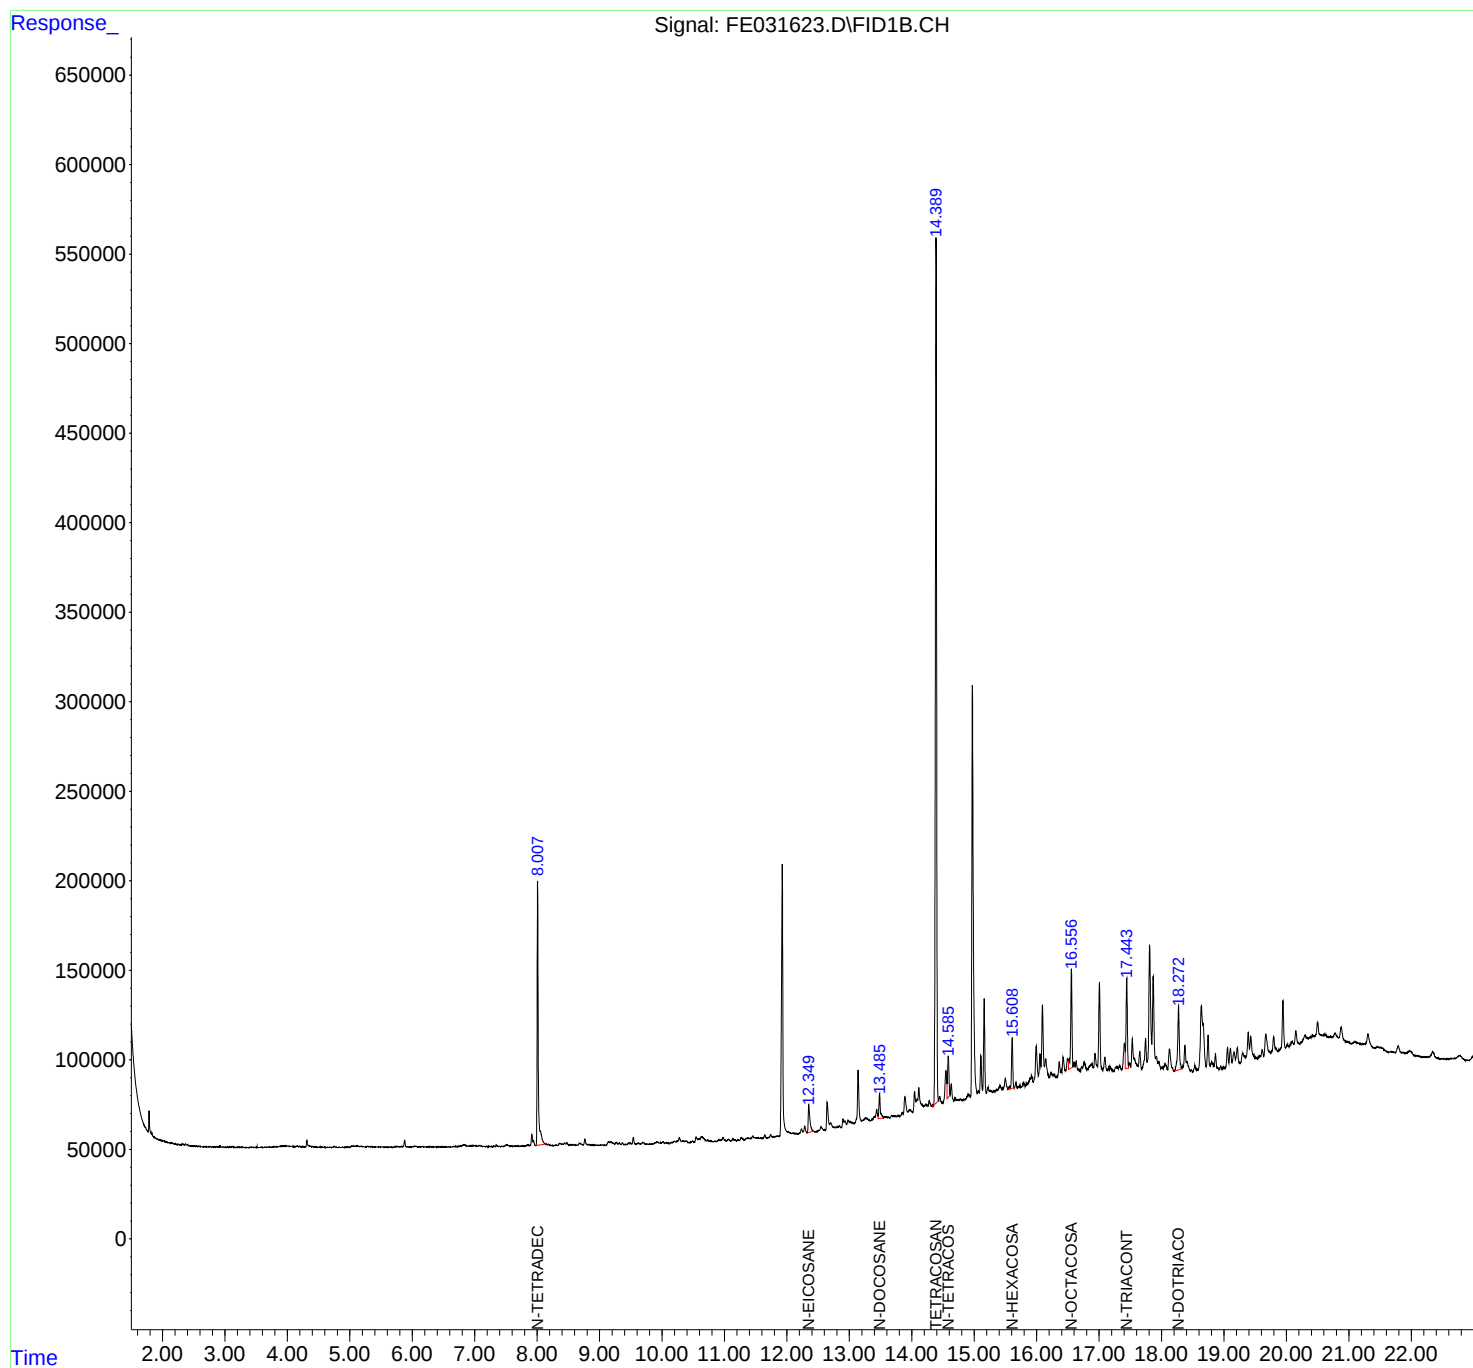


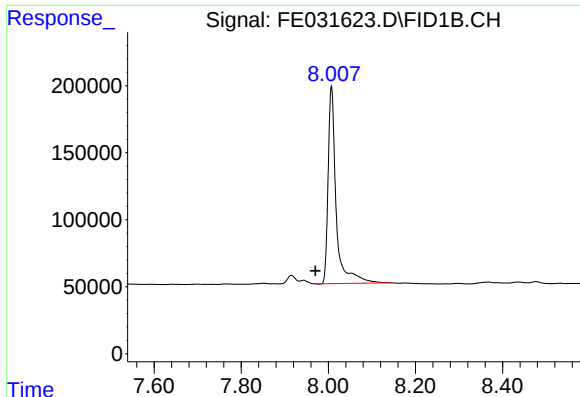

#4 N-TETRADECANE


R.T.: 8.007 min
Delta R.T.: 0.037 min
Response: 1897077
Conc: 4.56 ug/ml

Instrument :
FID_E
ClientSampleId :

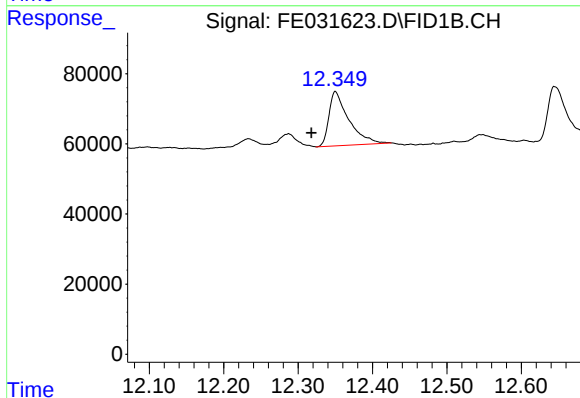


#7 N-EICOSANE

R.T.: 12.351 min
Delta R.T.: 0.033 min
Response: 285219
Conc: 0.67 ug/ml

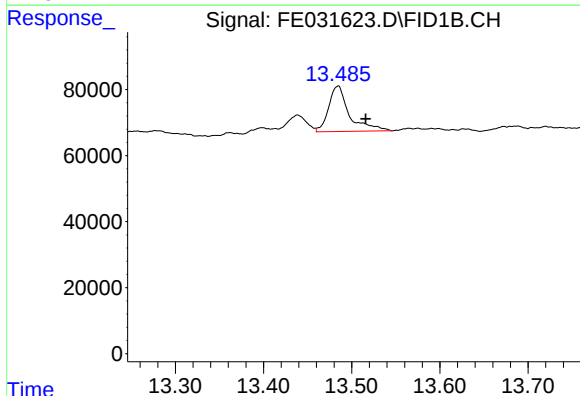


#8 N-DOCOSANE

R.T.: 13.484 min
Delta R.T.: -0.032 min
Response: 224352
Conc: 0.53 ug/ml

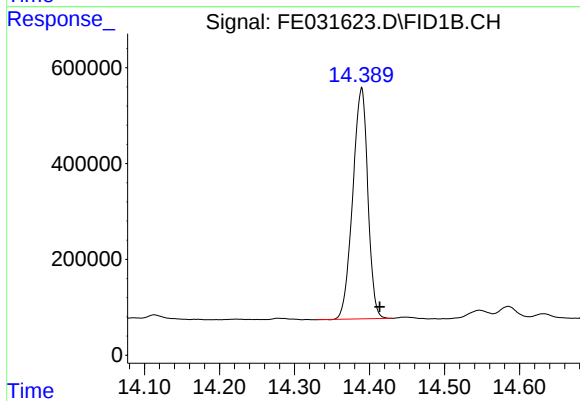

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.389 min
Delta R.T.: -0.024 min
Response: 6746453
Conc: 18.28 ug/ml

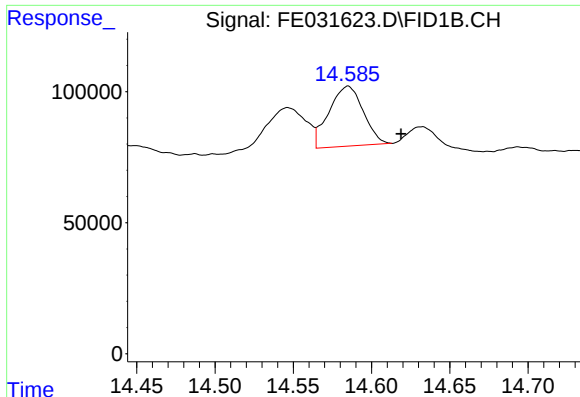

#10 N-TETRACOSANE


R.T.: 14.585 min
Delta R.T.: -0.034 min
Response: 349373
Conc: 0.82 ug/ml

Instrument :
FID_E
ClientSampleId :

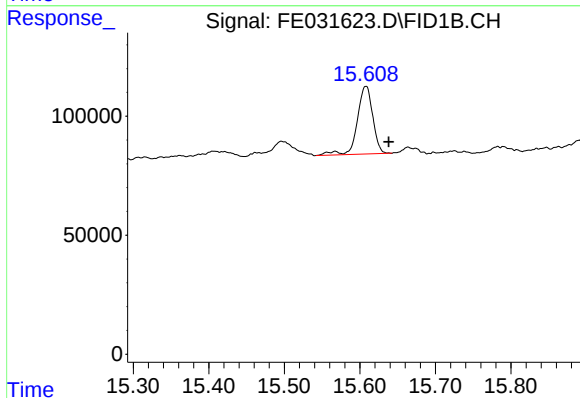


#11 N-HEXACOSANE

R.T.: 15.608 min
Delta R.T.: -0.030 min
Response: 403993
Conc: 0.96 ug/ml

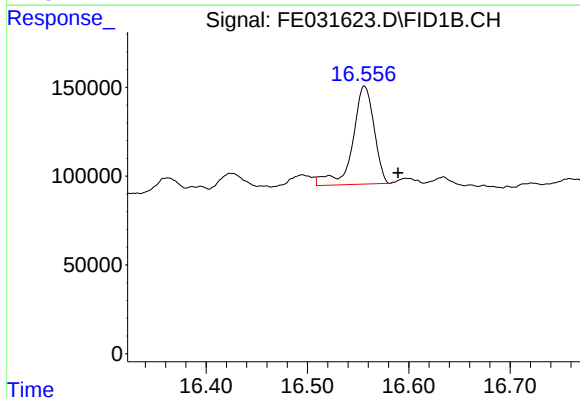


#12 N-OCTACOSANE

R.T.: 16.556 min
Delta R.T.: -0.033 min
Response: 810313
Conc: 1.93 ug/ml

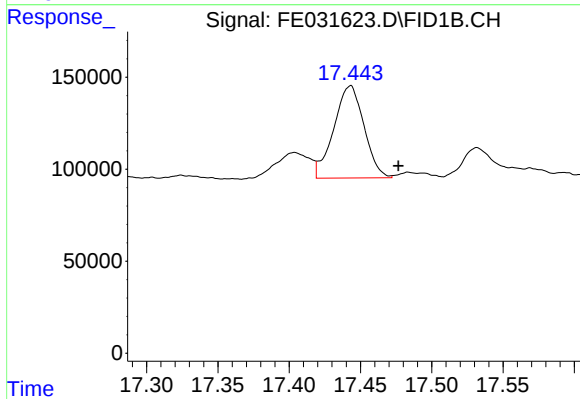

#13 N-TRIACONTANE

R.T.: 17.443 min
Delta R.T.: -0.034 min
Response: 742367
Conc: 1.78 ug/ml

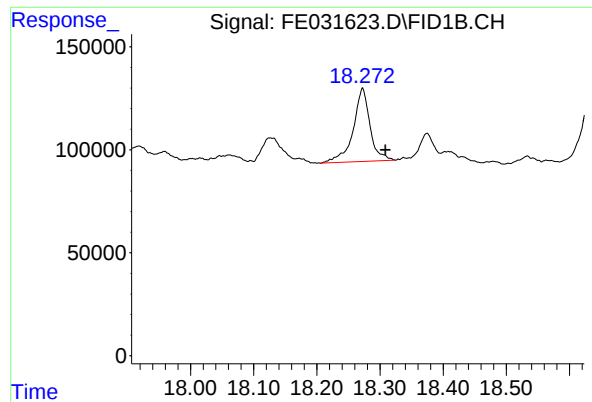

#14 N-DOTRIACONTANE

R.T.: 18.272 min
Delta R.T.: -0.036 min
Response: 657030
Conc: 1.66 ug/ml

Instrument :
FID_E
ClientSampleId :