

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040120\  
 Data File : FE031624.D  
 Signal(s) : FID1B.CH  
 Acq On : 01 Apr 2020 20:27  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Apr 02 00:34:07 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
 Quant Title :  
 QLast Update : Fri Mar 20 08:17:28 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.387 | 6657821  | 18.039 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.441 | 236444   | 0.566 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.273 | 266792   | 0.673 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040120\  
Data File : FE031624.D  
Signal(s) : FID1B.CH  
Acq On : 01 Apr 2020 20:27  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 02 00:34:07 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
Quant Title :  
QLast Update : Fri Mar 20 08:17:28 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

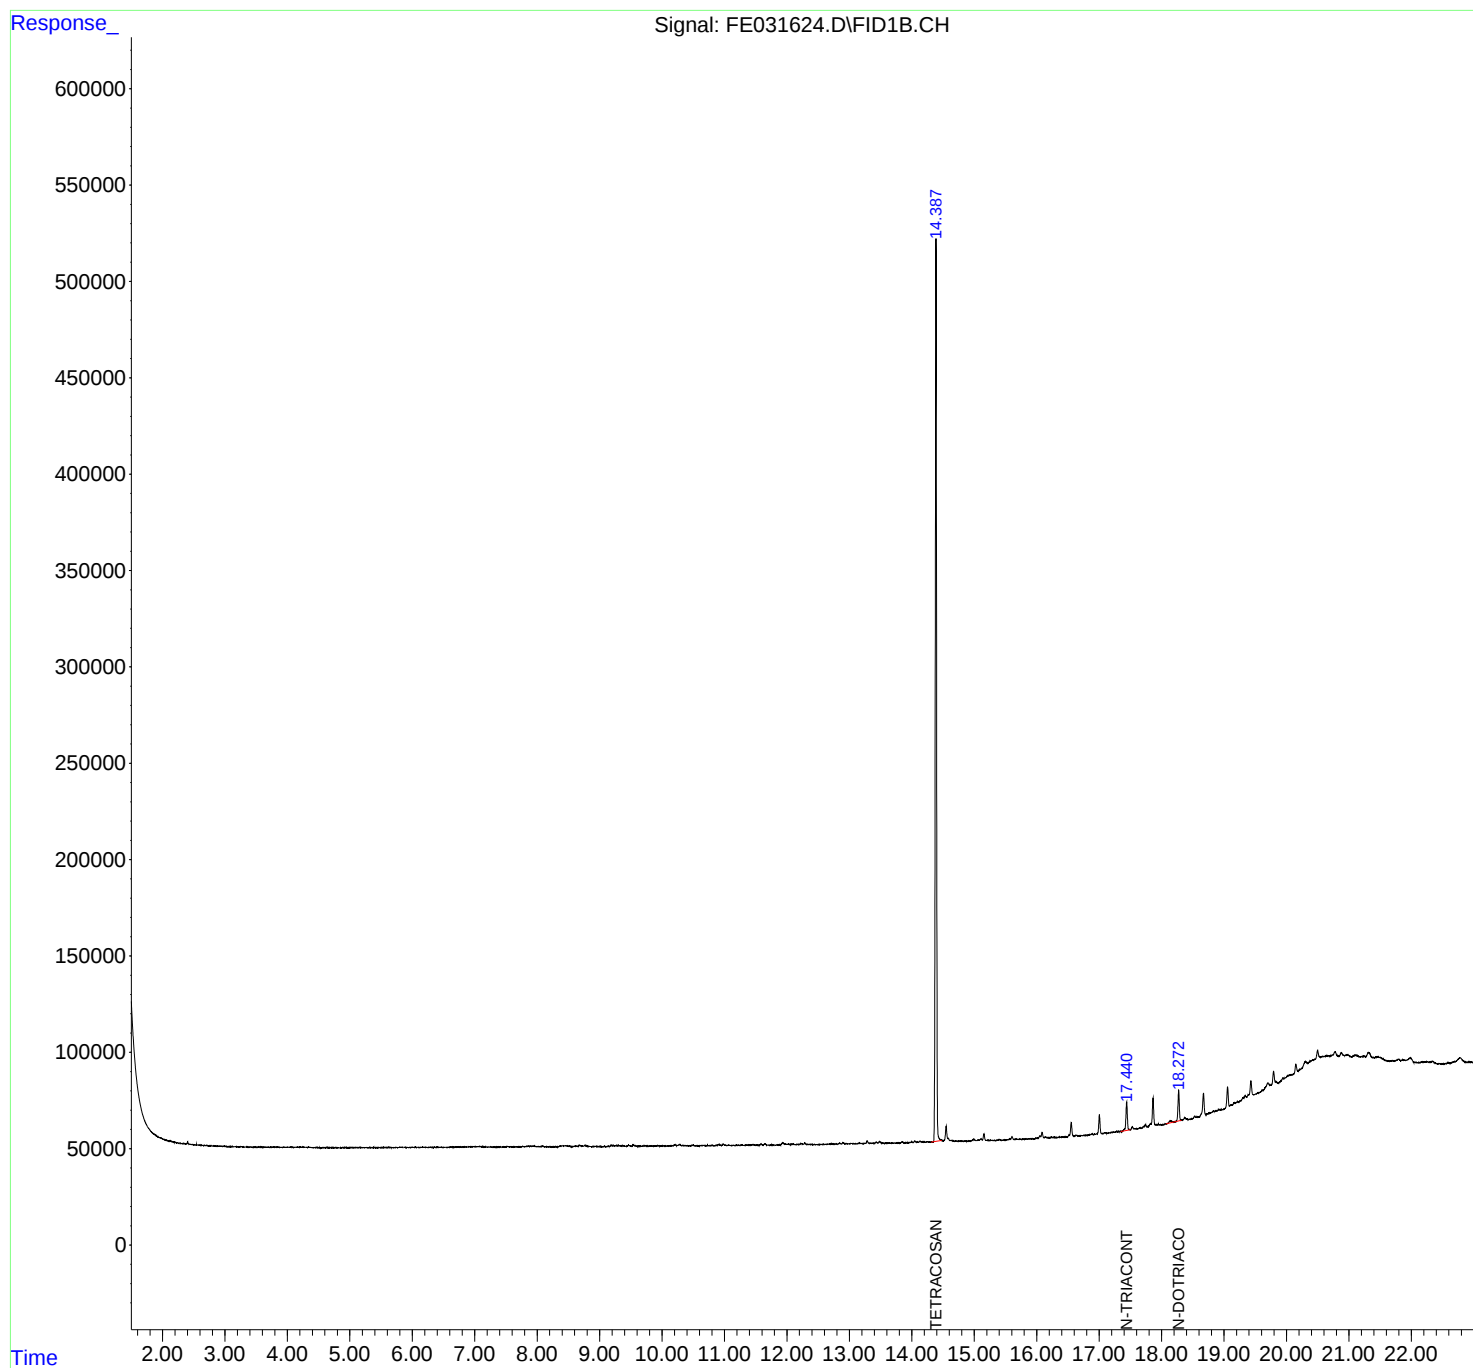


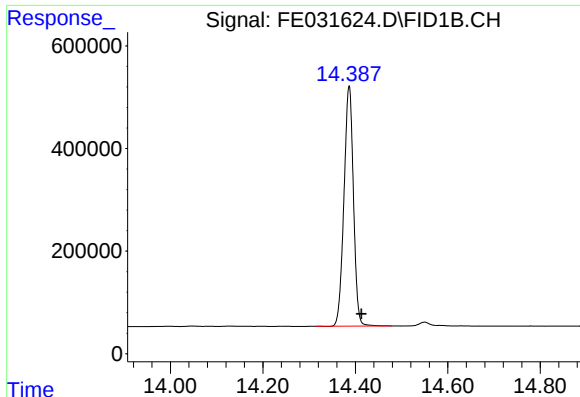

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.387 min  
Delta R.T.: -0.027 min  
Response: 6657821  
Conc: 18.04 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

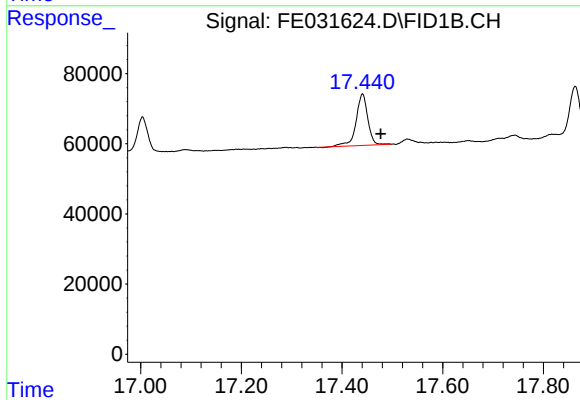

#13 N-TRIACONTANE

R.T.: 17.441 min  
Delta R.T.: -0.036 min  
Response: 236444  
Conc: 0.57 ug/ml

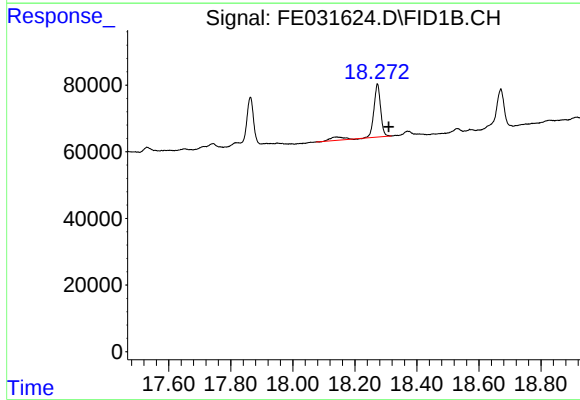

#14 N-DOTRIACONTANE

R.T.: 18.273 min  
Delta R.T.: -0.036 min  
Response: 266792  
Conc: 0.67 ug/ml