

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
 Data File : FE031630.D
 Signal(s) : FID1B.CH
 Acq On : 01 Apr 2020 23:45
 Operator : DD\AJ
 Sample : L2100-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 00:35:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.390	5915067	16.027 ug/ml
Target Compounds			
4) N-TETRADECANE	8.008	2001464	4.813 ug/ml
7) N-EICOSANE	12.343	2585180	6.048 ug/ml
8) N-DOCOSANE	13.509	716330	1.679 ug/ml
10) N-TETRACOSANE	14.569	2969637	6.973 ug/ml
11) N-HEXACOSANE	15.610	829032	1.974 ug/ml
12) N-OCTACOSANE	16.561	2717200	6.474 ug/ml
13) N-TRIACONTANE	17.449	1584280	3.791 ug/ml
14) N-DOTRIACONTANE	18.276	1423389	3.592 ug/ml
15) N-TETRATRIACONTANE	19.107	414659	1.199 ug/ml
16) N-HEXATRIACONTANE	19.802	624950	2.237 ug/ml
17) N-OCTATRIACONTANE	20.505	559343	2.471 ug/ml
18) N-TETRACONTANE	21.313	370539	1.726 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040120\
Data File : FE031630.D
Signal(s) : FID1B.CH
Acq On : 01 Apr 2020 23:45
Operator : DD\AJ
Sample : L2100-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 00:35:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

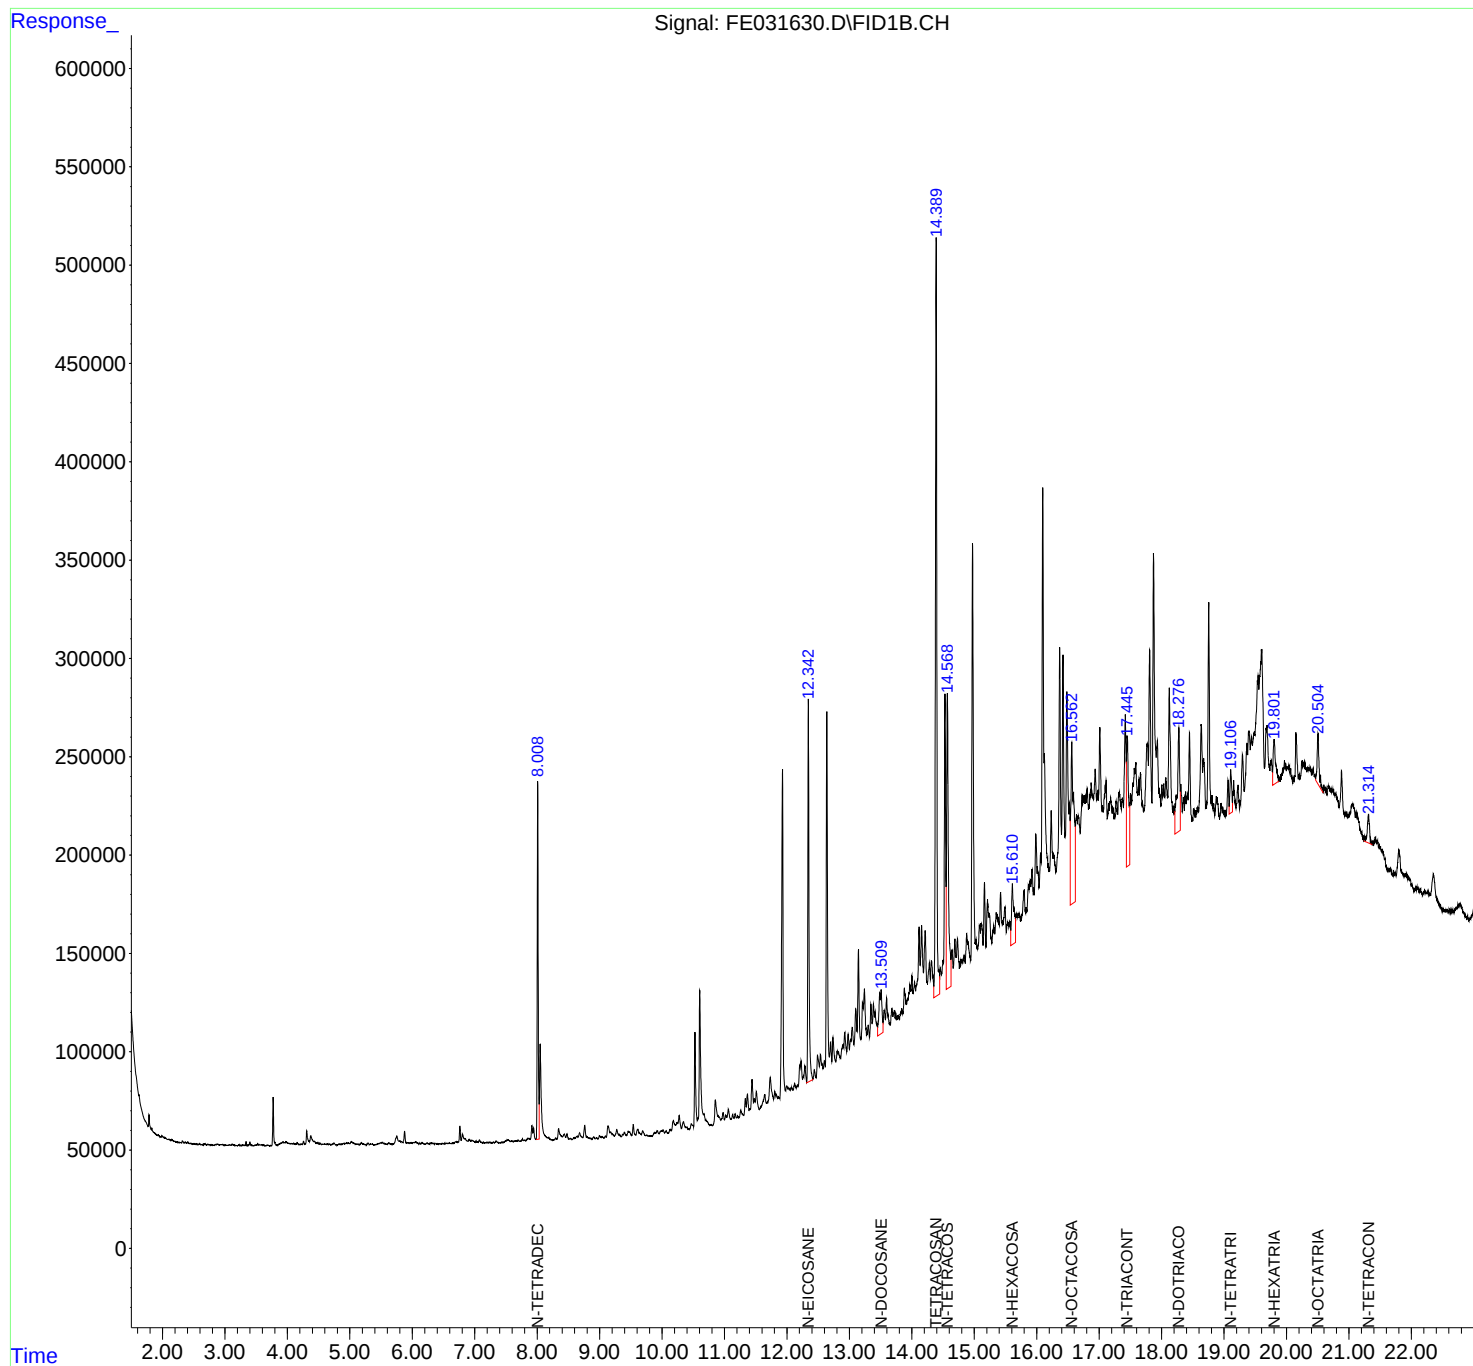


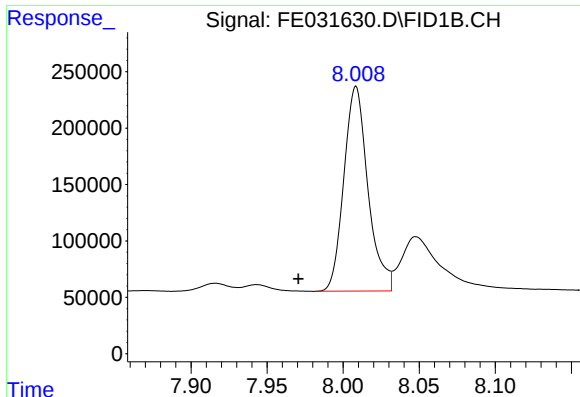

#4 N-TETRADECANE


R.T.: 8.008 min
Delta R.T.: 0.038 min
Response: 2001464
Conc: 4.81 ug/ml

Instrument :
FID_E
ClientSampleId :

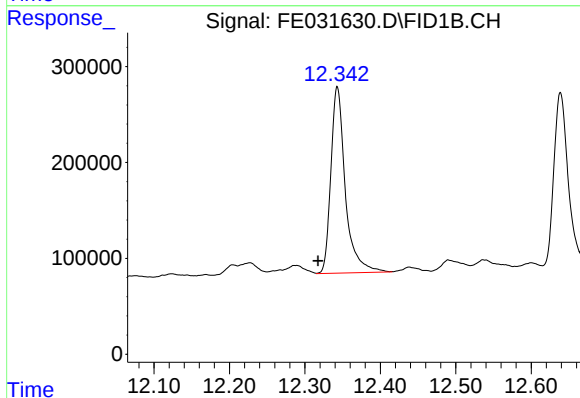


#7 N-EICOSANE

R.T.: 12.343 min
Delta R.T.: 0.025 min
Response: 2585180
Conc: 6.05 ug/ml

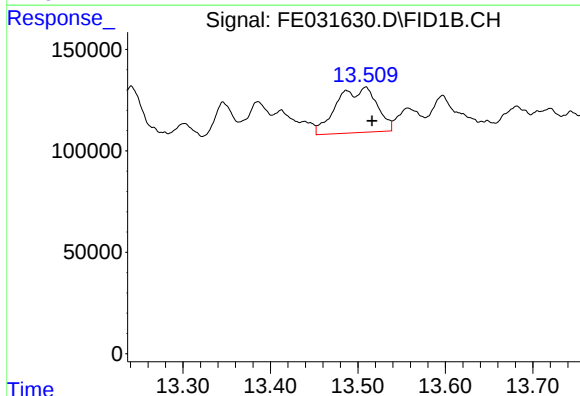


#8 N-DOCOSANE

R.T.: 13.509 min
Delta R.T.: -0.007 min
Response: 716330
Conc: 1.68 ug/ml

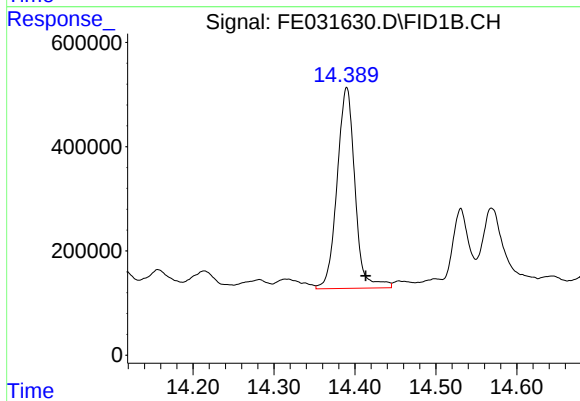

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.390 min
Delta R.T.: -0.024 min
Response: 5915067
Conc: 16.03 ug/ml

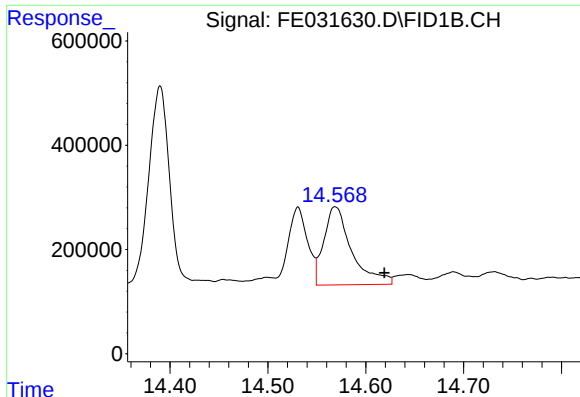

#10 N-TETRACOSANE


R.T.: 14.569 min
Delta R.T.: -0.050 min
Response: 2969637
Conc: 6.97 ug/ml

Instrument :
FID_E
ClientSampleId :

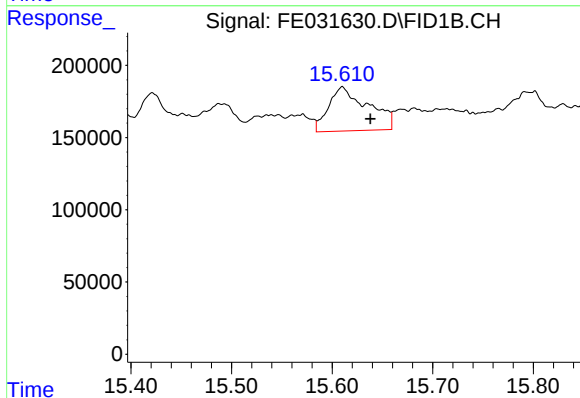


#11 N-HEXACOSANE

R.T.: 15.610 min
Delta R.T.: -0.028 min
Response: 829032
Conc: 1.97 ug/ml

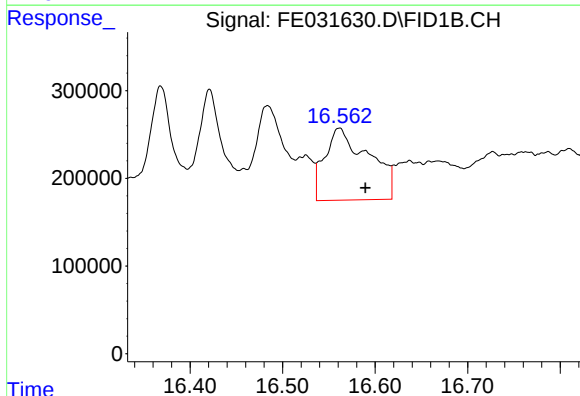


#12 N-OCTACOSANE

R.T.: 16.561 min
Delta R.T.: -0.028 min
Response: 2717200
Conc: 6.47 ug/ml

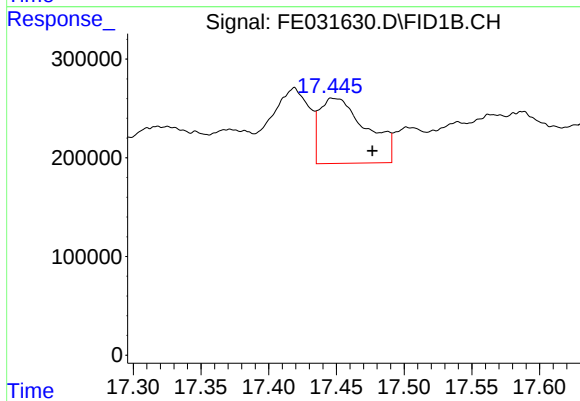

#13 N-TRIACONTANE


R.T.: 17.449 min
Delta R.T.: -0.028 min
Response: 1584280
Conc: 3.79 ug/ml

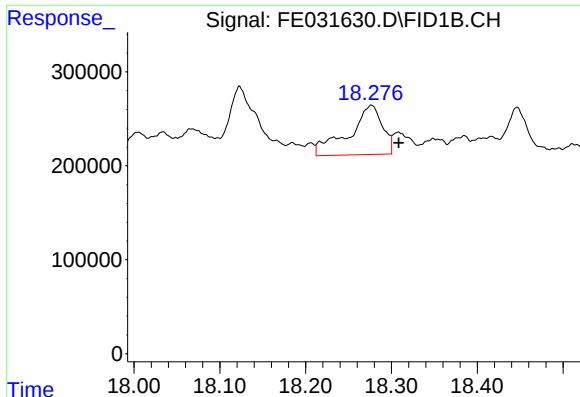

#14 N-DOTRIACONTANE


R.T.: 18.276 min
Delta R.T.: -0.032 min
Response: 1423389
Conc: 3.59 ug/ml

Instrument :
FID_E
ClientSampleId :

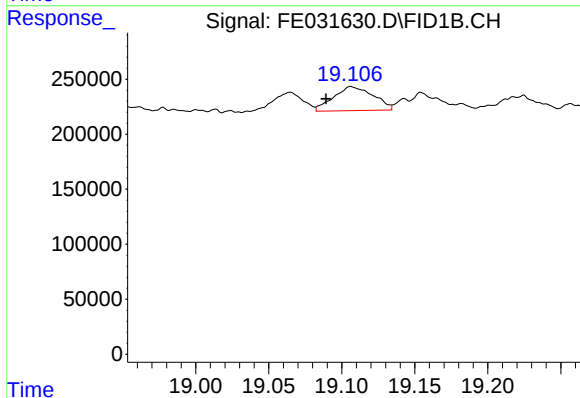


#15 N-TETRATRIACONTANE

R.T.: 19.107 min
Delta R.T.: 0.018 min
Response: 414659
Conc: 1.20 ug/ml

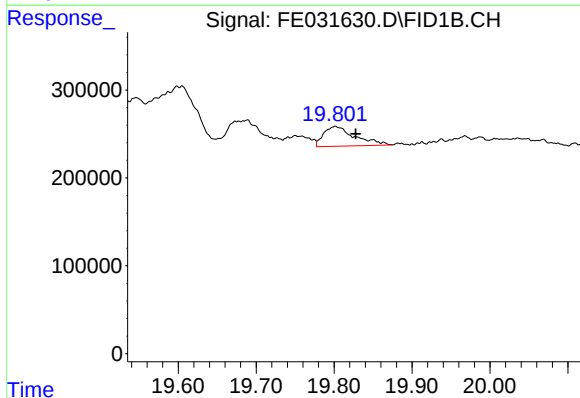


#16 N-HEXATRIACONTANE

R.T.: 19.802 min
Delta R.T.: -0.026 min
Response: 624950
Conc: 2.24 ug/ml

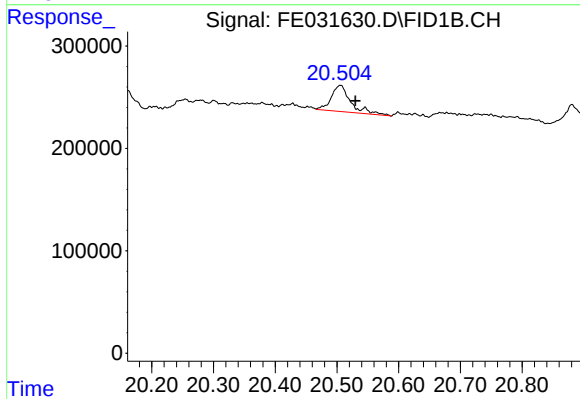

#17 N-OCTATRIACONTANE

R.T.: 20.505 min
Delta R.T.: -0.025 min
Response: 559343
Conc: 2.47 ug/ml

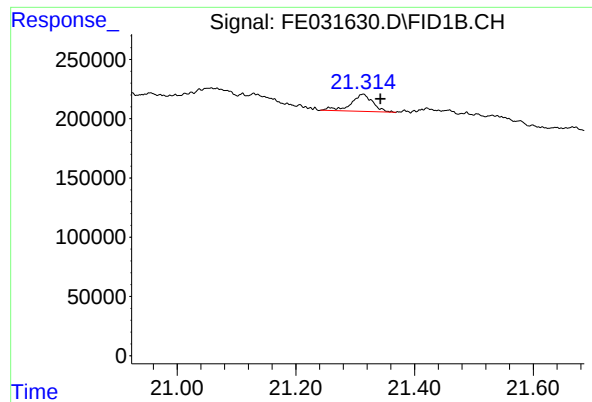

#18 N-TETRACONTANE

R.T.: 21.313 min
Delta R.T.: -0.030 min
Response: 370539
Conc: 1.73 ug/ml

Instrument :
FID_E
ClientSampleId :