

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040125AL\
 Data File : FE053104.D
 Signal(s) : FID1B.ch
 Acq On : 01 Apr 2025 20:27
 Operator : YP\AJ
 Sample : Q1681-01D
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 04:49:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032925.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 31 02:44:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.893	6225276	38.219 ug/ml
Spiked Amount 50.000		Recovery =	76.44%
12) S 1-chlorooctadecane (S...	13.338	4668413	38.889 ug/ml
Spiked Amount 50.000		Recovery =	77.78%
Target Compounds			
17) T n-Tricontane (C30)	18.062	181599	1.340 ug/ml
18) T n-Dotriacontane (C32)	18.896	317015	2.356 ug/ml
19) T n-Tetratriacontane (C34)	19.682	320960	2.480 ug/ml
20) T n-Hexatriacontane (C36)	20.424	283355	2.385 ug/ml
21) T n-Octatriacontane (C38)	21.162	220231	1.916 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040125AL\
Data File : FE053104.D
Signal(s) : FID1B.ch
Acq On : 01 Apr 2025 20:27
Operator : YP\AJ
Sample : Q1681-01D
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 04:49:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032925.M
Quant Title : GC Extractables
QLast Update : Mon Mar 31 02:44:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

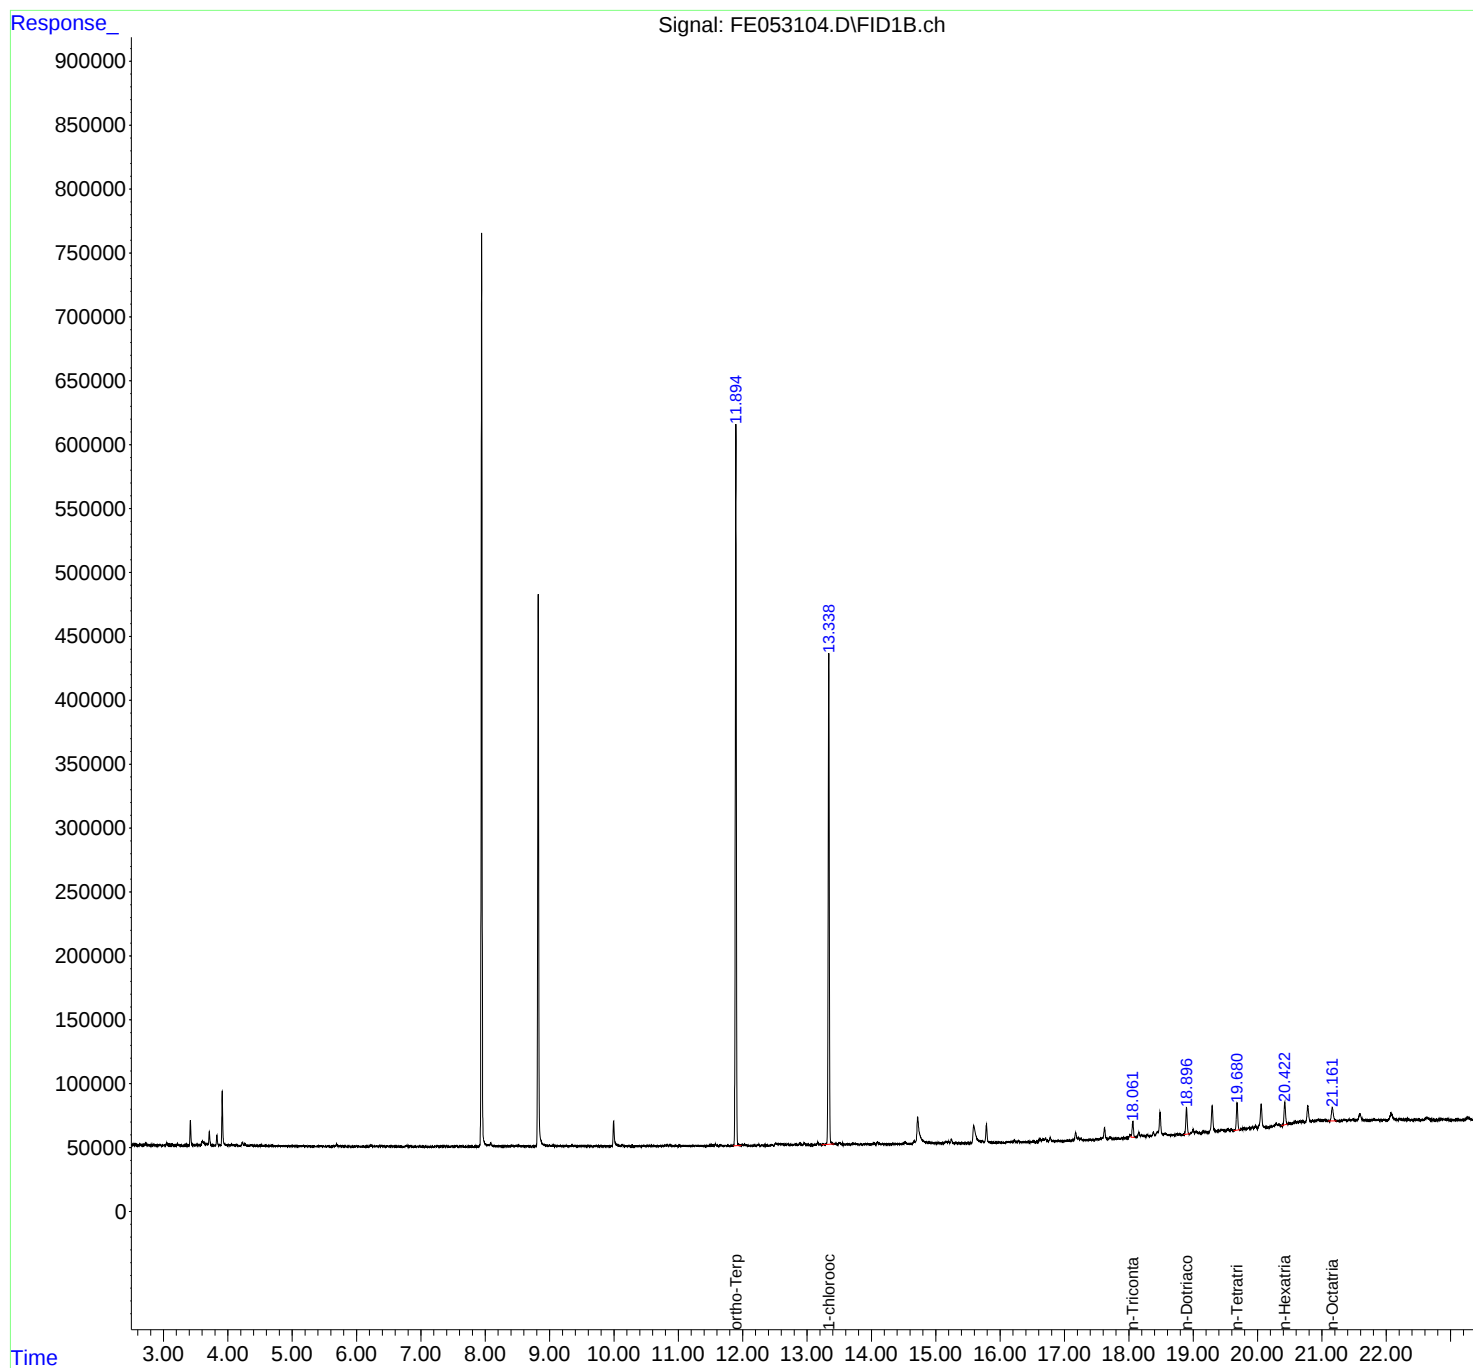


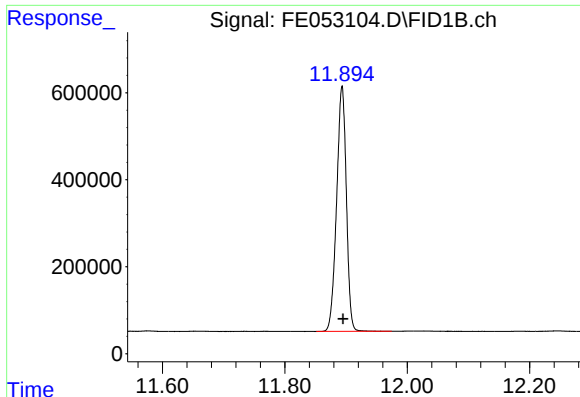

#9 ortho-Terphenyl (SURR)


R.T.: 11.893 min
Delta R.T.: -0.002 min
Response: 6225276
Conc: 38.22 ug/ml

Instrument :
FID_E
ClientSampleId :

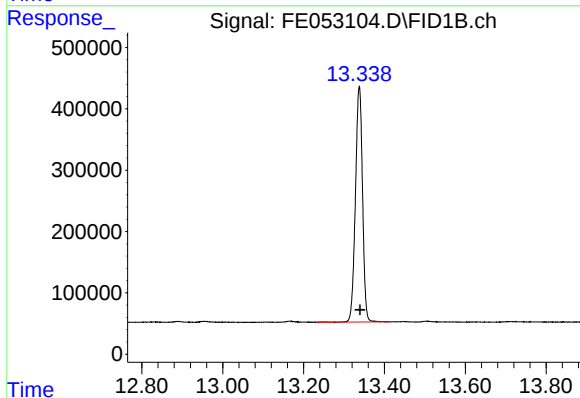


#12 1-chlorooctadecane (SURR)

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 4668413
Conc: 38.89 ug/ml

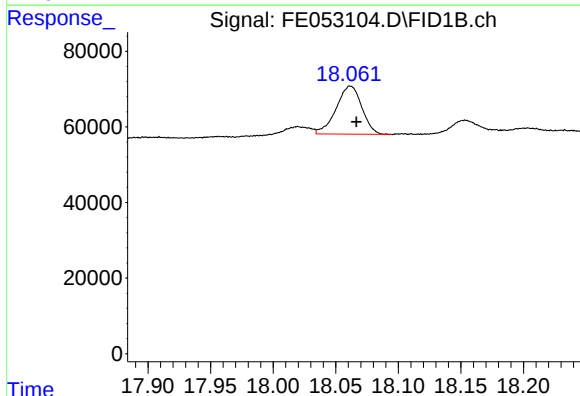


#17 n-Tricontane (C30)

R.T.: 18.062 min
Delta R.T.: -0.005 min
Response: 181599
Conc: 1.34 ug/ml

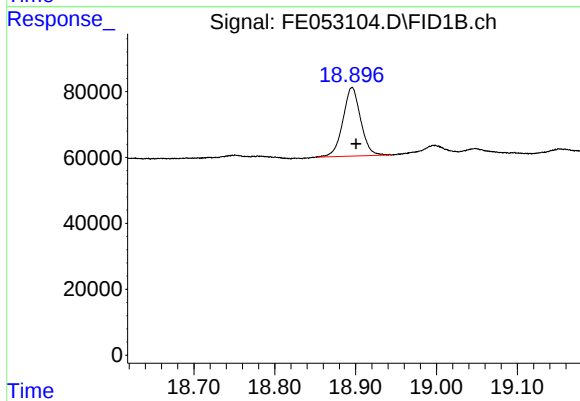

#18 n-Dotriacontane (C32)


R.T.: 18.896 min
Delta R.T.: -0.005 min
Response: 317015
Conc: 2.36 ug/ml

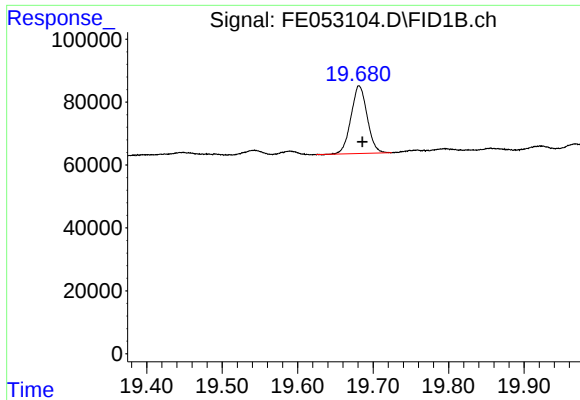

#19 n-Tetratriacontane (C34)


R.T.: 19.682 min
Delta R.T.: -0.004 min
Response: 320960
Conc: 2.48 ug/ml

Instrument :
FID_E
ClientSampleId :

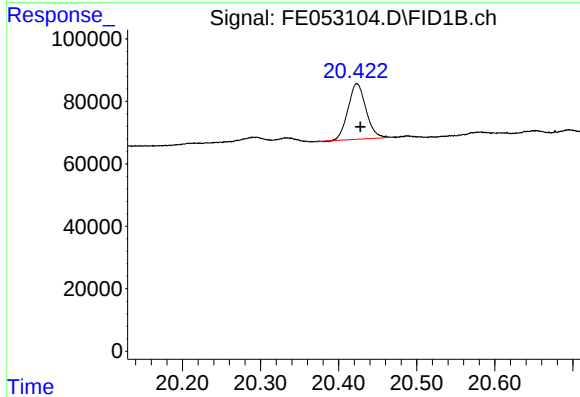

#20 n-Hexatriacontane (C36)

R.T.: 20.424 min
Delta R.T.: -0.004 min
Response: 283355
Conc: 2.39 ug/ml

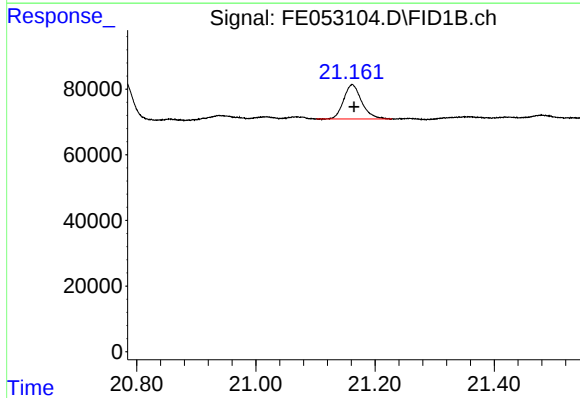

#21 n-Octatriacontane (C38)

R.T.: 21.162 min
Delta R.T.: -0.003 min
Response: 220231
Conc: 1.92 ug/ml