

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
Data File : FE031634.D
Signal(s) : FID1B.CH
Acq On : 02 Apr 2020 10:11
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 00:32:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.442	252783	0.605 ug/ml
14) N-DOTRIACONTANE	18.273	267947	0.676 ug/ml
15) N-TETRATRIACONTANE	19.056	226411	0.655 ug/ml
16) N-HEXATRIACONTANE	19.797	14863	0.053 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
Data File : FE031634.D
Signal(s) : FID1B.CH
Acq On : 02 Apr 2020 10:11
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 03 00:32:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

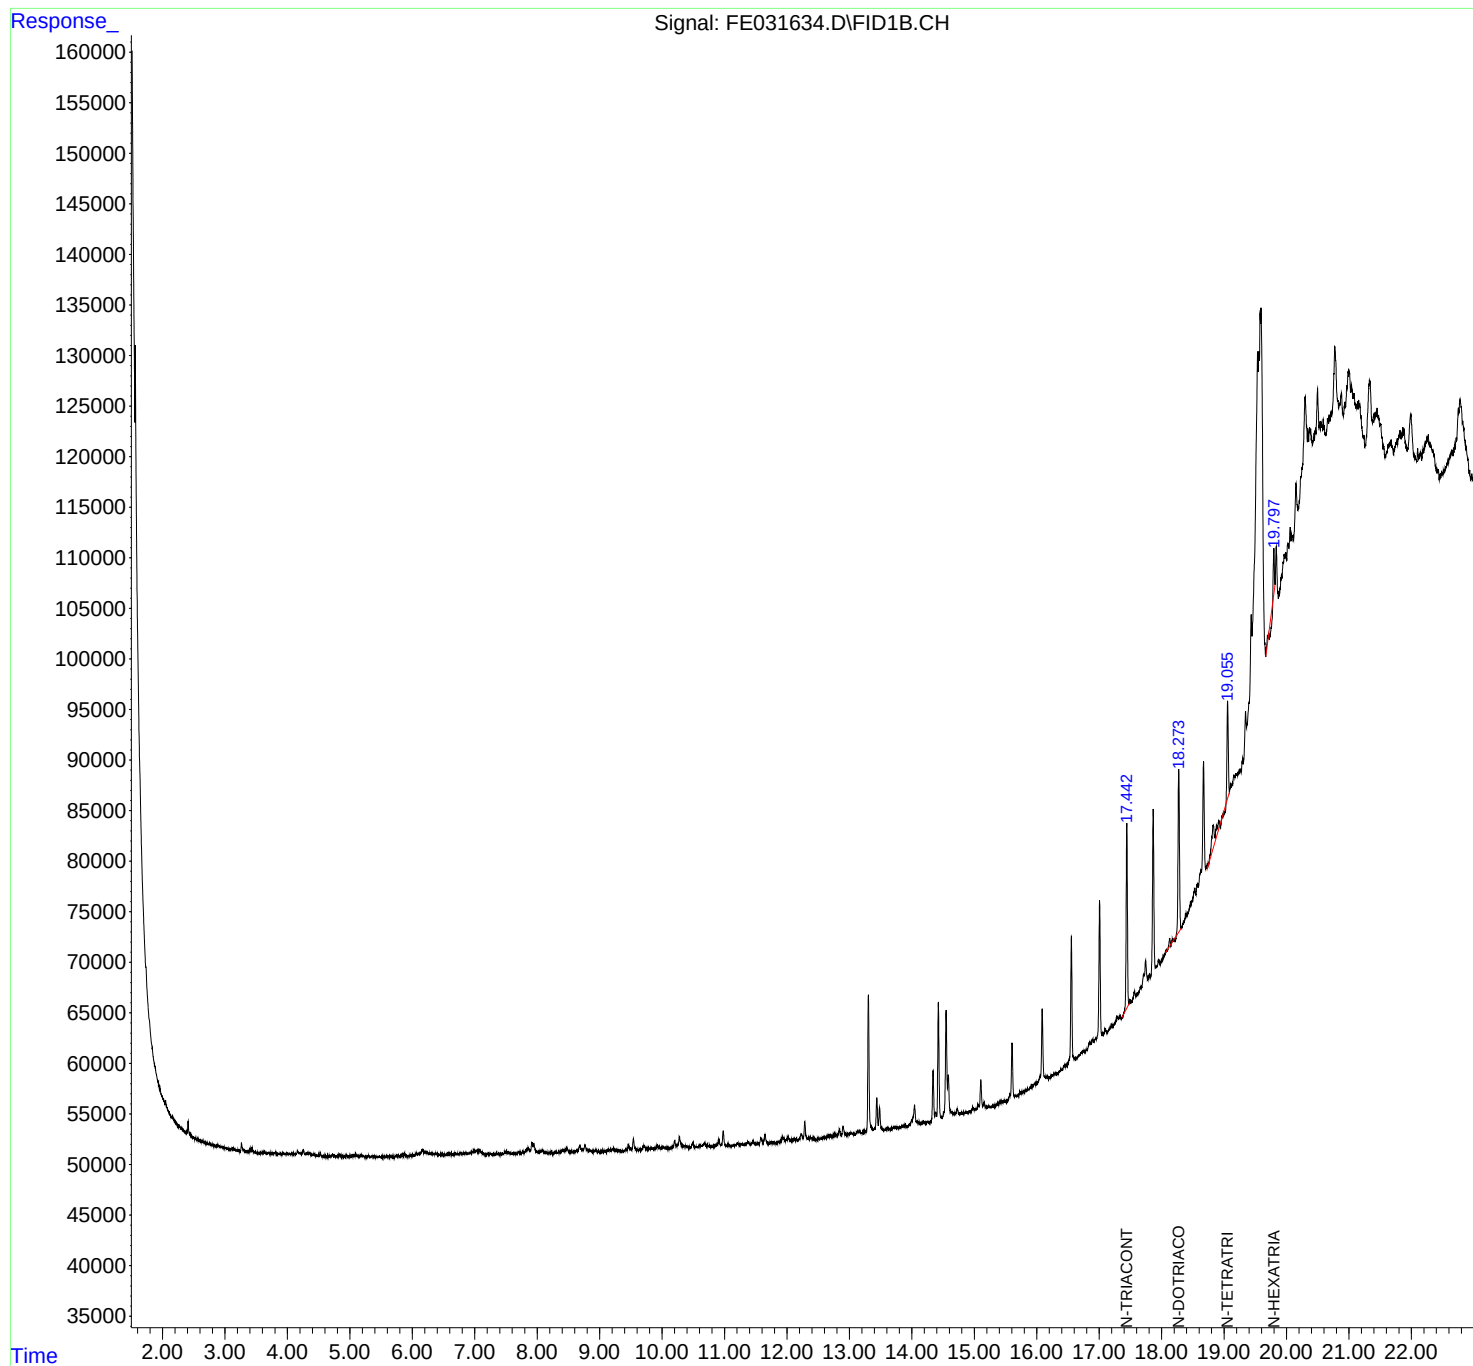


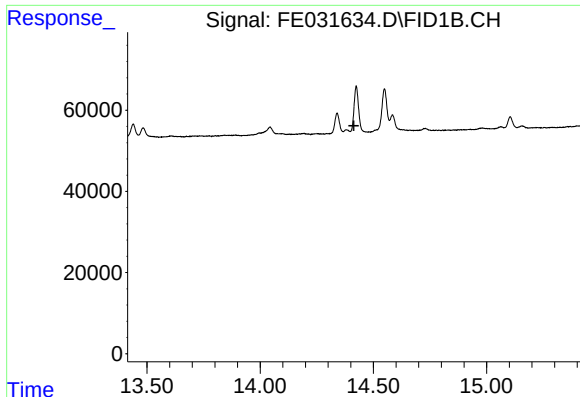

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.413 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

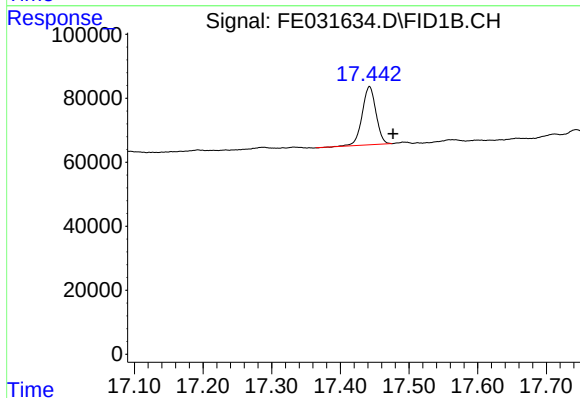


#13 N-TRIACONTANE

R.T.: 17.442 min
Delta R.T.: -0.034 min
Response: 252783
Conc: 0.60 ug/ml

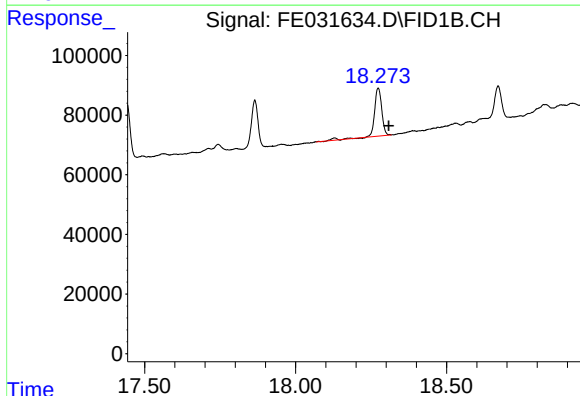


#14 N-DOTRIACONTANE

R.T.: 18.273 min
Delta R.T.: -0.035 min
Response: 267947
Conc: 0.68 ug/ml

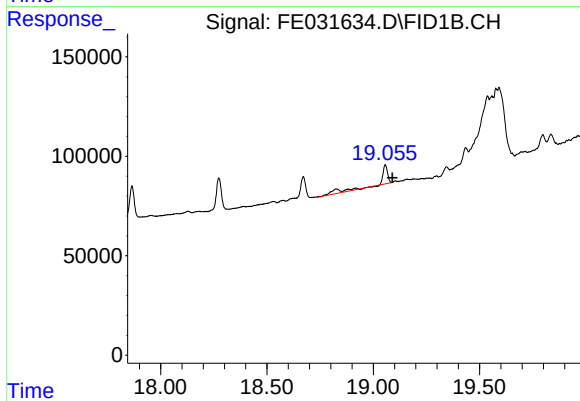

#15 N-TETRATRIACONTANE

R.T.: 19.056 min
Delta R.T.: -0.033 min
Response: 226411
Conc: 0.65 ug/ml

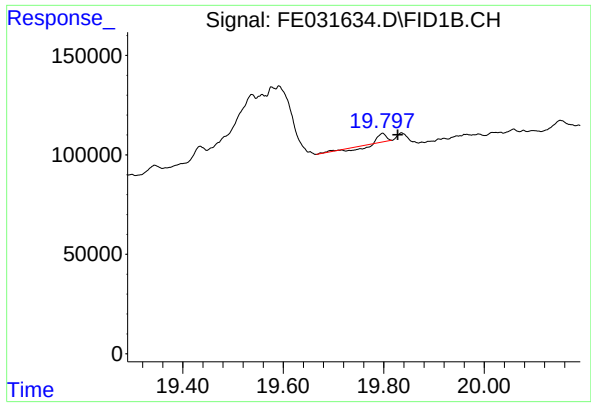

#16 N-HEXATRIACONTANE

R.T.: 19.797 min

Delta R.T.: -0.030 min

Response: 14863

Conc: 0.05 ug/ml

Instrument :
FID_E
ClientSampleId :