

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
 Data File : FE031639.D
 Signal(s) : FID1B.CH
 Acq On : 02 Apr 2020 14:06
 Operator : DD\AJ
 Sample : L2100-06 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 00:33:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.385	3332866	9.030 ug/ml
Target Compounds			
4) N-TETRADECANE	8.007	966269	2.323 ug/ml
7) N-EICOSANE	12.342	1654409	3.870 ug/ml
10) N-TETRACOSANE	14.569	1475997	3.466 ug/ml
11) N-HEXACOSANE	15.609	172496	0.411 ug/ml
12) N-OCTACOSANE	16.587	321313	0.766 ug/ml
13) N-TRIACONTANE	17.447	854398	2.045 ug/ml
14) N-DOTRIACONTANE	18.276	722473	1.823 ug/ml
15) N-TETRATRIACONTANE	19.058	191249	0.553 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
Data File : FE031639.D
Signal(s) : FID1B.CH
Acq On : 02 Apr 2020 14:06
Operator : DD\AJ
Sample : L2100-06 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 00:33:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

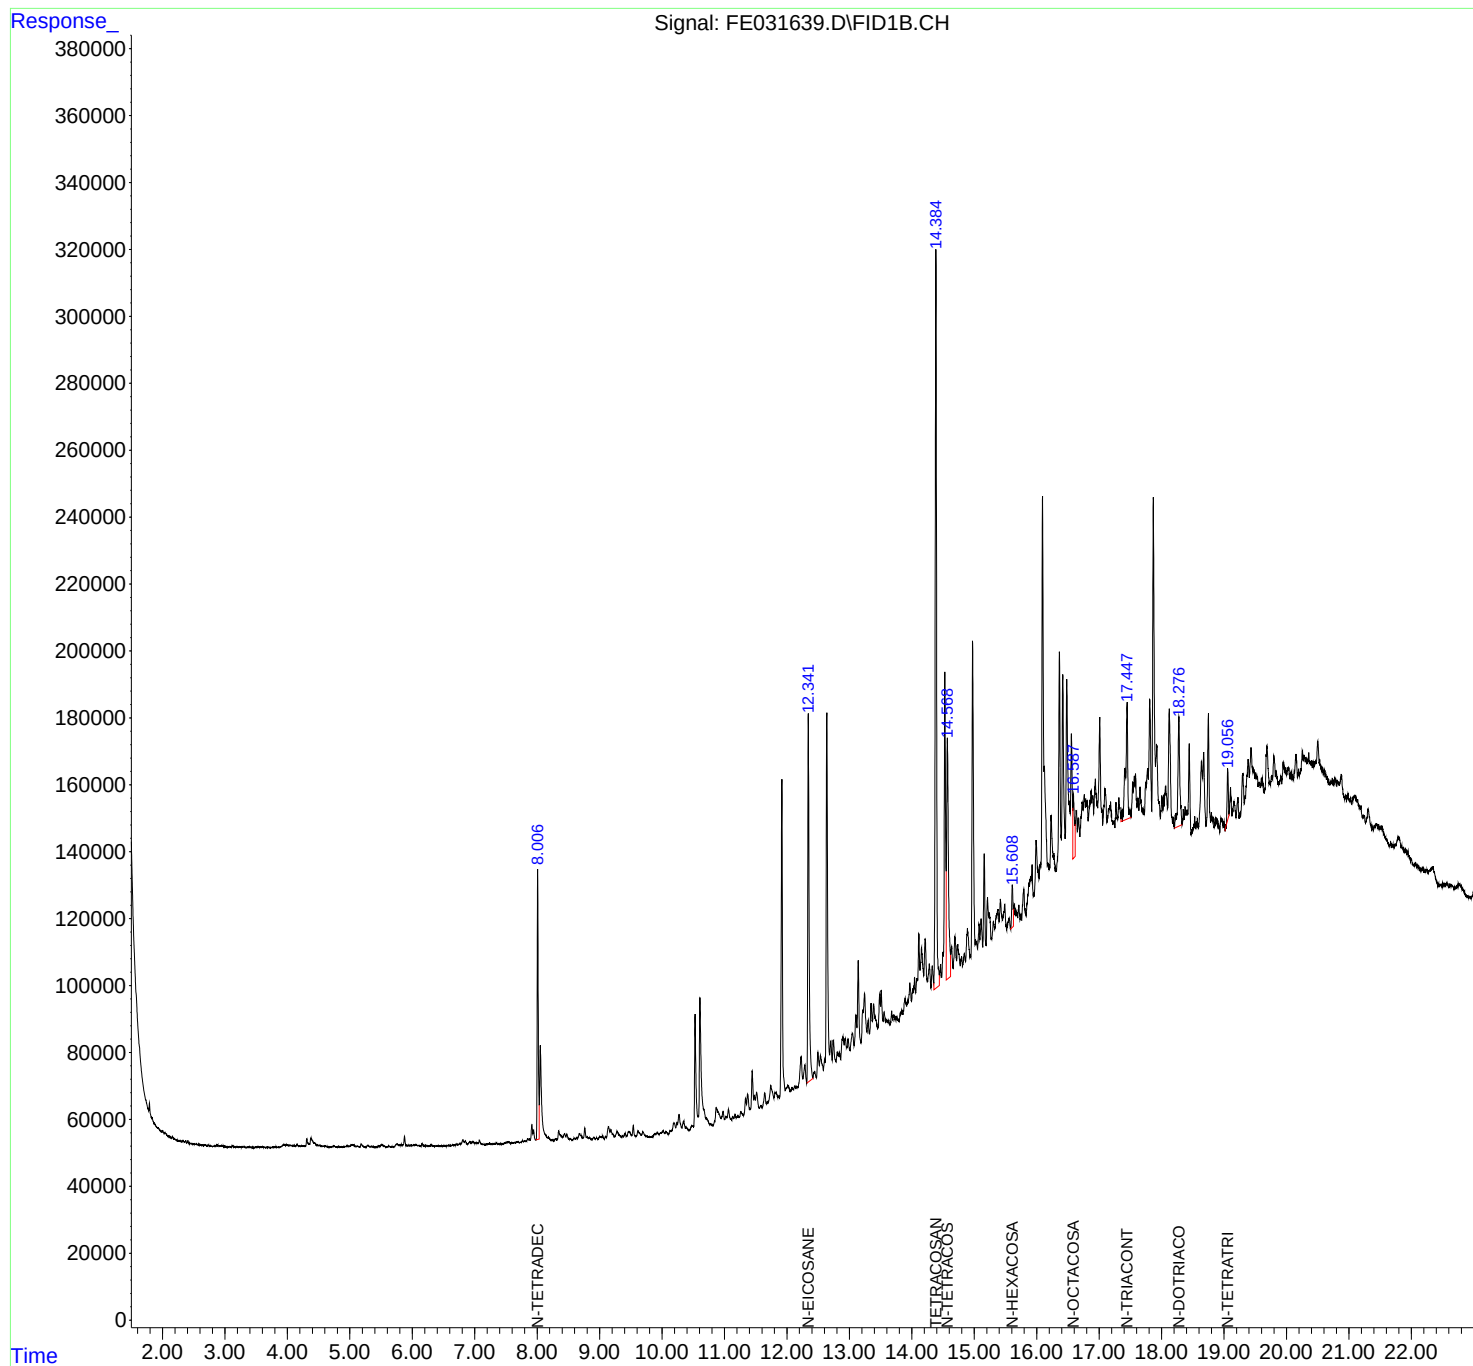


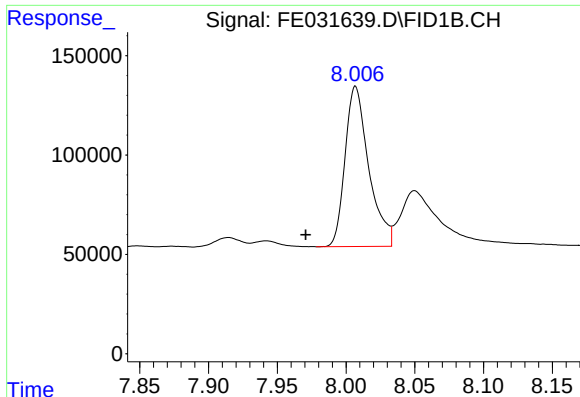

#4 N-TETRADECANE


R.T.: 8.007 min
Delta R.T.: 0.037 min
Response: 966269
Conc: 2.32 ug/ml

Instrument :
FID_E
ClientSampleId :

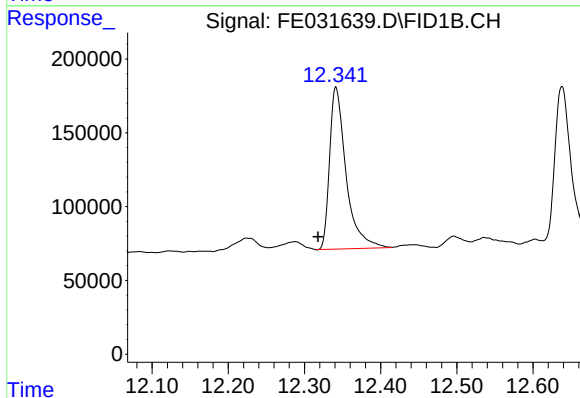


#7 N-EICOSANE

R.T.: 12.342 min
Delta R.T.: 0.024 min
Response: 1654409
Conc: 3.87 ug/ml

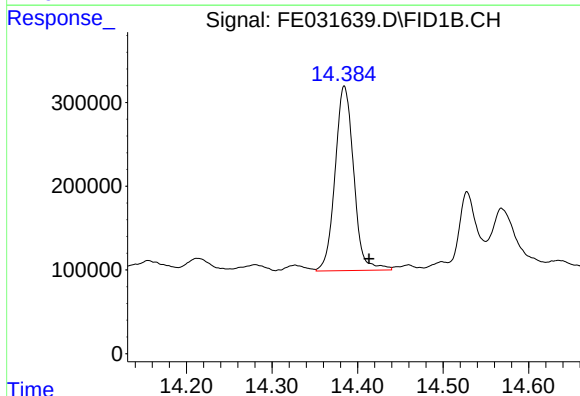


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.385 min
Delta R.T.: -0.029 min
Response: 3332866
Conc: 9.03 ug/ml

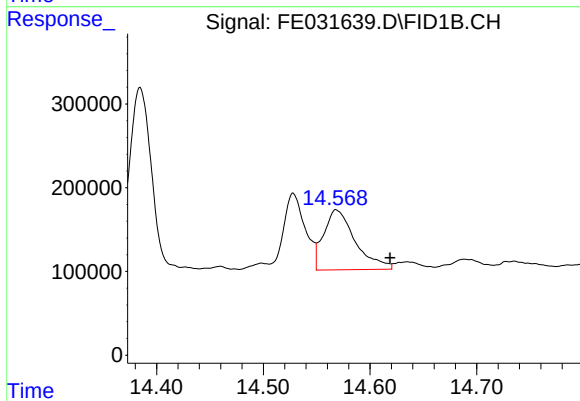

#10 N-TETRACOSANE


R.T.: 14.569 min
Delta R.T.: -0.050 min
Response: 1475997
Conc: 3.47 ug/ml

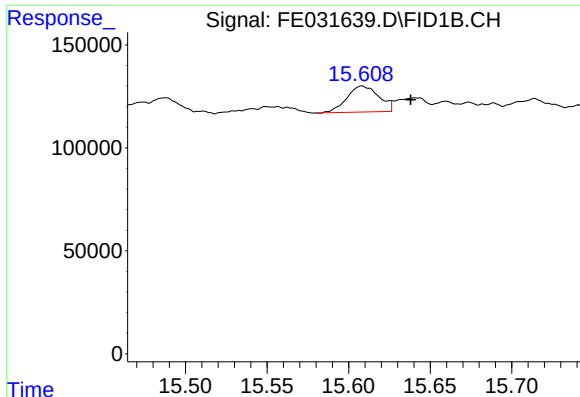

#11 N-HEXACOSANE


R.T.: 15.609 min
Delta R.T.: -0.029 min
Response: 172496
Conc: 0.41 ug/ml

Instrument :
FID_E
ClientSampleId :

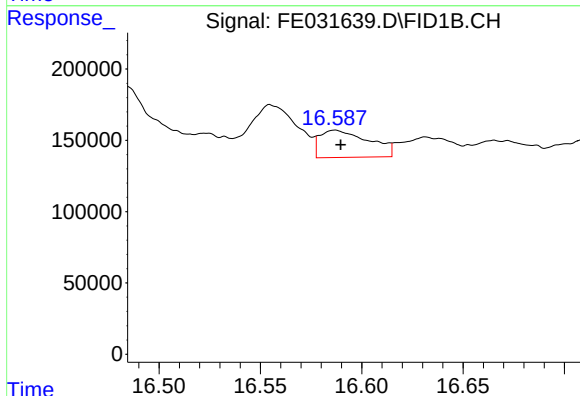


#12 N-OCTACOSANE

R.T.: 16.587 min
Delta R.T.: -0.002 min
Response: 321313
Conc: 0.77 ug/ml

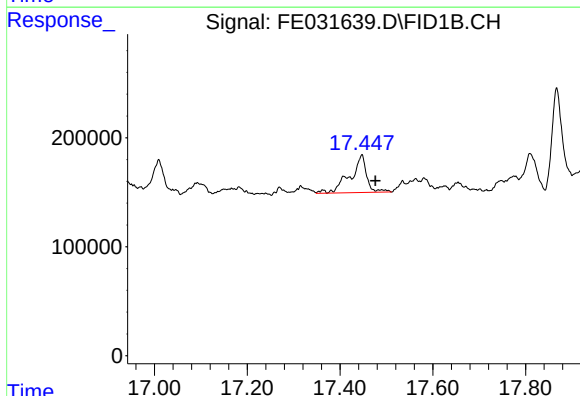


#13 N-TRIACONTANE

R.T.: 17.447 min
Delta R.T.: -0.030 min
Response: 854398
Conc: 2.04 ug/ml

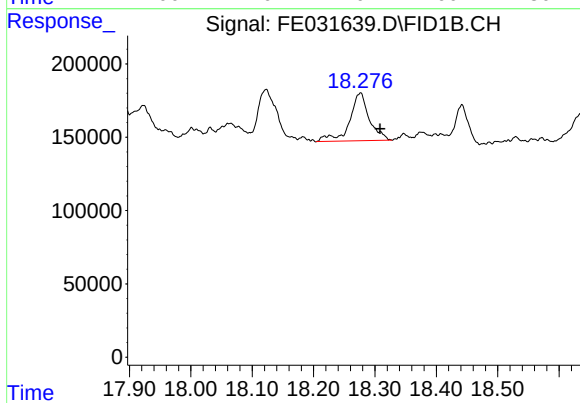

#14 N-DOTRIACONTANE

R.T.: 18.276 min
Delta R.T.: -0.033 min
Response: 722473
Conc: 1.82 ug/ml

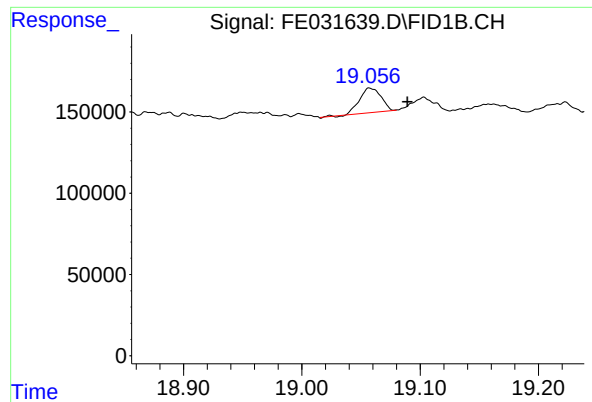

#15 N-TETRATRIACONTANE

R.T.: 19.058 min

Delta R.T.: -0.031 min

Response: 191249

Conc: 0.55 ug/ml

Instrument :
FID_E
ClientSampleId :