

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
 Data File : FE031663.D
 Signal(s) : FID1B.CH
 Acq On : 03 Apr 2020 3:25
 Operator : DD\AJ
 Sample : L2129-32 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 04:36:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.378	2469041	6.690 ug/ml
Target Compounds			
4) N-TETRADECANE	8.009	349638	0.841 ug/ml
5) N-HEXADECANE	9.546	618027	1.453 ug/ml
6) N-OCTADECANE	11.055	800327	1.869 ug/ml
7) N-EICOSANE	12.343	9405057	22.001 ug/ml
8) N-DOCOSANE	13.501	755565	1.771 ug/ml
10) N-TETRACOSANE	14.562f	5061744	11.886 ug/ml
11) N-HEXACOSANE	15.614	645393	1.537 ug/ml
12) N-OCTACOSANE	16.577	883692	2.106 ug/ml
13) N-TRIACONTANE	17.437	670522	1.605 ug/ml
14) N-DOTRIACONTANE	18.263	721945	1.822 ug/ml
15) N-TETRATRIACONTANE	19.050	183708	0.531 ug/ml
16) N-HEXATRIACONTANE	19.790	494621	1.771 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040220\
Data File : FE031663.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 3:25
Operator : DD\AJ
Sample : L2129-32 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 04:36:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

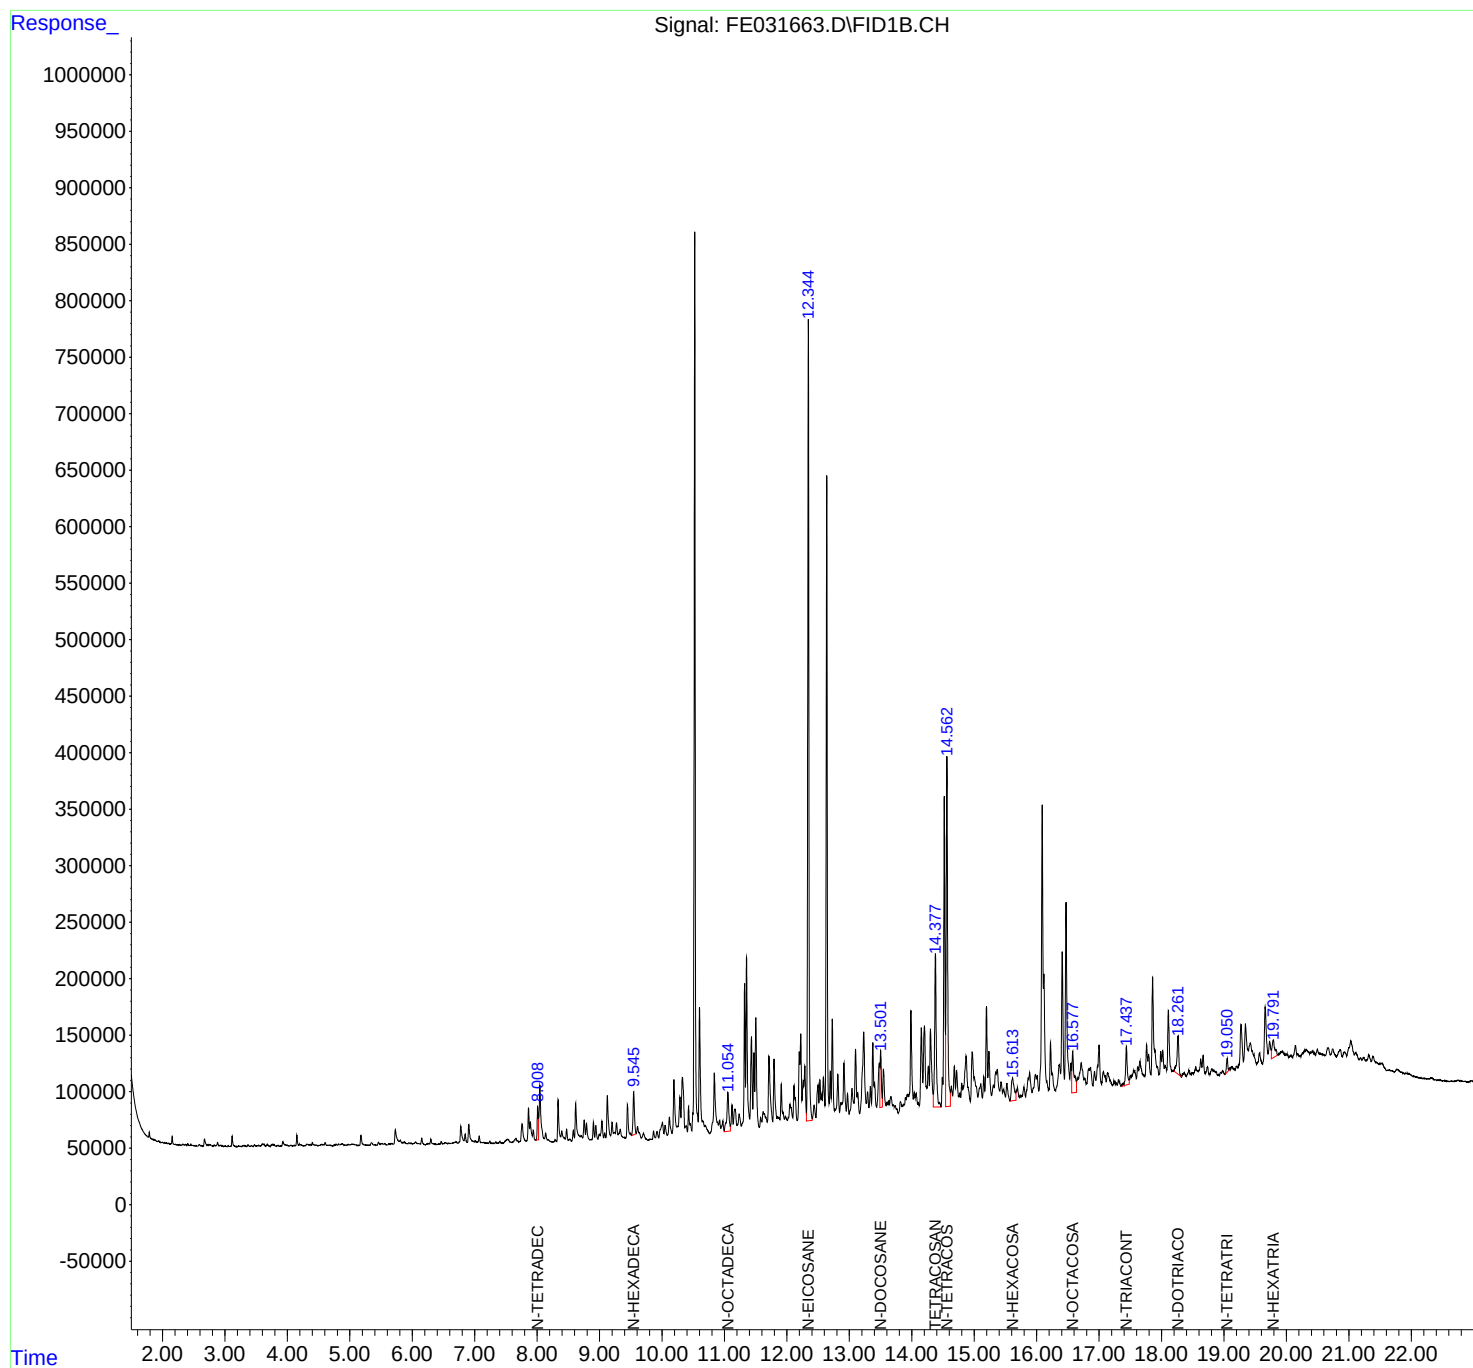


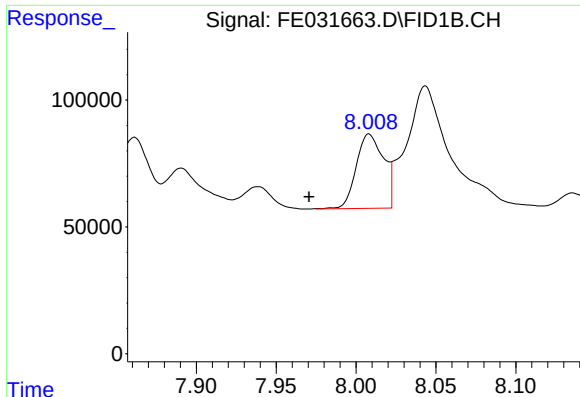

#4 N-TETRADECANE


R.T.: 8.009 min
Delta R.T.: 0.038 min
Response: 349638
Conc: 0.84 ug/ml

Instrument :
FID_E
ClientSampleId :

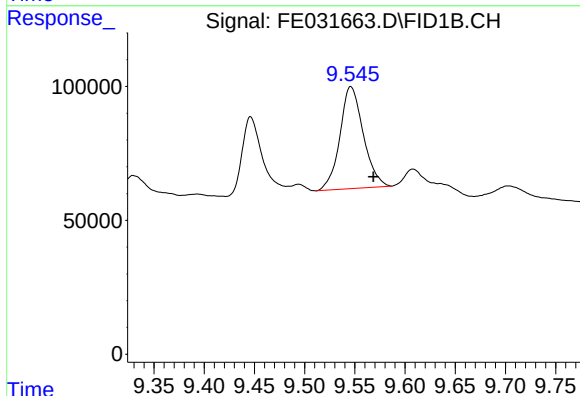


#5 N-HEXADECANE

R.T.: 9.546 min
Delta R.T.: -0.022 min
Response: 618027
Conc: 1.45 ug/ml

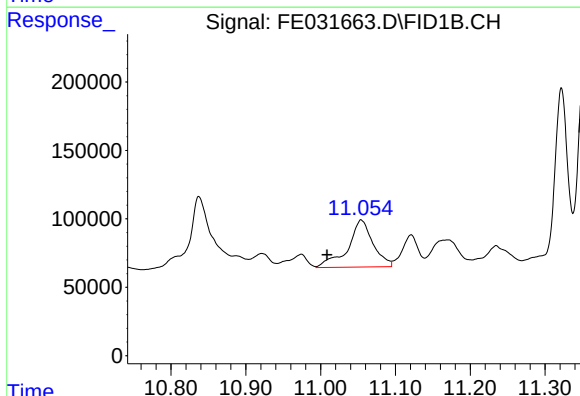


#6 N-OCTADECANE

R.T.: 11.055 min
Delta R.T.: 0.046 min
Response: 800327
Conc: 1.87 ug/ml

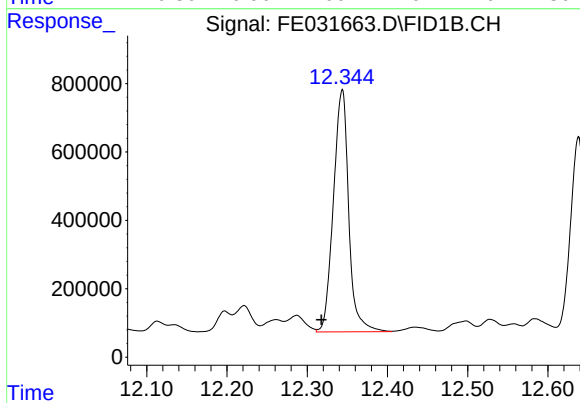

#7 N-EICOSANE


R.T.: 12.343 min
Delta R.T.: 0.026 min
Response: 9405057
Conc: 22.00 ug/ml

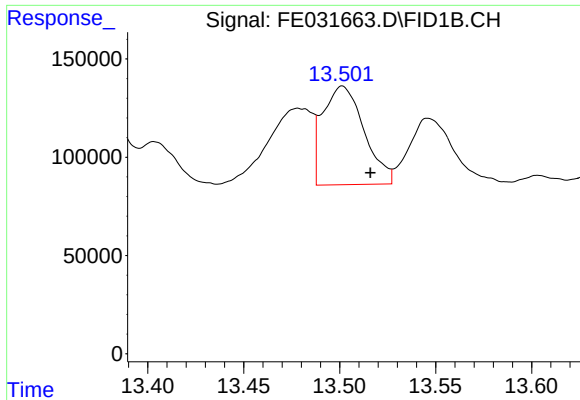

#8 N-DOCOSANE


R.T.: 13.501 min
Delta R.T.: -0.015 min
Response: 755565
Conc: 1.77 ug/ml

Instrument :
FID_E
ClientSampleId :

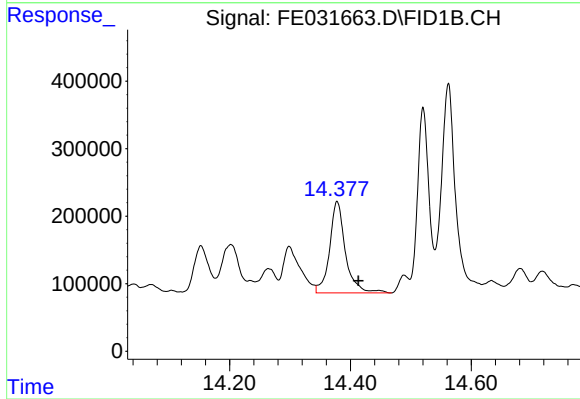


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.378 min
Delta R.T.: -0.035 min
Response: 2469041
Conc: 6.69 ug/ml

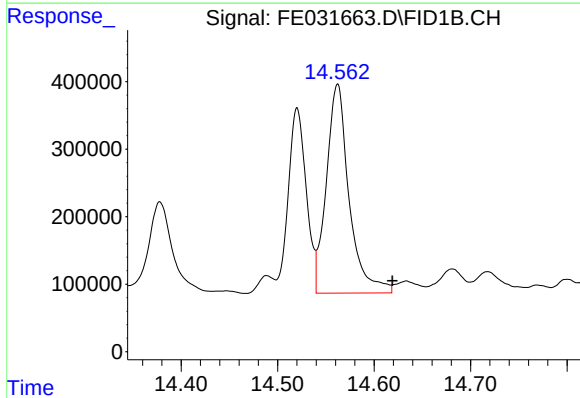


#10 N-TETRACOSANE

R.T.: 14.562 min
Delta R.T.: -0.057 min
Response: 5061744
Conc: 11.89 ug/ml

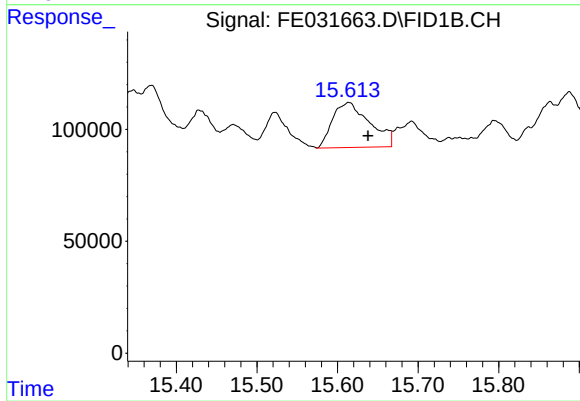

#11 N-HEXACOSANE


R.T.: 15.614 min
Delta R.T.: -0.024 min
Response: 645393
Conc: 1.54 ug/ml

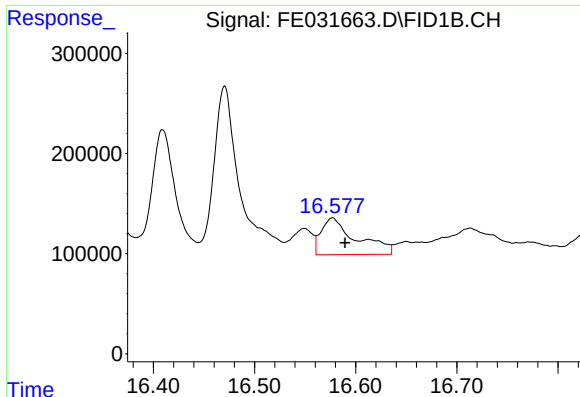

#12 N-OCTACOSANE


R.T.: 16.577 min
Delta R.T.: -0.012 min
Response: 883692
Conc: 2.11 ug/ml

Instrument :
FID_E
ClientSampleId :

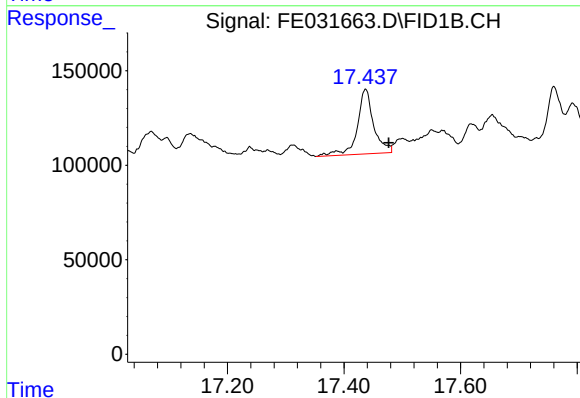


#13 N-TRIACONTANE

R.T.: 17.437 min
Delta R.T.: -0.040 min
Response: 670522
Conc: 1.60 ug/ml

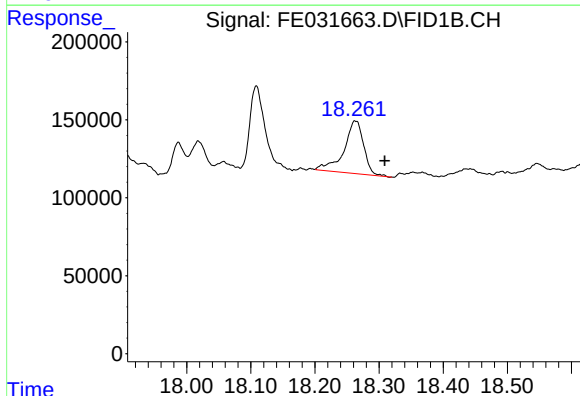


#14 N-DOTRIACONTANE

R.T.: 18.263 min
Delta R.T.: -0.045 min
Response: 721945
Conc: 1.82 ug/ml

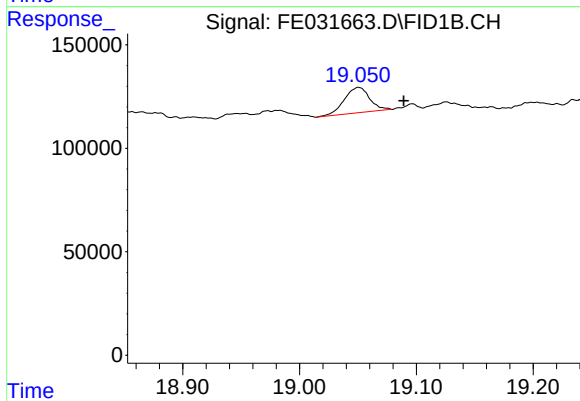

#15 N-TETRATRIACONTANE

R.T.: 19.050 min
Delta R.T.: -0.039 min
Response: 183708
Conc: 0.53 ug/ml

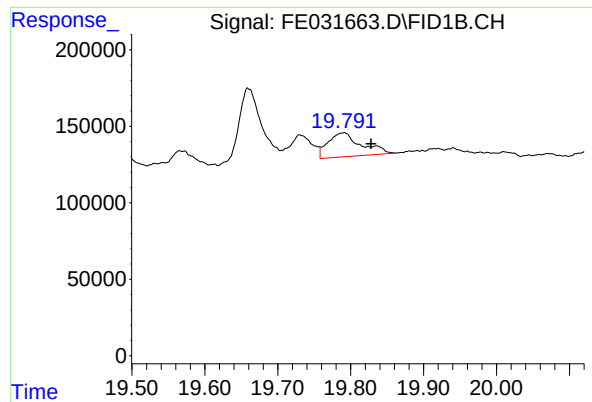

#16 N-HEXATRIACONTANE

R.T.: 19.790 min
Delta R.T.: -0.038 min
Response: 494621
Conc: 1.77 ug/ml

Instrument :
FID_E
ClientSampleId :