

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040220\  
Data File : FE031637.D  
Signal(s) : FID1B.CH  
Acq On : 02 Apr 2020 11:50  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Apr 03 00:32:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
Quant Title :  
QLast Update : Fri Mar 20 08:17:28 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.159  | 10709994 | 26.140 ug/ml |
| 12) N-OCTACOSANE            | 16.564 | 14194712 | 33.822 ug/ml |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040220\  
Data File : FE031637.D  
Signal(s) : FID1B.CH  
Acq On : 02 Apr 2020 11:50  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Apr 03 00:32:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
Quant Title :  
QLast Update : Fri Mar 20 08:17:28 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

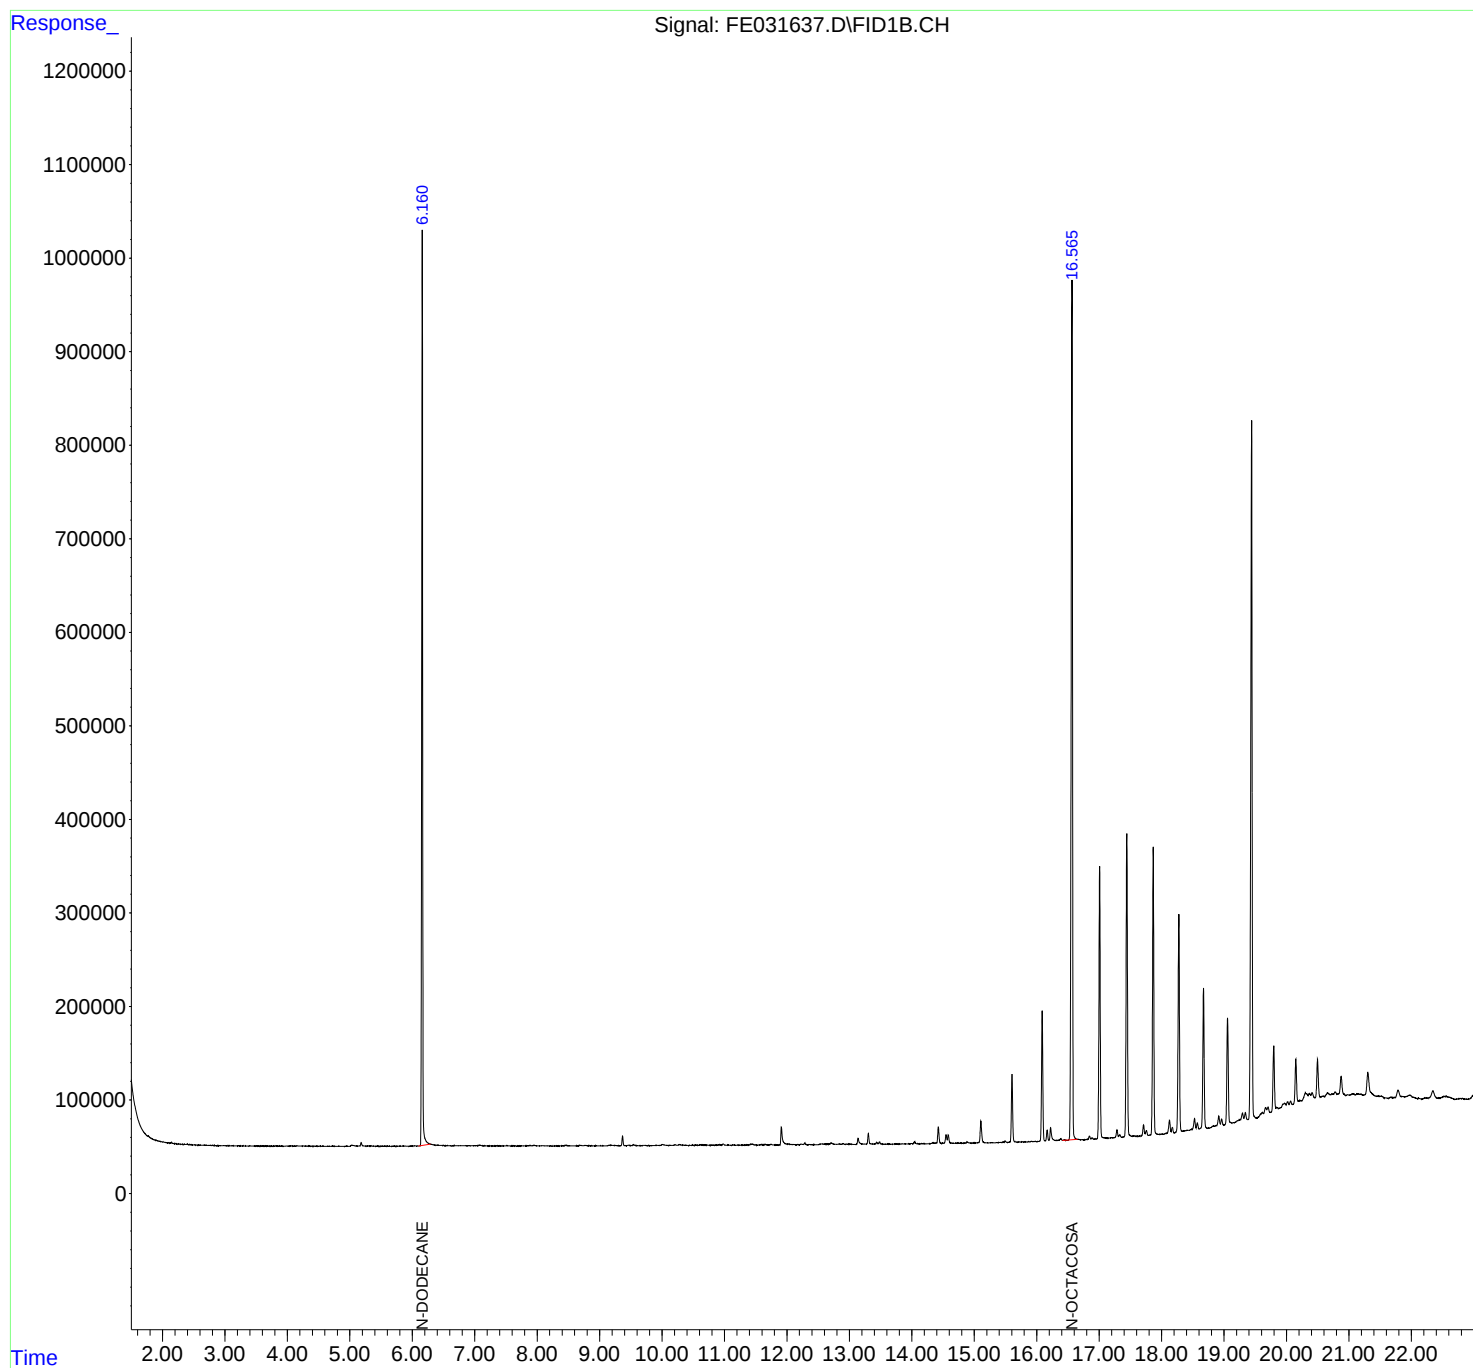


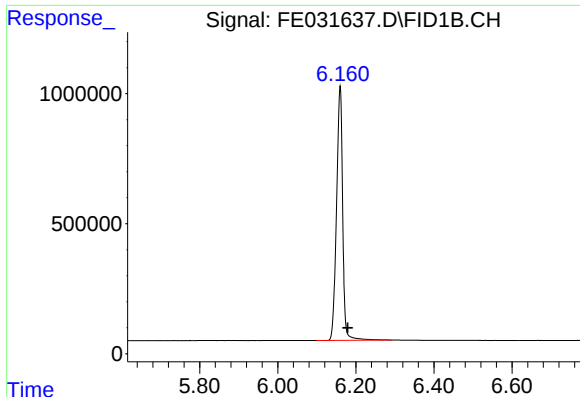

#3 N-DODECANE


R.T.: 6.159 min  
Delta R.T.: -0.020 min  
Response: 10709994  
Conc: 26.14 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

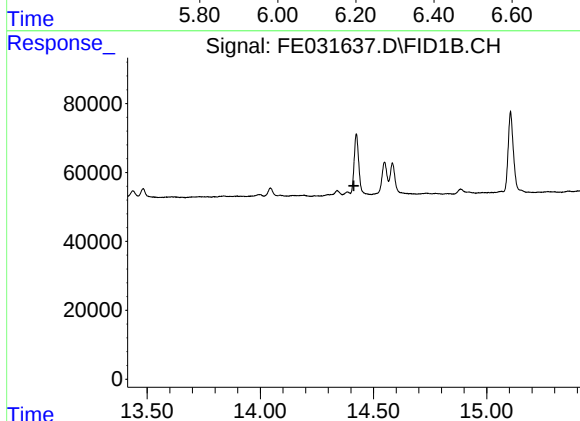

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.413 min  
Response: 0  
Conc: N.D.

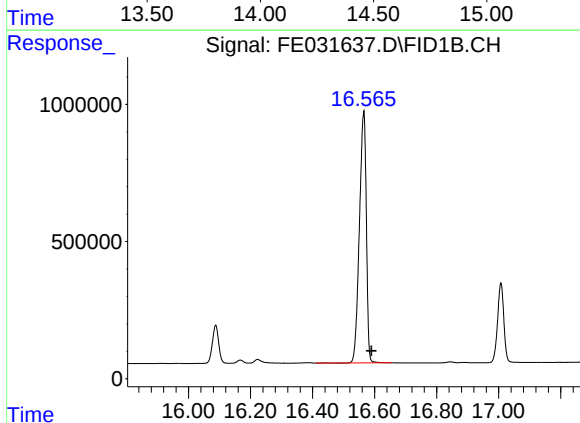

#12 N-OCTACOSANE

R.T.: 16.564 min  
Delta R.T.: -0.025 min  
Response: 14194712  
Conc: 33.82 ug/ml