

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040220\  
 Data File : FE031661.D  
 Signal(s) : FID1B.CH  
 Acq On : 03 Apr 2020 2:19  
 Operator : DD\AJ  
 Sample : L2129-12 5X  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 TP-7-A

Manual Integrations  
 APPROVED

Sohil  
 4/3/2020 4:16:22 PM

Integration File: autoint1.e  
 Quant Time: Apr 03 04:36:23 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
 Quant Title :  
 QLast Update : Fri Mar 20 08:17:28 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.387 | 4302192  | 11.657 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040220\  
Data File : FE031661.D  
Signal(s) : FID1B.CH  
Acq On : 03 Apr 2020 2:19  
Operator : DD\AJ  
Sample : L2129-12 5X  
Misc :  
ALS Vial : 24 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
TP-7-A


Manual Integrations  
APPROVED

Sohil  
4/3/2020 4:16:22 PM

Integration File: autoint1.e  
Quant Time: Apr 03 04:36:23 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE031020.M  
Quant Title :  
QLast Update : Fri Mar 20 08:17:28 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

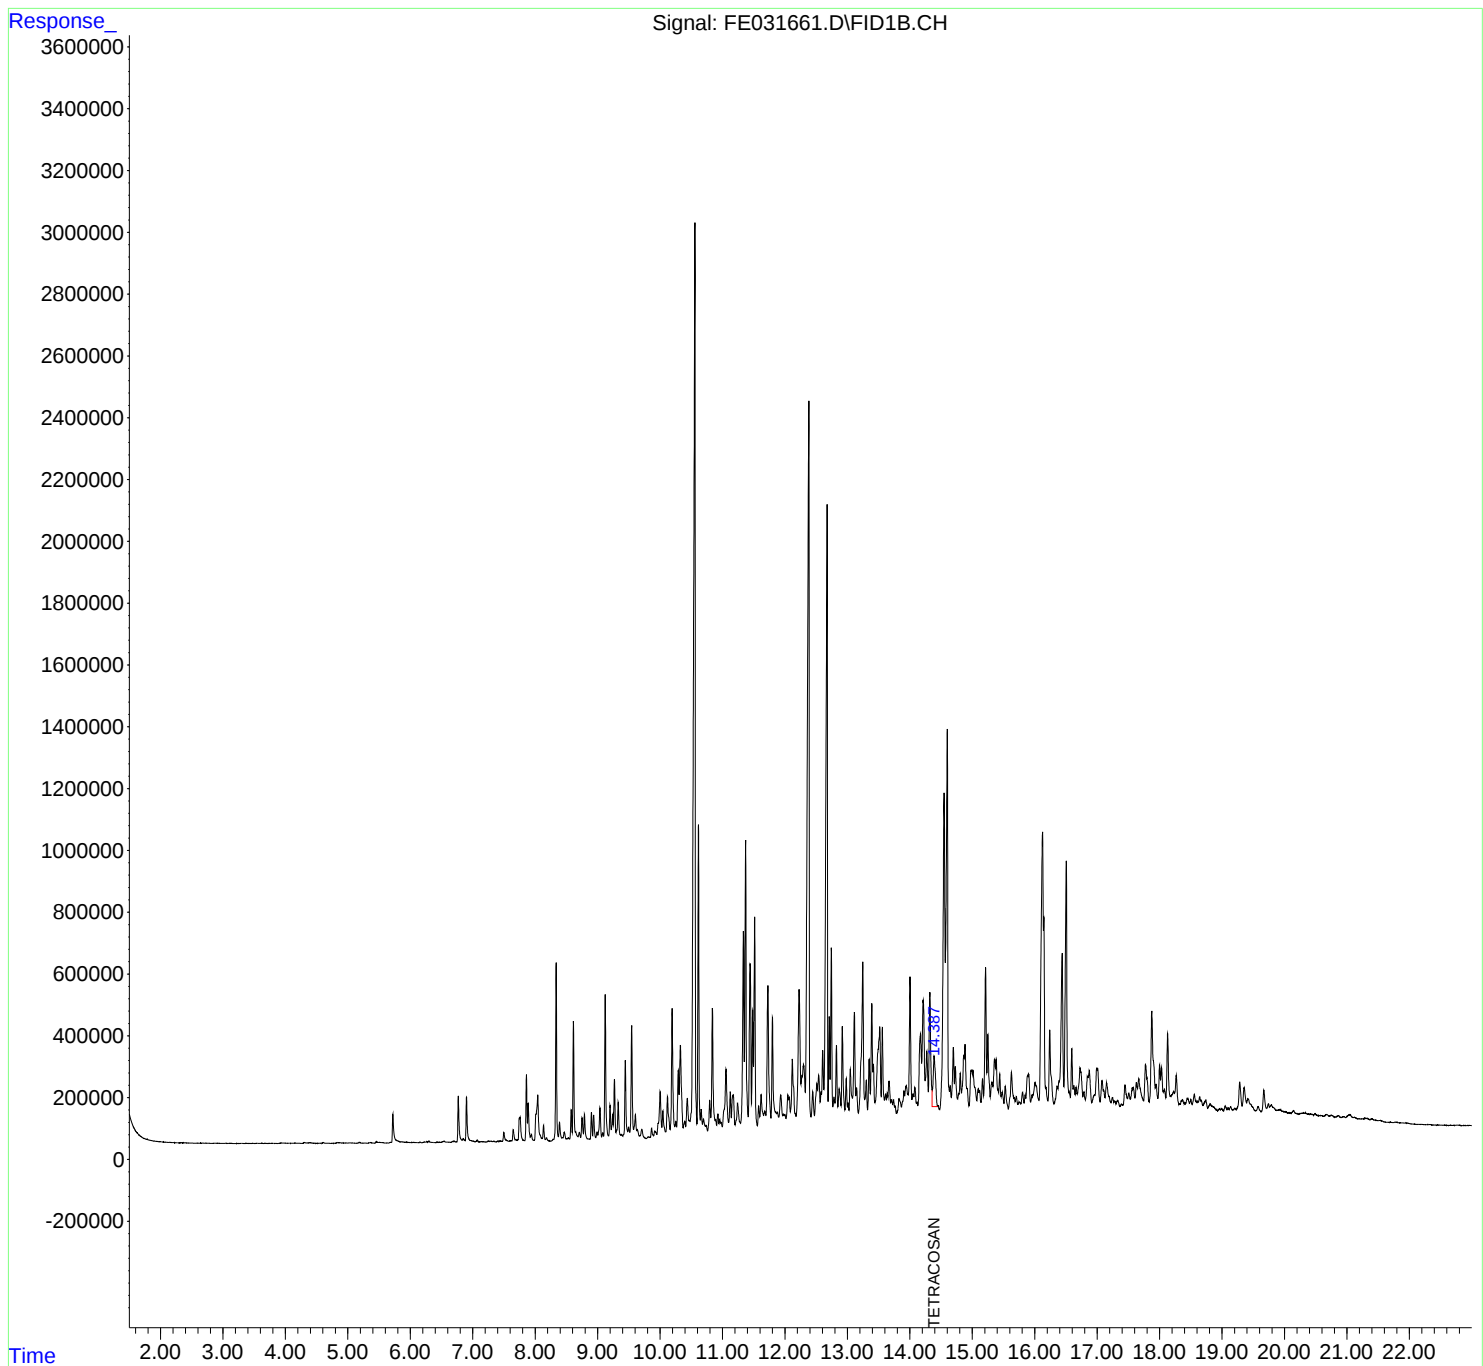

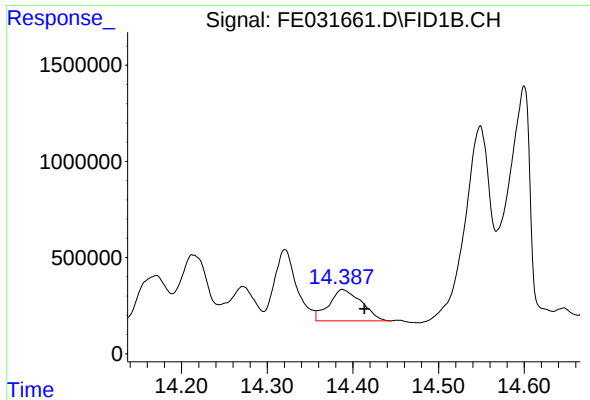

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.387 min  
Delta R.T.: -0.027 min  
Response: 4302192  
Conc: 11.66 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
TP-7-A

Manual Integrations  
APPROVED

Sohil  
4/3/2020 4:16:22 PM