

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040224AL\
 Data File : FE047422.D
 Signal(s) : FID1B.ch
 Acq On : 02 Apr 2024 01:48
 Operator : YP\AJ
 Sample : 10 PPM ALIPHATIC HC STD4
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 02 05:24:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 02 05:23:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.981	1740516	10.000 ug/ml
Spiked Amount 50.000		Recovery =	20.00%
12) S 1-chlorooctadecane (S...	13.414	1348078	10.000 ug/ml
Spiked Amount 50.000		Recovery =	20.00%
Target Compounds			
1) T n-Nonane (C9)	3.363	1592578	10.000 ug/ml
2) T n-Decane (C10)	4.615	1621111	10.000 ug/ml
3) T A~Naphthalene (C11.7)	6.323	1703897	10.000 ug/ml
4) T n-Dodecane (C12)	6.782	1629791	10.000 ug/ml
5) T A~2-methylnaphthalene...	7.419	1641302	10.000 ug/ml
6) T n-Tetradecane (C14)	8.609	1615638	10.000 ug/ml
7) T n-Hexadecane (C16)	10.217	1668301	10.000 ug/ml
8) T n-Octadecane (C18)	11.659	1685149	10.000 ug/ml
10) T n-Eicosane (C20)	12.968	1623521	10.000 ug/ml
11) T n-Heneicosane (C21)	13.580	1594323	10.000 ug/ml
13) T n-Docosane (C22)	14.167	1608267	10.000 ug/ml
14) T n-Tetracosane (C24)	15.268	1647049	10.000 ug/ml
15) T n-Hexacosane (C26)	16.287	1639553	10.000 ug/ml
16) T n-Octacosane (C28)	17.235	1639621	10.000 ug/ml
17) T n-Tricontane (C30)	18.121	1689327	10.000 ug/ml
18) T n-Dotriacontane (C32)	18.951	1672532	10.000 ug/ml
19) T n-Tetratriacontane (C34)	19.735	1603113	10.000 ug/ml
20) T n-Hexatriacontane (C36)	20.471	1594055	10.000 ug/ml
21) T n-Octatriacontane (C38)	21.214	1618036	10.000 ug/ml
22) T n-Tetracontane (C40)	22.144	1648316	10.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040224AL\
Data File : FE047422.D
Signal(s) : FID1B.ch
Acq On : 02 Apr 2024 01:48
Operator : YP\AJ
Sample : 10 PPM ALIPHATIC HC STD4
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 02 05:24:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
Quant Title : GC Extractables
QLast Update : Tue Apr 02 05:23:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

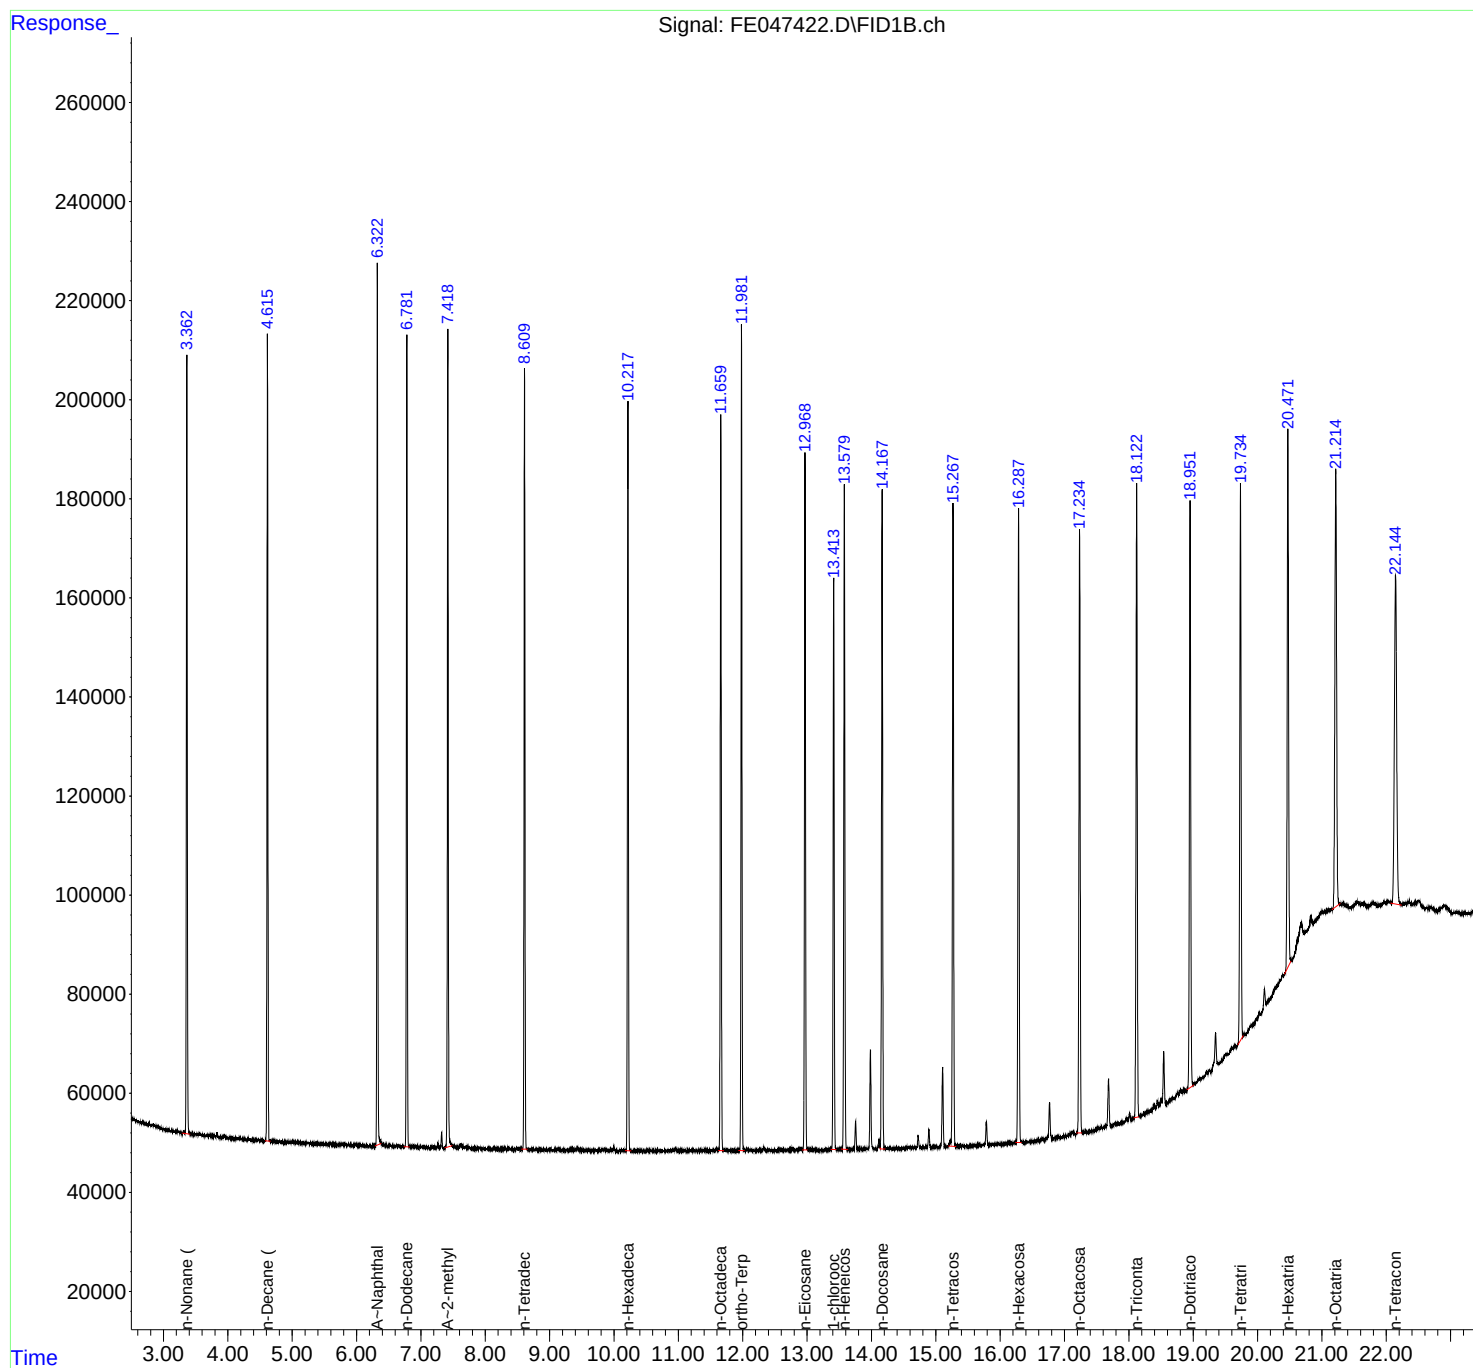


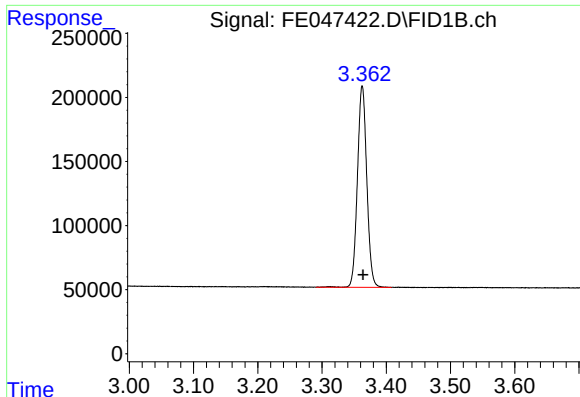

#1 n-Nonane (C9)


R.T.: 3.363 min
Delta R.T.: -0.001 min
Response: 1592578
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

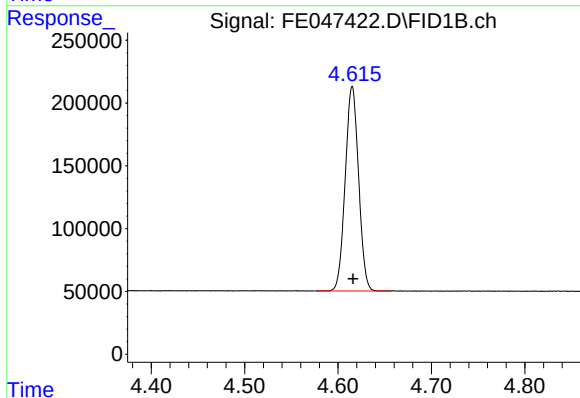


#2 n-Decane (C10)

R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 1621111
Conc: 10.00 ug/ml

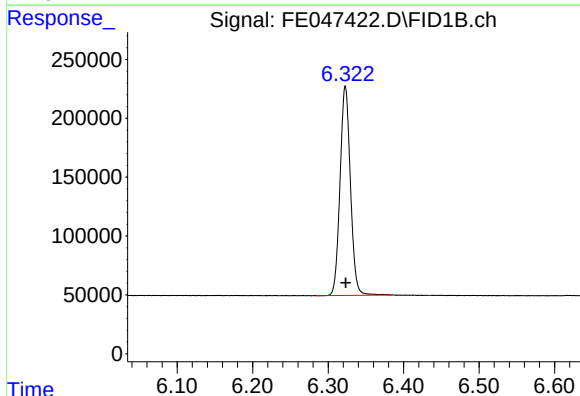


#3 A~Naphthalene (C11.7)

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 1703897
Conc: 10.00 ug/ml

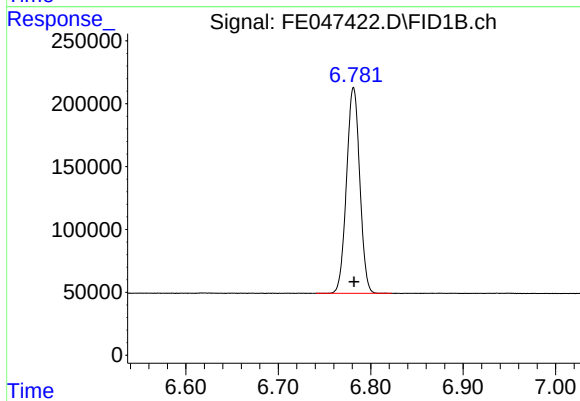

#4 n-Dodecane (C12)


R.T.: 6.782 min
Delta R.T.: 0.000 min
Response: 1629791
Conc: 10.00 ug/ml

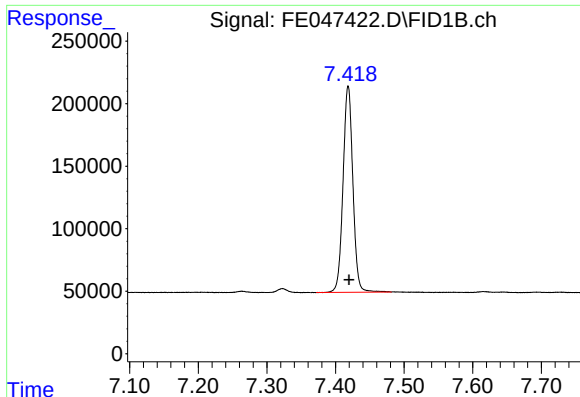

#5 A~2-methylnaphthalene (C12.89)


R.T.: 7.419 min
Delta R.T.: -0.001 min
Response: 1641302
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

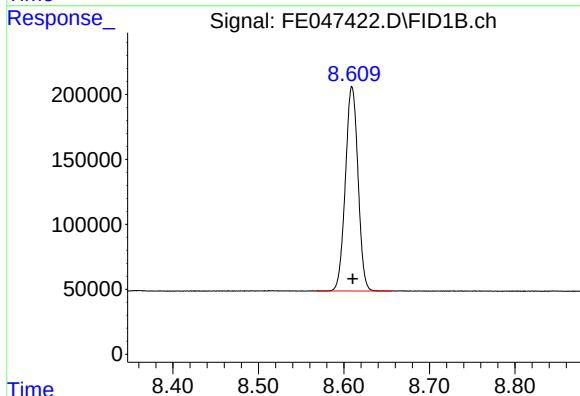


#6 n-Tetradecane (C14)

R.T.: 8.609 min
Delta R.T.: 0.000 min
Response: 1615638
Conc: 10.00 ug/ml

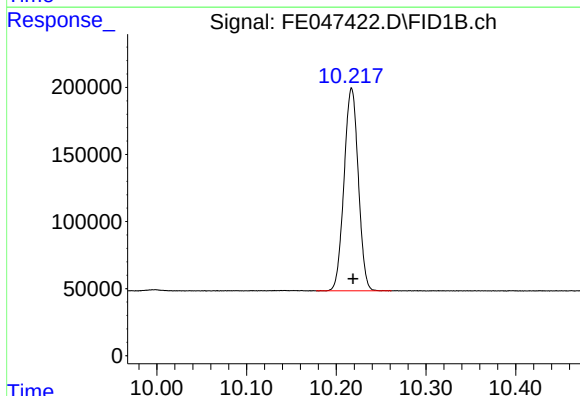


#7 n-Hexadecane (C16)

R.T.: 10.217 min
Delta R.T.: -0.001 min
Response: 1668301
Conc: 10.00 ug/ml

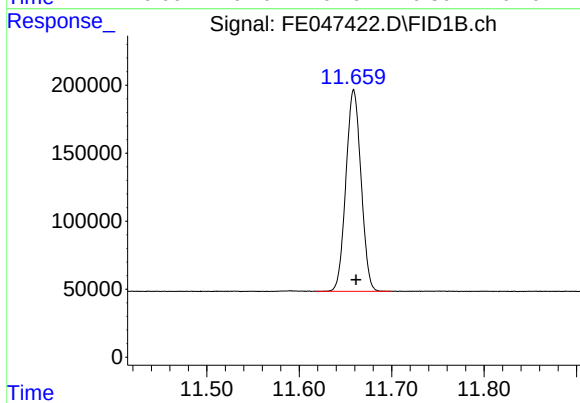

#8 n-Octadecane (C18)


R.T.: 11.659 min
Delta R.T.: -0.003 min
Response: 1685149
Conc: 10.00 ug/ml

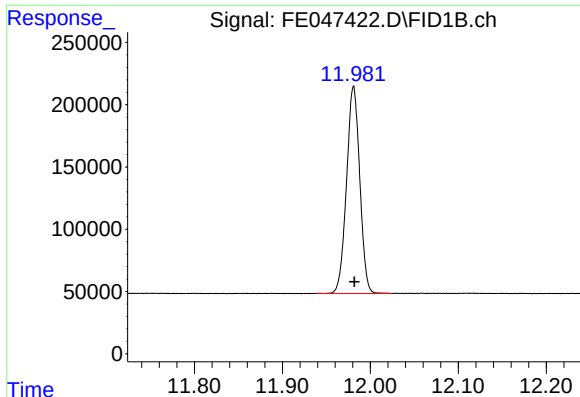

#9 ortho-Terphenyl (SURR)


R.T.: 11.981 min
Delta R.T.: -0.001 min
Response: 1740516
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

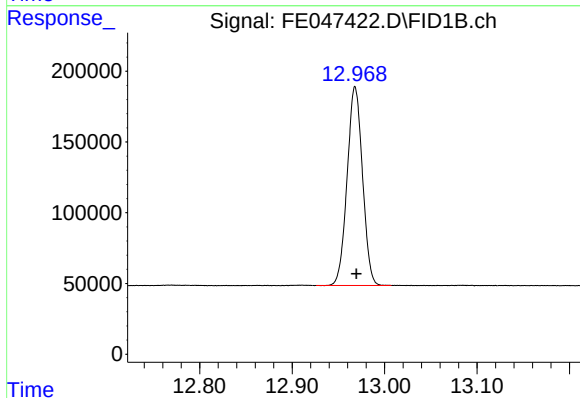


#10 n-Eicosane (C20)

R.T.: 12.968 min
Delta R.T.: -0.002 min
Response: 1623521
Conc: 10.00 ug/ml

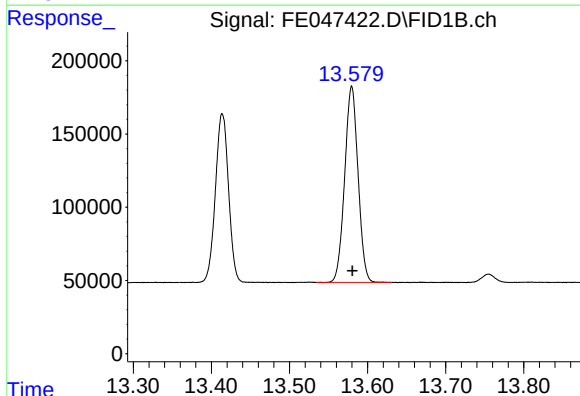


#11 n-Heneicosane (C21)

R.T.: 13.580 min
Delta R.T.: 0.000 min
Response: 1594323
Conc: 10.00 ug/ml

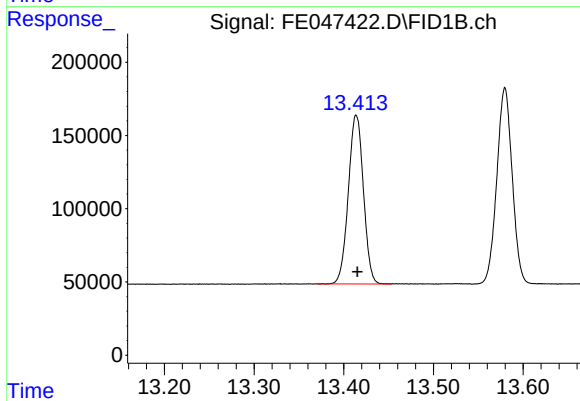

#12 1-chlorooctadecane (SURR)


R.T.: 13.414 min
Delta R.T.: -0.001 min
Response: 1348078
Conc: 10.00 ug/ml

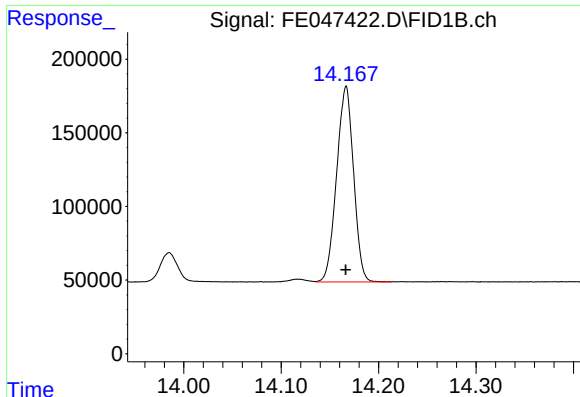

#13 n-Docosane (C22)


R.T.: 14.167 min
Delta R.T.: 0.000 min
Response: 1608267
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

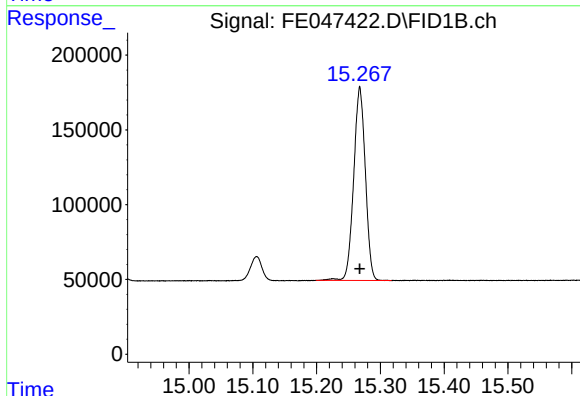


#14 n-Tetracosane (C24)

R.T.: 15.268 min
Delta R.T.: 0.000 min
Response: 1647049
Conc: 10.00 ug/ml

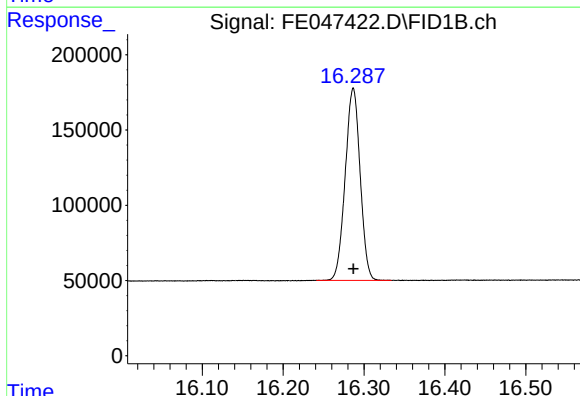


#15 n-Hexacosane (C26)

R.T.: 16.287 min
Delta R.T.: 0.000 min
Response: 1639553
Conc: 10.00 ug/ml

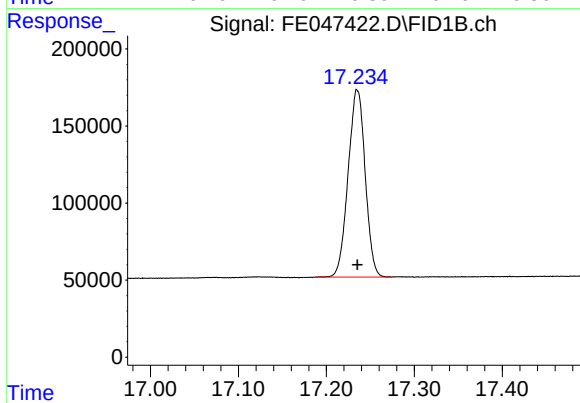

#16 n-Octacosane (C28)


R.T.: 17.235 min
Delta R.T.: 0.000 min
Response: 1639621
Conc: 10.00 ug/ml

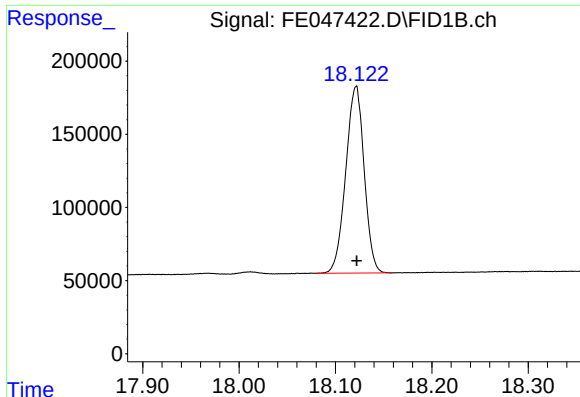

#17 n-Tricontane (C30)


R.T.: 18.121 min
Delta R.T.: 0.000 min
Response: 1689327
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

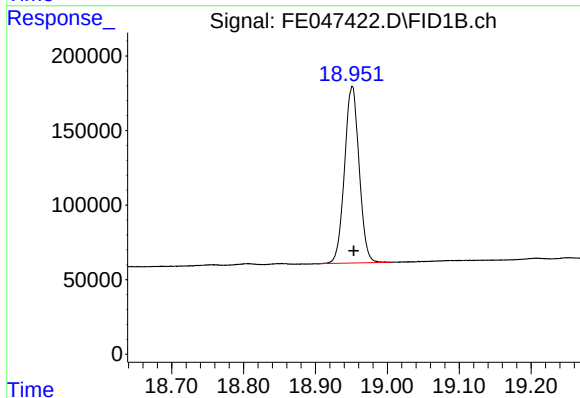


#18 n-Dotriacontane (C32)

R.T.: 18.951 min
Delta R.T.: -0.002 min
Response: 1672532
Conc: 10.00 ug/ml

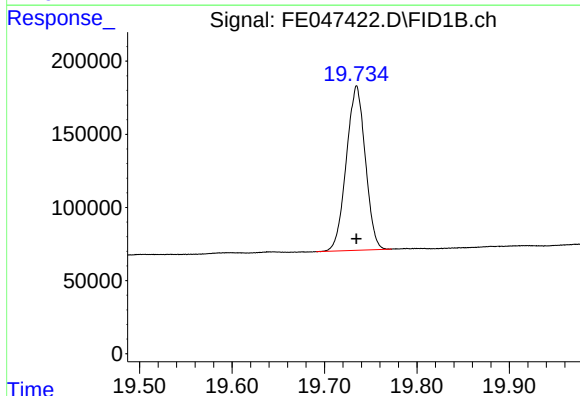


#19 n-Tetratriacontane (C34)

R.T.: 19.735 min
Delta R.T.: 0.000 min
Response: 1603113
Conc: 10.00 ug/ml

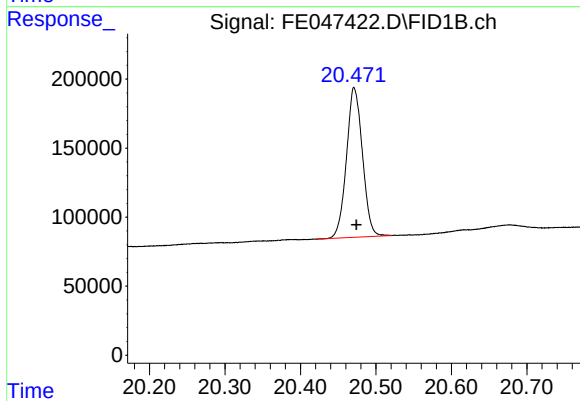

#20 n-Hexatriacontane (C36)


R.T.: 20.471 min
Delta R.T.: -0.003 min
Response: 1594055
Conc: 10.00 ug/ml

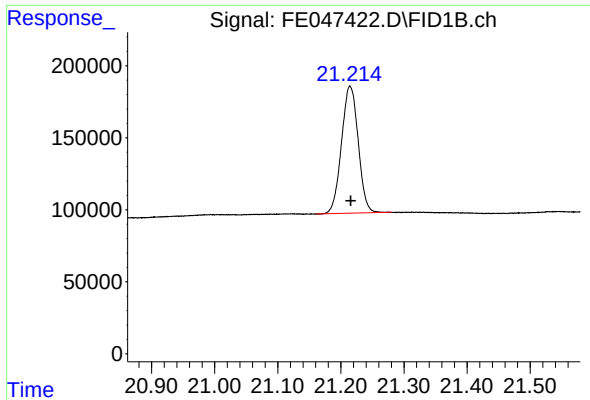

#21 n-Octatriacontane (C38)

R.T.: 21.214 min
Delta R.T.: -0.001 min
Response: 1618036
Conc: 10.00 ug/ml

Instrument :
FID_E
ClientSampleId :

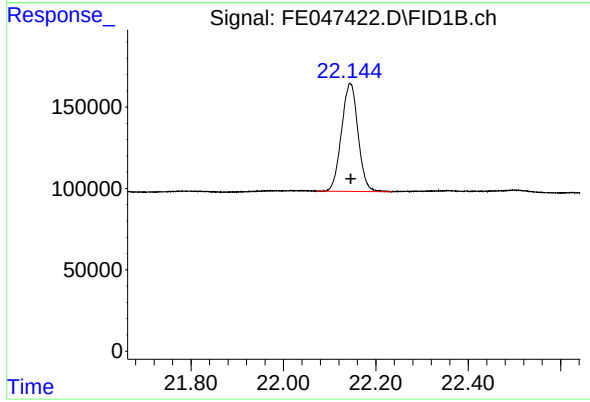

#22 n-Tetracontane (C40)

R.T.: 22.144 min
Delta R.T.: -0.002 min
Response: 1648316
Conc: 10.00 ug/ml