

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
 Data File : FE031670.D
 Signal(s) : FID1B.CH
 Acq On : 03 Apr 2020 9:02
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 23:55:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	209797	0.568 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.545	219172	0.522 ug/ml
13) N-TRIACONTANE	17.432	308916	0.739 ug/ml
14) N-DOTRIACONTANE	18.263	317454	0.801 ug/ml
15) N-TETRATRIACONTANE	19.044	161407	0.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031670.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 9:02
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 03 23:55:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

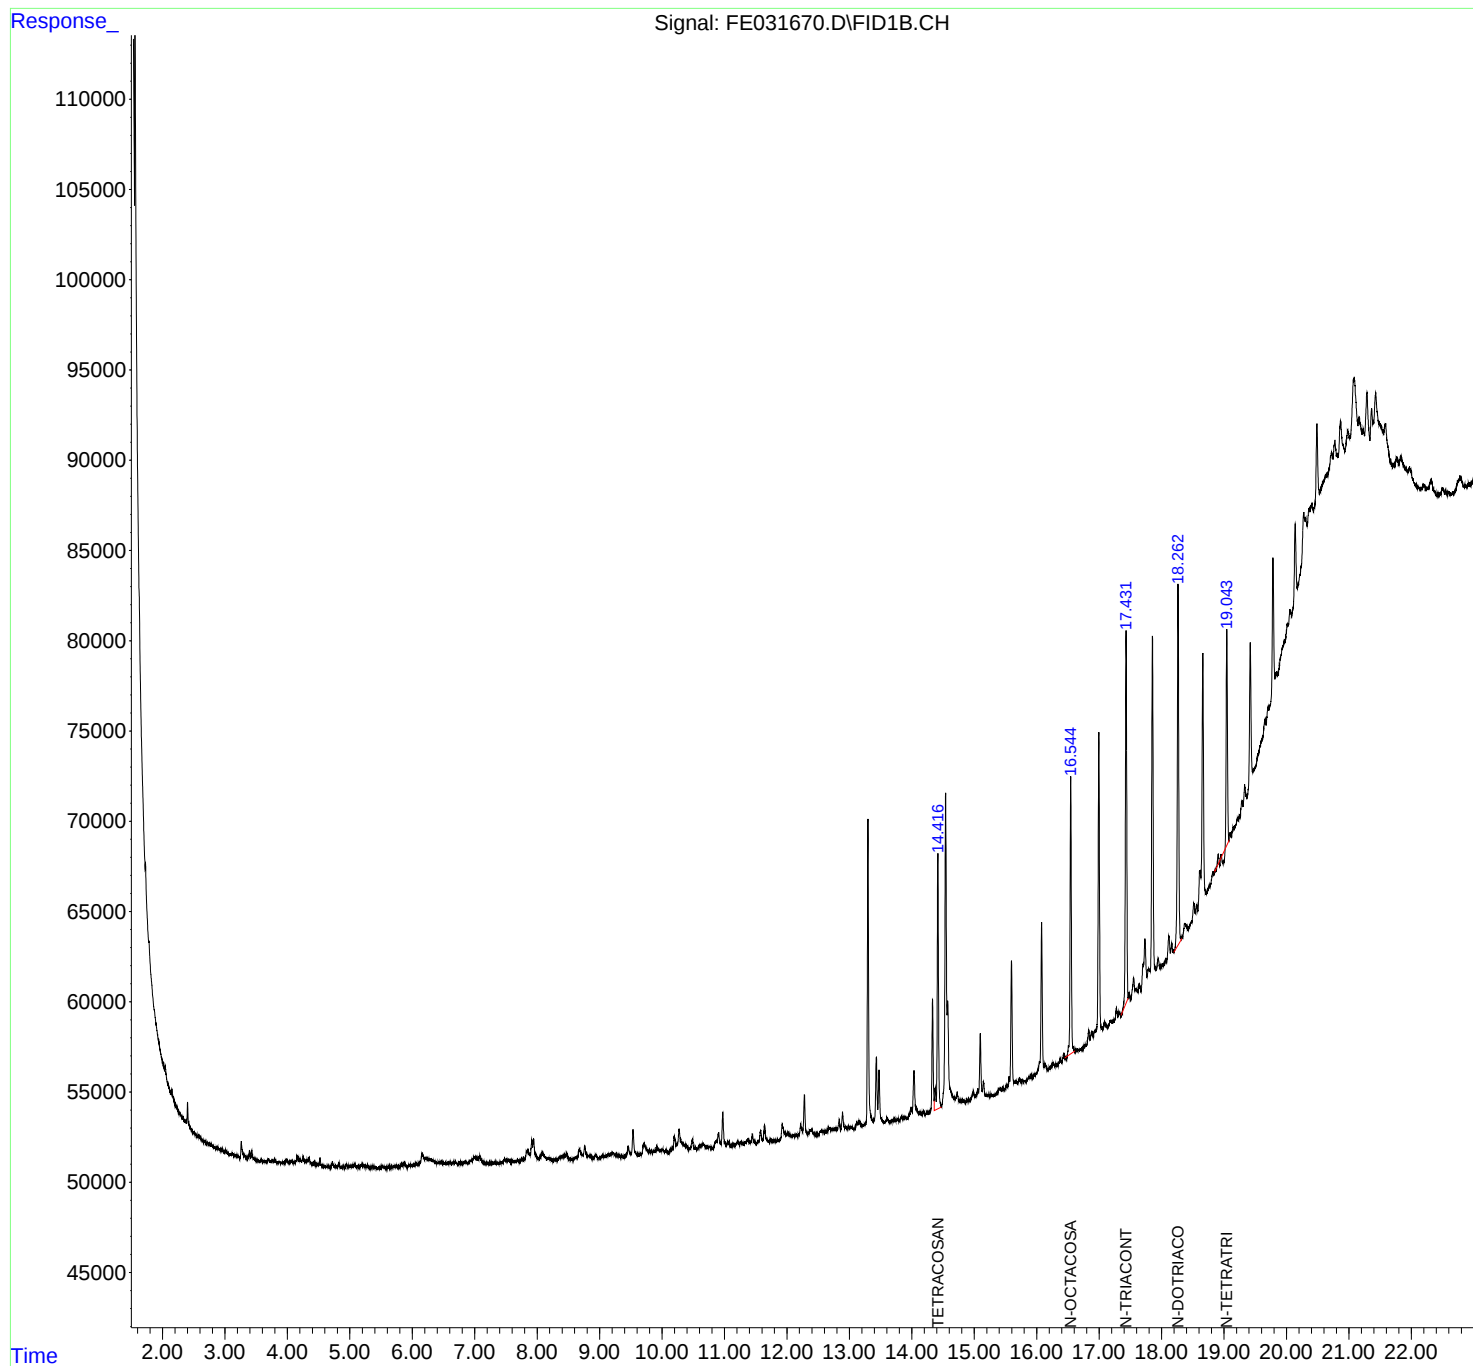


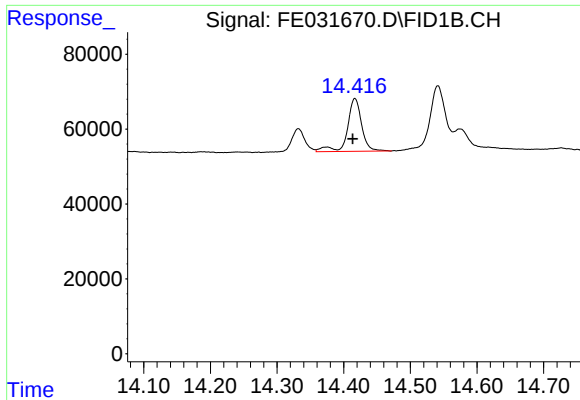

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.417 min
Delta R.T.: 0.003 min
Response: 209797
Conc: 0.57 ug/ml

Instrument :
FID_E
ClientSampleId :

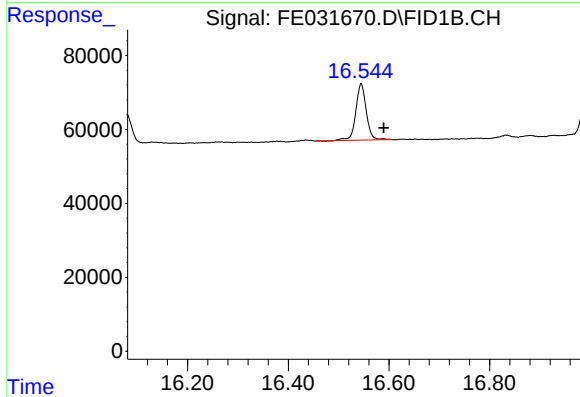


#12 N-OCTACOSANE

R.T.: 16.545 min
Delta R.T.: -0.045 min
Response: 219172
Conc: 0.52 ug/ml

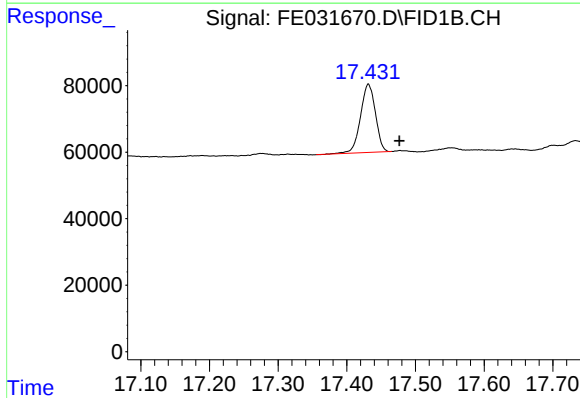


#13 N-TRIACONTANE

R.T.: 17.432 min
Delta R.T.: -0.045 min
Response: 308916
Conc: 0.74 ug/ml

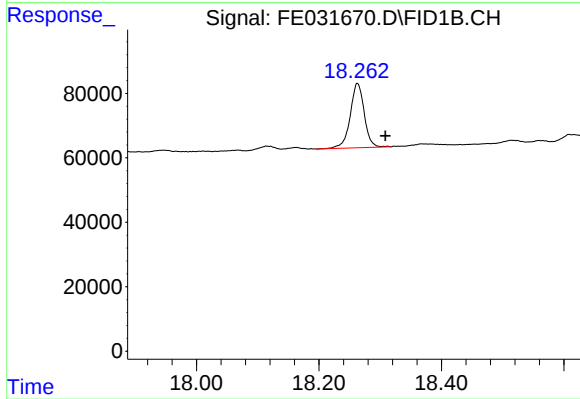

#14 N-DOTRIACONTANE

R.T.: 18.263 min
Delta R.T.: -0.046 min
Response: 317454
Conc: 0.80 ug/ml

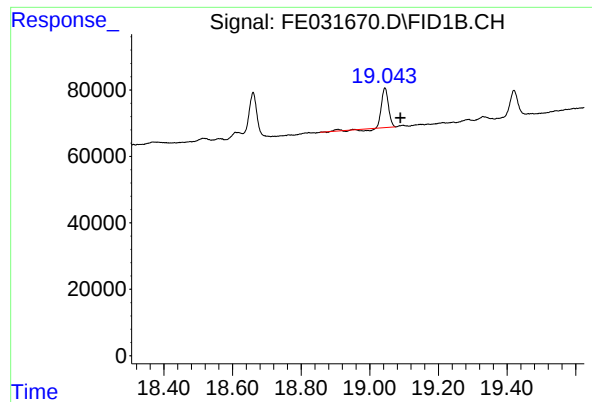

#15 N-TETRATRIACONTANE

R.T.: 19.044 min
Delta R.T.: -0.045 min
Response: 161407
Conc: 0.47 ug/ml

Instrument :
FID_E
ClientSampleId :