

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
 Data File : FE031683.D
 Signal(s) : FID1B.CH
 Acq On : 03 Apr 2020 17:18
 Operator : DD\AJ
 Sample : L2135-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 23:57:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.373	3634149	9.847 ug/ml
Target Compounds			
4) N-TETRADECANE	8.004	1343735	3.231 ug/ml
10) N-TETRACOSANE	14.572	278656	0.654 ug/ml
11) N-HEXACOSANE	15.592	423874	1.009 ug/ml
12) N-OCTACOSANE	16.542	488476	1.164 ug/ml
13) N-TRIACONTANE	17.427	482194	1.154 ug/ml
14) N-DOTRIACONTANE	18.257f	392516	0.990 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031683.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 17:18
Operator : DD\AJ
Sample : L2135-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 23:57:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

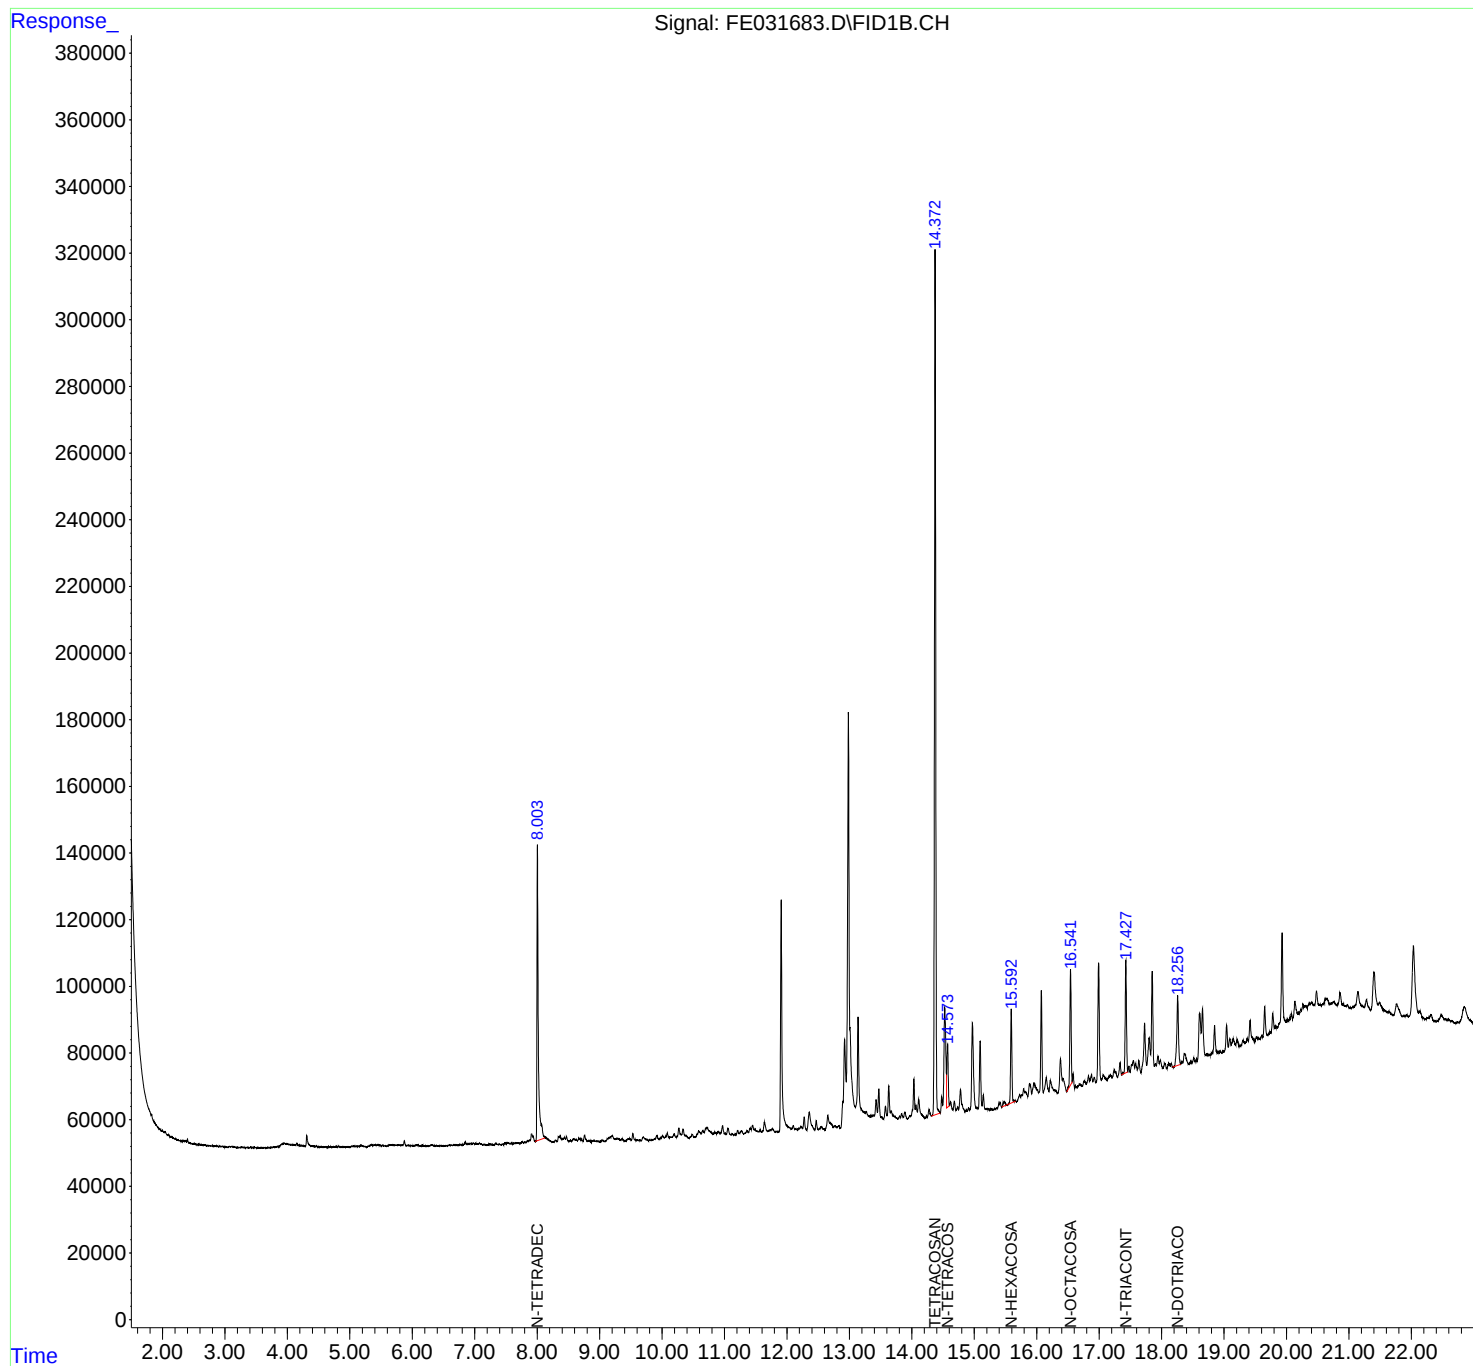


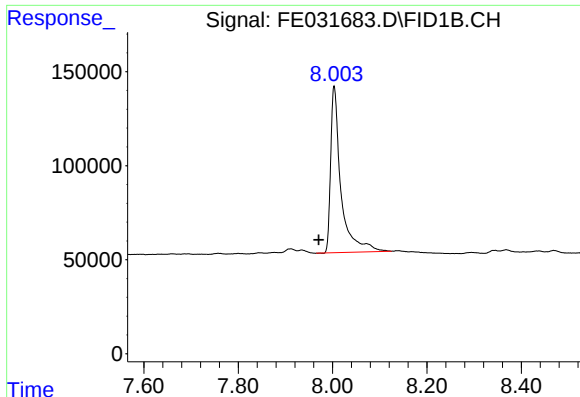

#4 N-TETRADECANE


R.T.: 8.004 min
Delta R.T.: 0.033 min
Response: 1343735
Conc: 3.23 ug/ml

Instrument :
FID_E
ClientSampleId :

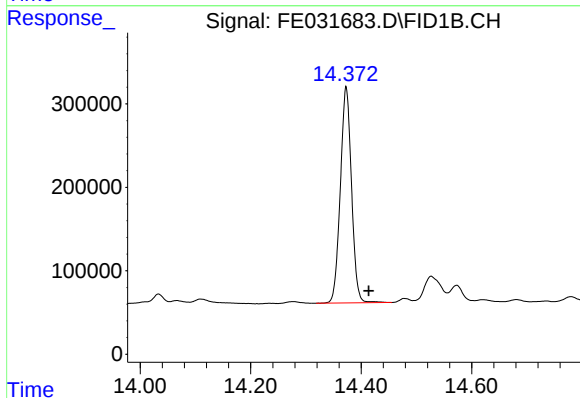


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.373 min
Delta R.T.: -0.041 min
Response: 3634149
Conc: 9.85 ug/ml

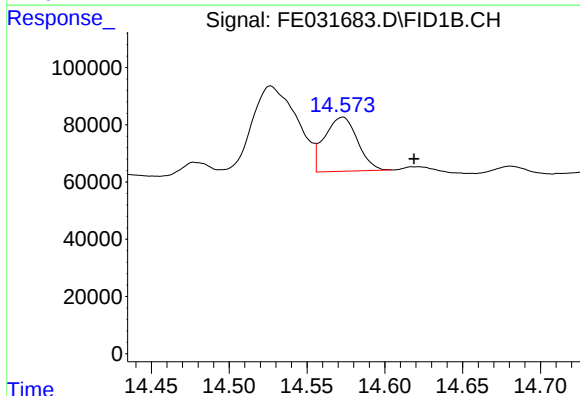


#10 N-TETRACOSANE

R.T.: 14.572 min
Delta R.T.: -0.046 min
Response: 278656
Conc: 0.65 ug/ml

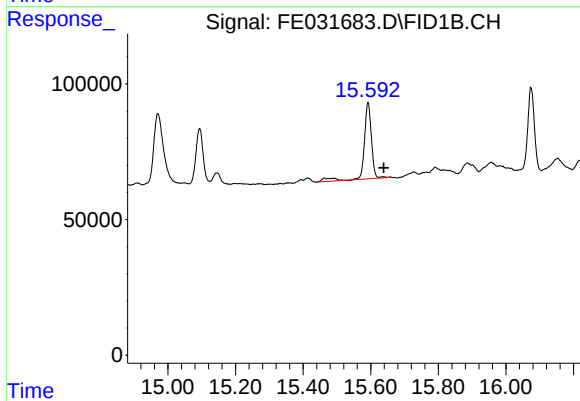

#11 N-HEXACOSANE


R.T.: 15.592 min
Delta R.T.: -0.046 min
Response: 423874
Conc: 1.01 ug/ml

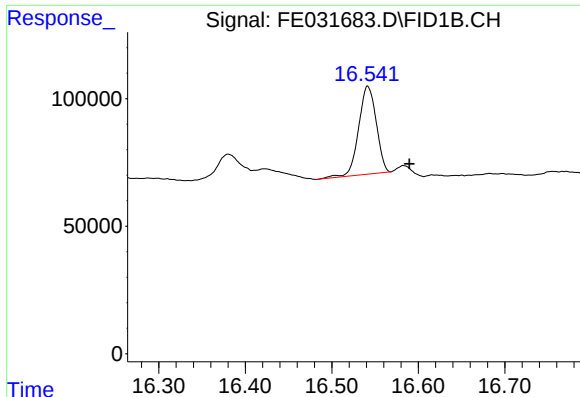

#12 N-OCTACOSANE


R.T.: 16.542 min
Delta R.T.: -0.048 min
Response: 488476
Conc: 1.16 ug/ml

Instrument :
FID_E
ClientSampleId :

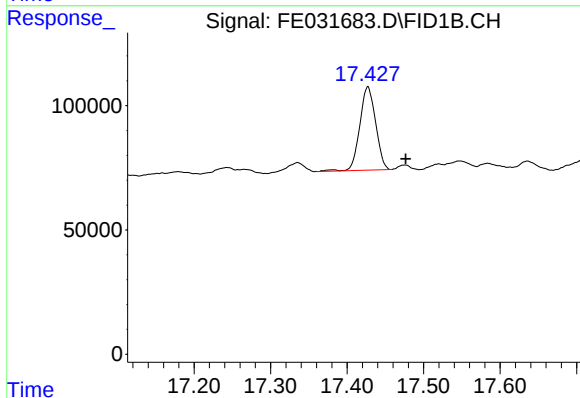

#13 N-TRIACONTANE

R.T.: 17.427 min
Delta R.T.: -0.049 min
Response: 482194
Conc: 1.15 ug/ml

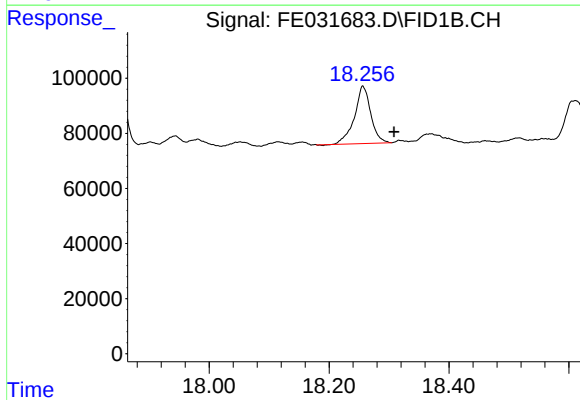

#14 N-DOTRIACONTANE

R.T.: 18.257 min
Delta R.T.: -0.052 min
Response: 392516
Conc: 0.99 ug/ml