

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
 Data File : FE031685.D
 Signal(s) : FID1B.CH
 Acq On : 03 Apr 2020 18:25
 Operator : DD\AJ
 Sample : L2135-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 23:58:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.375	7060079	19.129 ug/ml
Target Compounds			
4) N-TETRADECANE	8.004	2871355	6.904 ug/ml
8) N-DOCOSANE	13.472	212039	0.497 ug/ml
10) N-TETRACOSANE	14.573	434024	1.019 ug/ml
11) N-HEXACOSANE	15.593	652391	1.553 ug/ml
12) N-OCTACOSANE	16.541	766290	1.826 ug/ml
13) N-TRIACONTANE	17.428	694656	1.662 ug/ml
14) N-DOTRIACONTANE	18.258f	467303	1.179 ug/ml
16) N-HEXATRIACONTANE	19.781	279364	1.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031685.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 18:25
Operator : DD\AJ
Sample : L2135-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 23:58:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

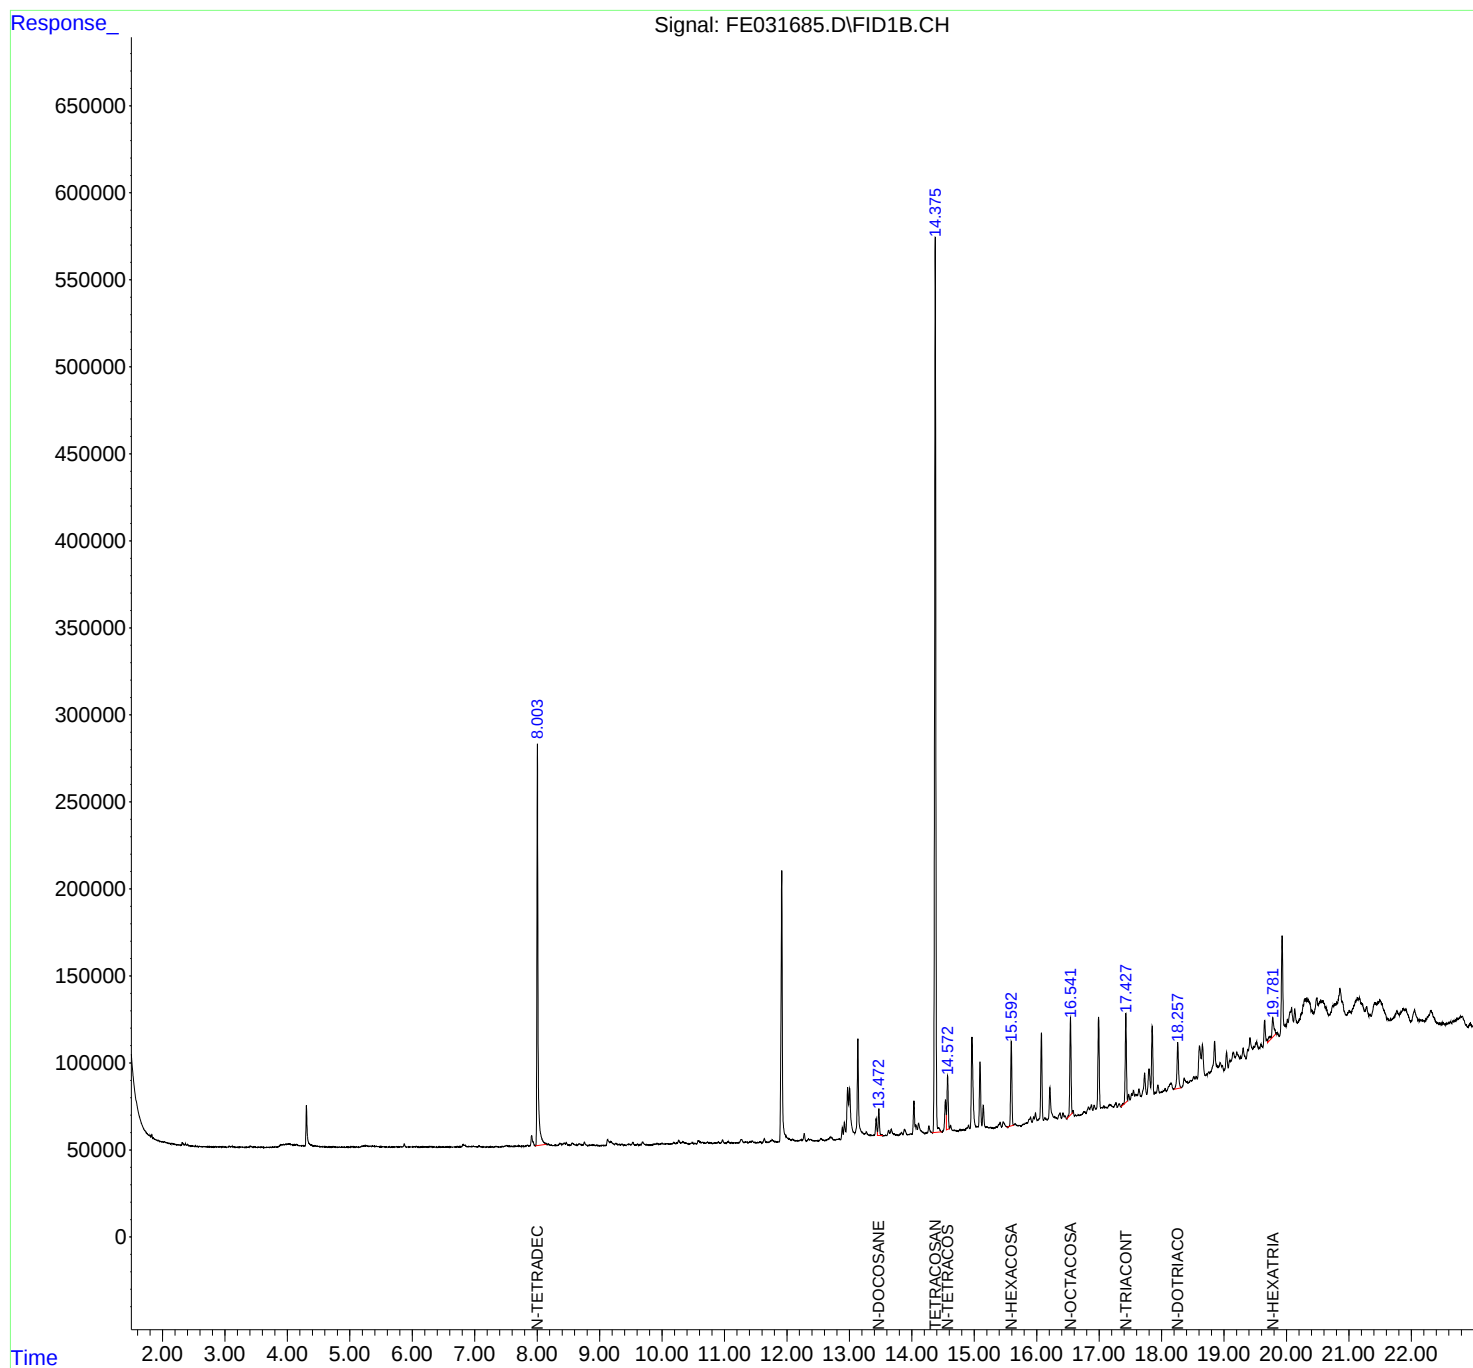


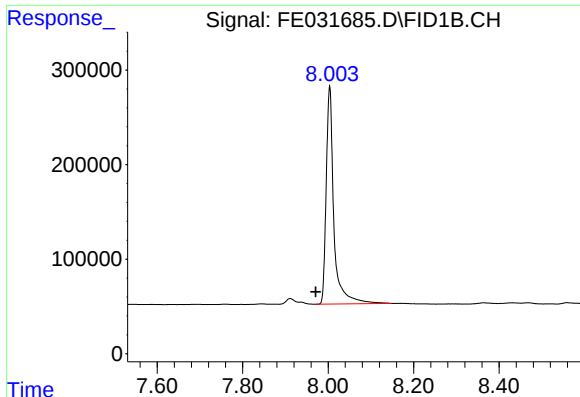

#4 N-TETRADECANE


R.T.: 8.004 min
Delta R.T.: 0.033 min
Response: 2871355
Conc: 6.90 ug/ml

Instrument :
FID_E
ClientSampleId :

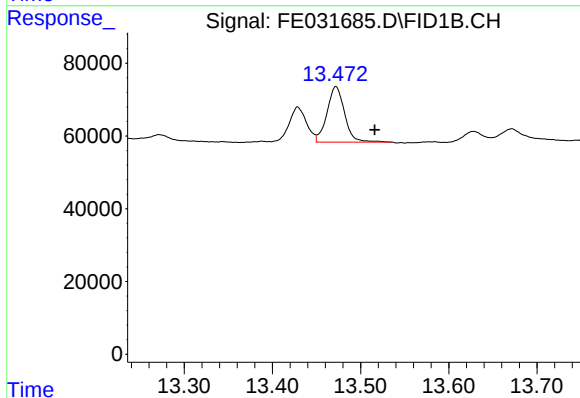


#8 N-DOCOSANE

R.T.: 13.472 min
Delta R.T.: -0.044 min
Response: 212039
Conc: 0.50 ug/ml

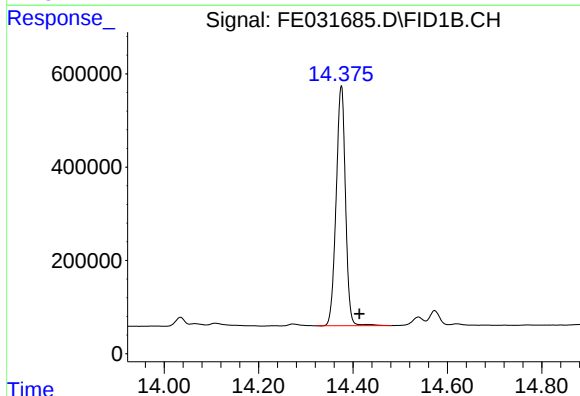


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.375 min
Delta R.T.: -0.038 min
Response: 7060079
Conc: 19.13 ug/ml

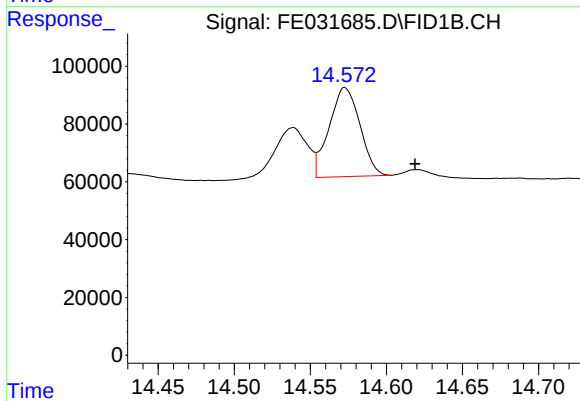

#10 N-TETRACOSANE


R.T.: 14.573 min
Delta R.T.: -0.046 min
Response: 434024
Conc: 1.02 ug/ml

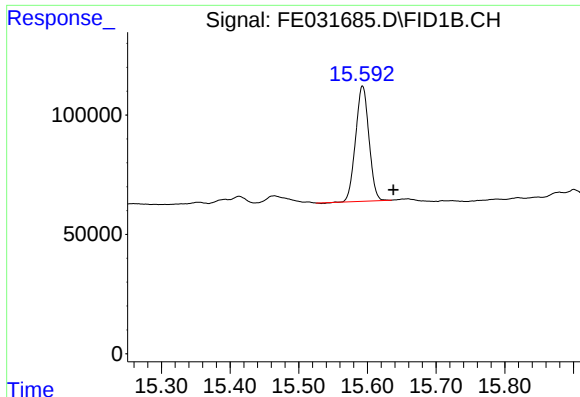

#11 N-HEXACOSANE


R.T.: 15.593 min
Delta R.T.: -0.045 min
Response: 652391
Conc: 1.55 ug/ml

Instrument :
FID_E
ClientSampleId :

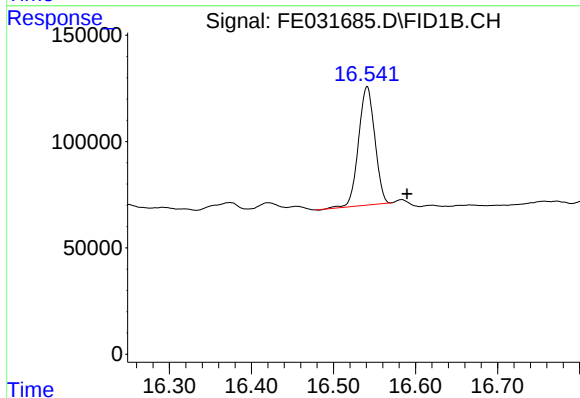


#12 N-OCTACOSANE

R.T.: 16.541 min
Delta R.T.: -0.049 min
Response: 766290
Conc: 1.83 ug/ml

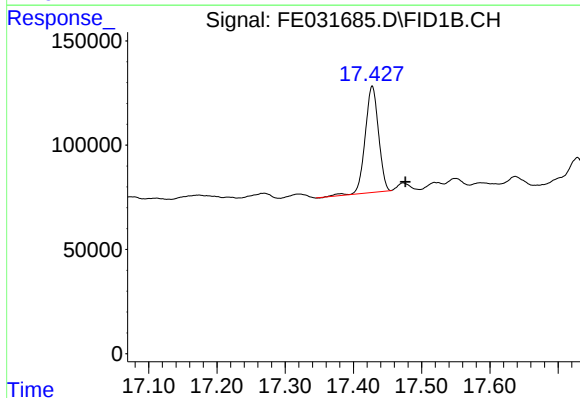


#13 N-TRIACONTANE

R.T.: 17.428 min
Delta R.T.: -0.049 min
Response: 694656
Conc: 1.66 ug/ml

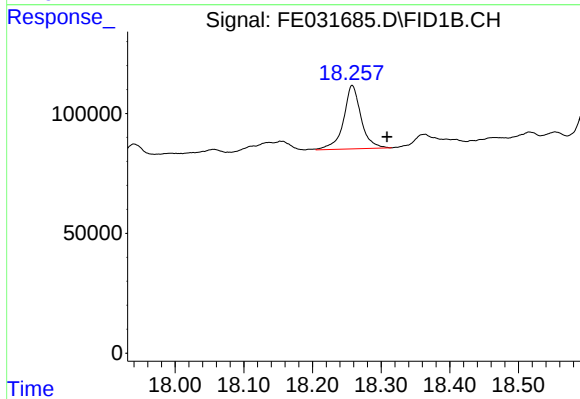

#14 N-DOTRIACONTANE

R.T.: 18.258 min
Delta R.T.: -0.051 min
Response: 467303
Conc: 1.18 ug/ml

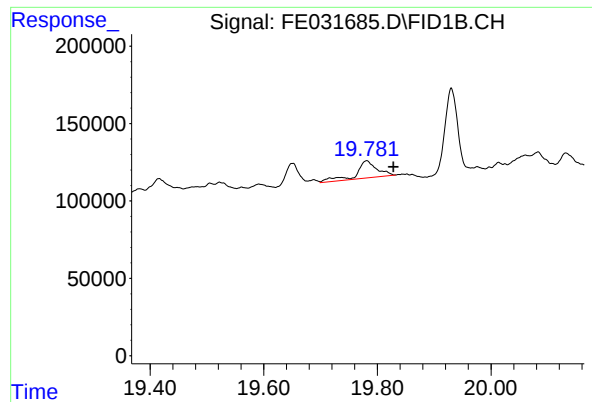

#16 N-HEXATRIACONTANE

R.T.: 19.781 min
Delta R.T.: -0.047 min
Response: 279364
Conc: 1.00 ug/ml

Instrument :
FID_E
ClientSampleId :