

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
 Data File : FE031688.D
 Signal(s) : FID1B.CH
 Acq On : 03 Apr 2020 20:05
 Operator : DD\AJ
 Sample : L2135-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 03 23:58:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Fri Mar 20 08:17:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.376	7721500	20.921 ug/ml
Target Compounds			
4) N-TETRADECANE	8.003	2562032	6.160 ug/ml
7) N-EICOSANE	12.351	292353	0.684 ug/ml
8) N-DOCOSANE	13.472	213118	0.500 ug/ml
10) N-TETRACOSANE	14.573	614384	1.443 ug/ml
11) N-HEXACOSANE	15.592	836095	1.991 ug/ml
12) N-OCTACOSANE	16.540	1267878	3.021 ug/ml
13) N-TRIACONTANE	17.427	1248000	2.986 ug/ml
14) N-DOTRIACONTANE	18.258f	700053	1.767 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031688.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 20:05
Operator : DD\AJ
Sample : L2135-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 03 23:58:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

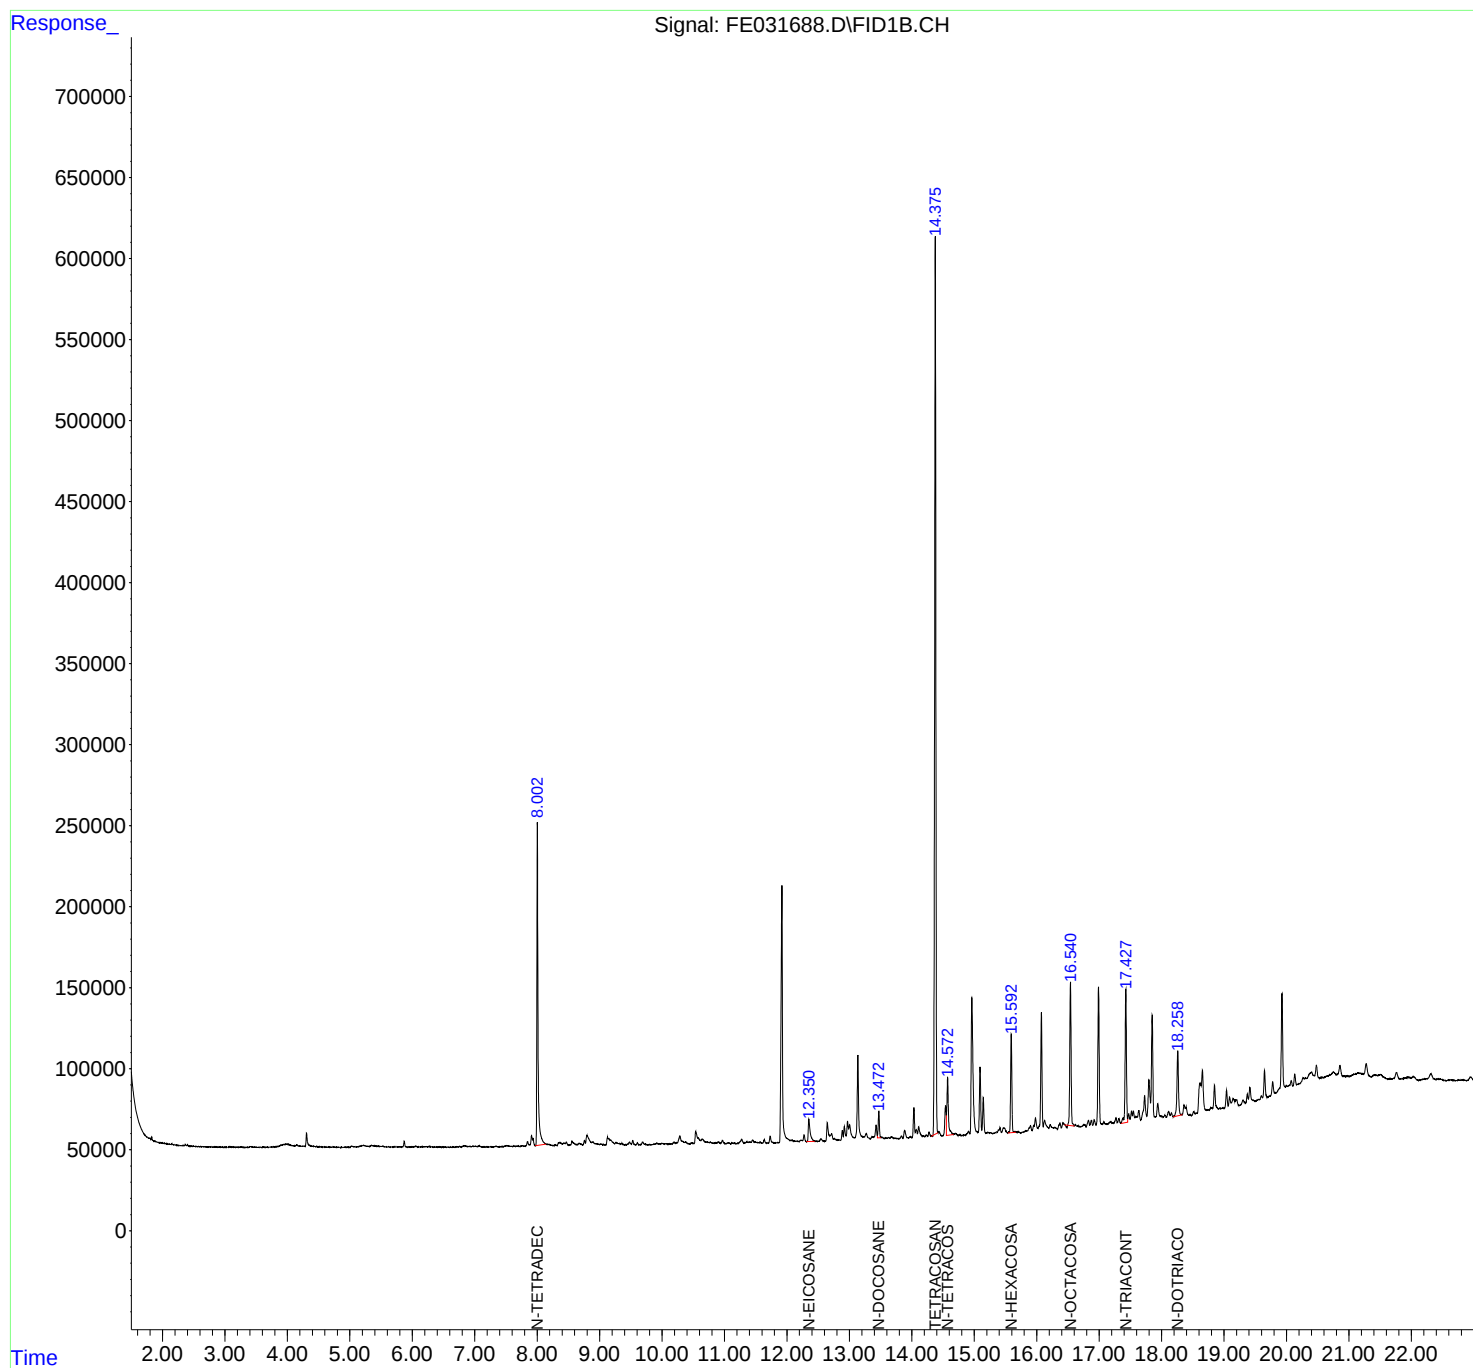


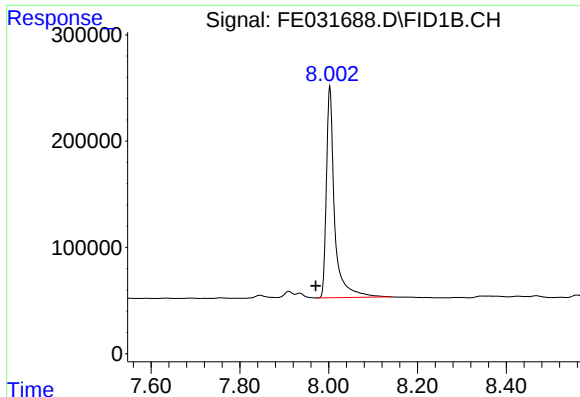

#4 N-TETRADECANE


R.T.: 8.003 min
Delta R.T.: 0.032 min
Response: 2562032
Conc: 6.16 ug/ml

Instrument :
FID_E
ClientSampleId :

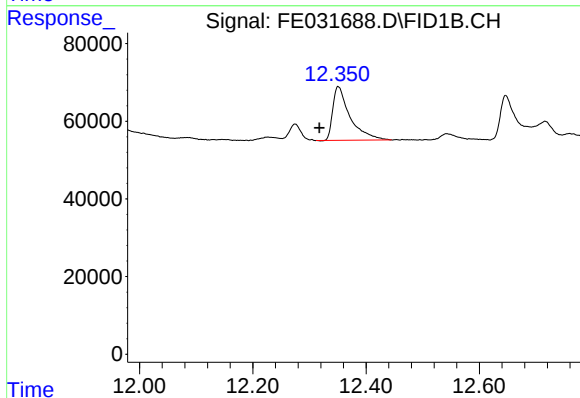


#7 N-EICOSANE

R.T.: 12.351 min
Delta R.T.: 0.034 min
Response: 292353
Conc: 0.68 ug/ml

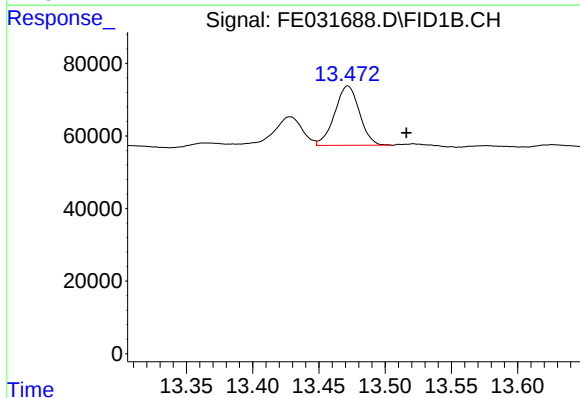


#8 N-DOCOSANE

R.T.: 13.472 min
Delta R.T.: -0.044 min
Response: 213118
Conc: 0.50 ug/ml

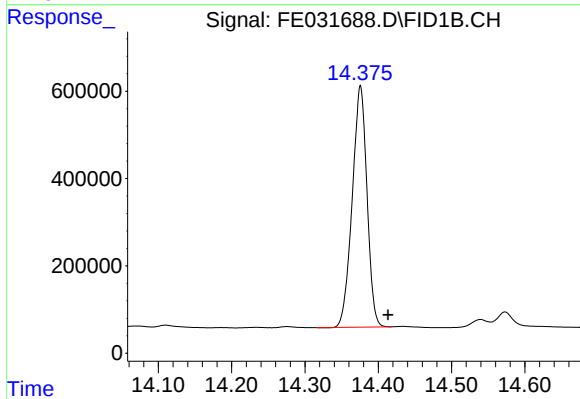

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.376 min
Delta R.T.: -0.038 min
Response: 7721500
Conc: 20.92 ug/ml

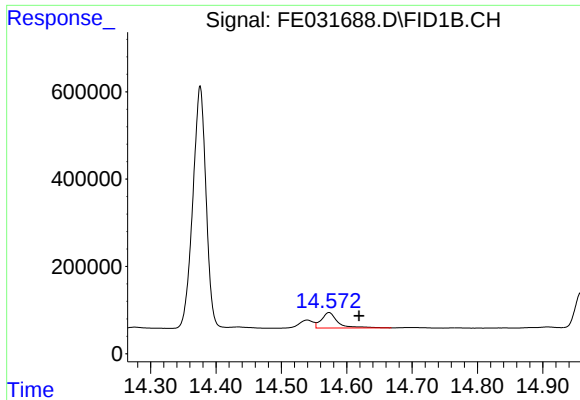

#10 N-TETRACOSANE


R.T.: 14.573 min
Delta R.T.: -0.046 min
Response: 614384
Conc: 1.44 ug/ml

Instrument :
FID_E
ClientSampleId :

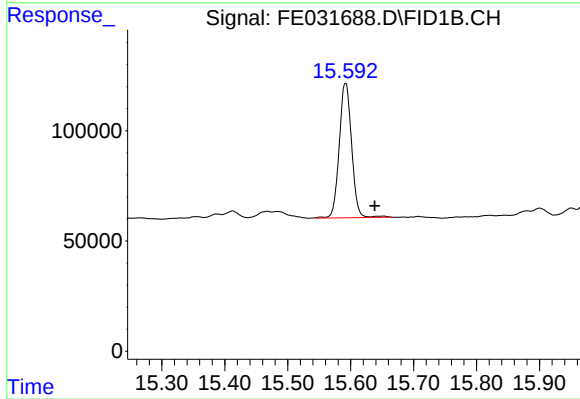


#11 N-HEXACOSANE

R.T.: 15.592 min
Delta R.T.: -0.046 min
Response: 836095
Conc: 1.99 ug/ml

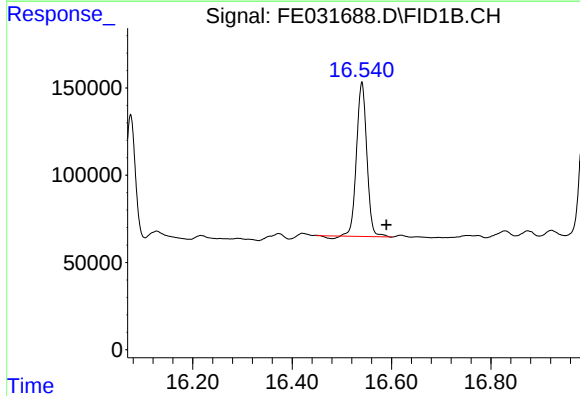


#12 N-OCTACOSANE

R.T.: 16.540 min
Delta R.T.: -0.049 min
Response: 1267878
Conc: 3.02 ug/ml

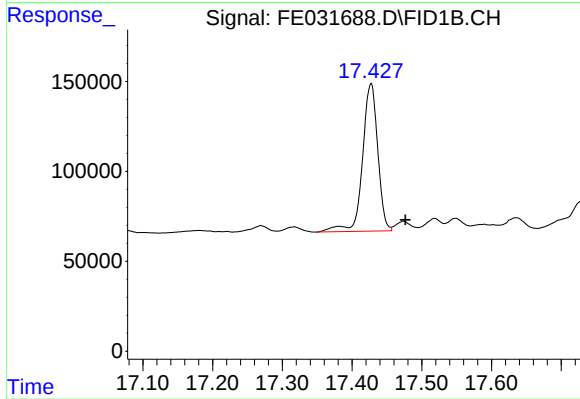

#13 N-TRIACONTANE

R.T.: 17.427 min
Delta R.T.: -0.050 min
Response: 1248000
Conc: 2.99 ug/ml

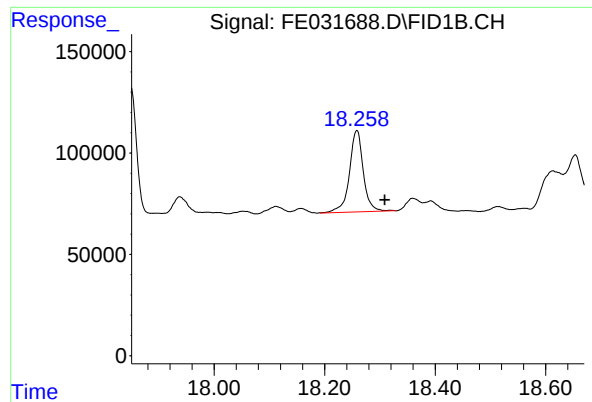

#14 N-DOTRIACONTANE

R.T.: 18.258 min
Delta R.T.: -0.051 min
Response: 700053
Conc: 1.77 ug/ml

Instrument :
FID_E
ClientSampleId :