

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031675.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 12:08
Operator : DD\AJ
Sample : L2129-42 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP-3-A

Integration File: Sample.e
Quant Time: Apr 03 23:56:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.376	3833267	10.386 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040320\
Data File : FE031675.D
Signal(s) : FID1B.CH
Acq On : 03 Apr 2020 12:08
Operator : DD\AJ
Sample : L2129-42 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP-3-A

Integration File: Sample.e
Quant Time: Apr 03 23:56:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Fri Mar 20 08:17:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

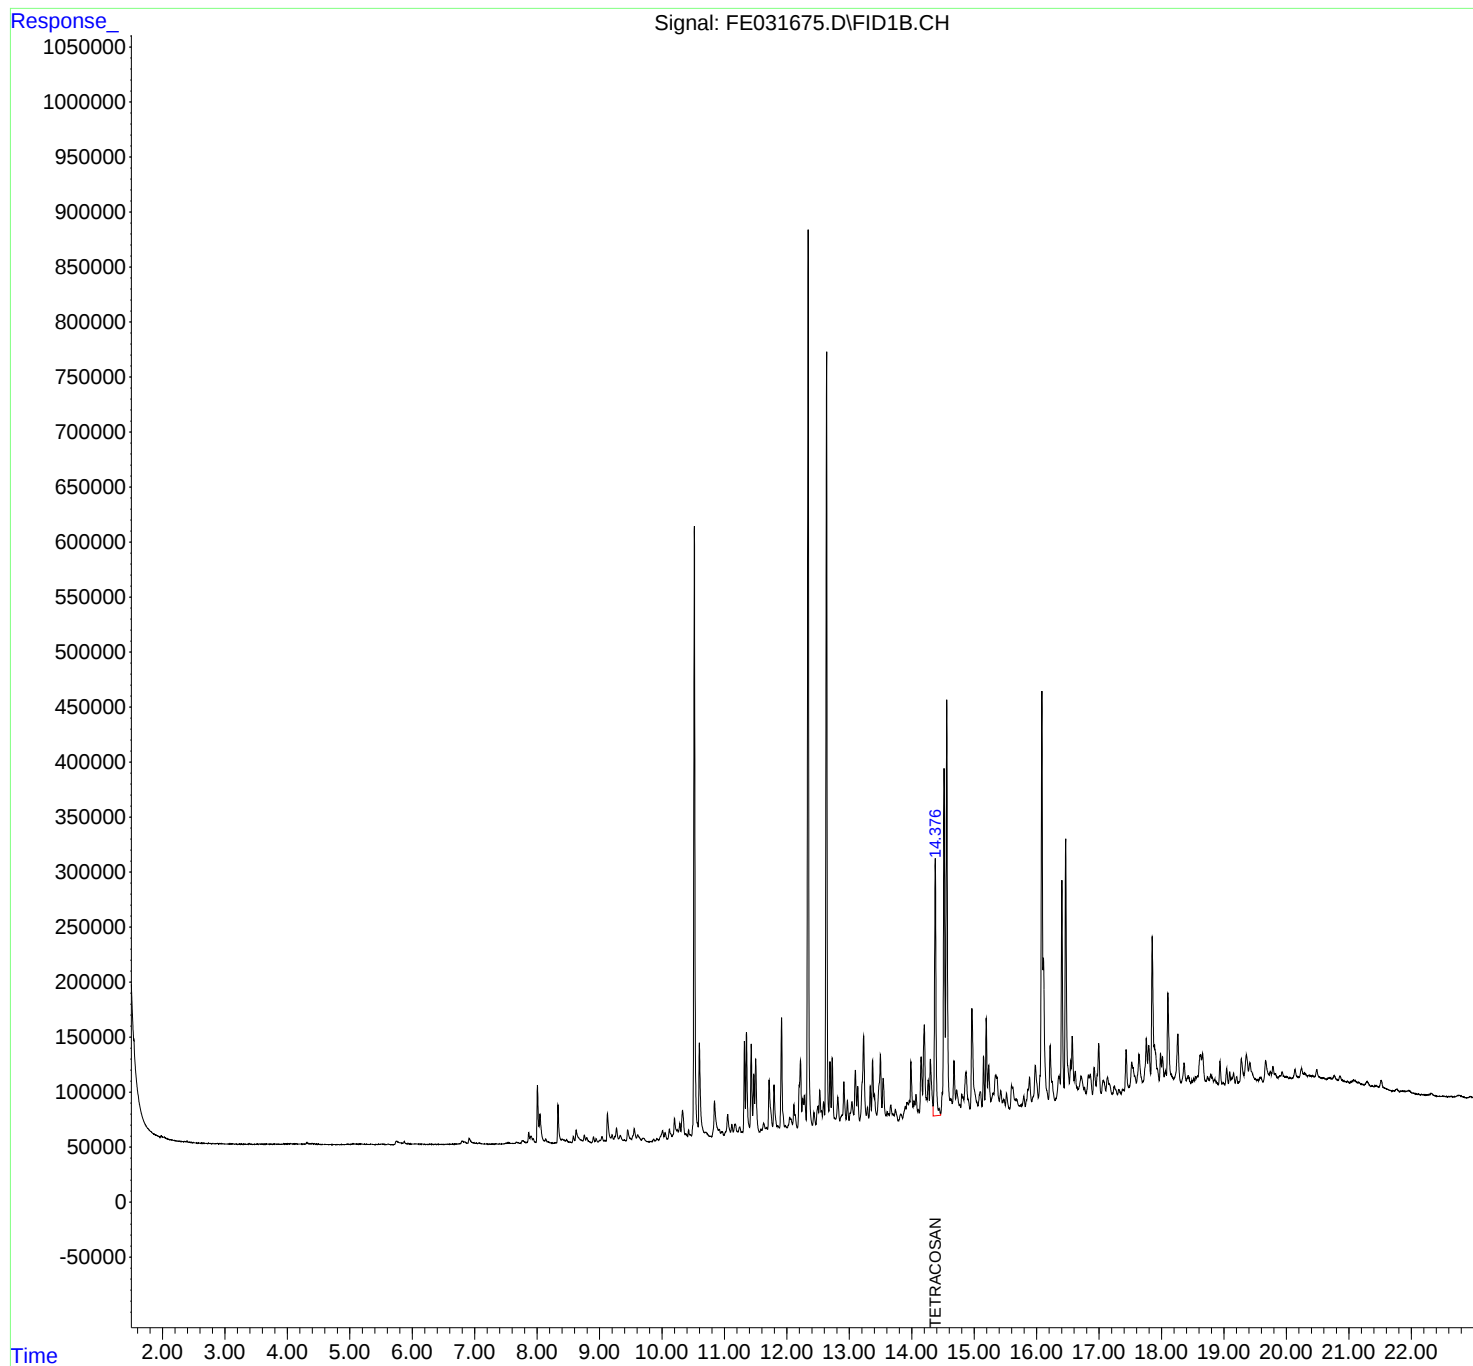

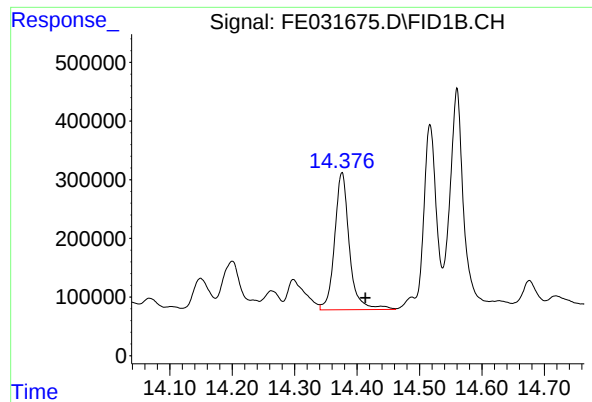

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.376 min
Delta R.T.: -0.038 min
Response: 3833267
Conc: 10.39 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-3-A