

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040423AL\
Data File : FE041155.D
Signal(s) : FID1B.ch
Acq On : 04 Apr 2023 13:51
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 04 23:52:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.846	21657	0.139 ug/ml
19) T	n-Tetratriacontane (C34)	19.631	18478	0.119 ug/ml
20) T	n-Hexatriacontane (C36)	20.411	201742	1.328 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040423AL\
Data File : FE041155.D
Signal(s) : FID1B.ch
Acq On : 04 Apr 2023 13:51
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 04 23:52:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

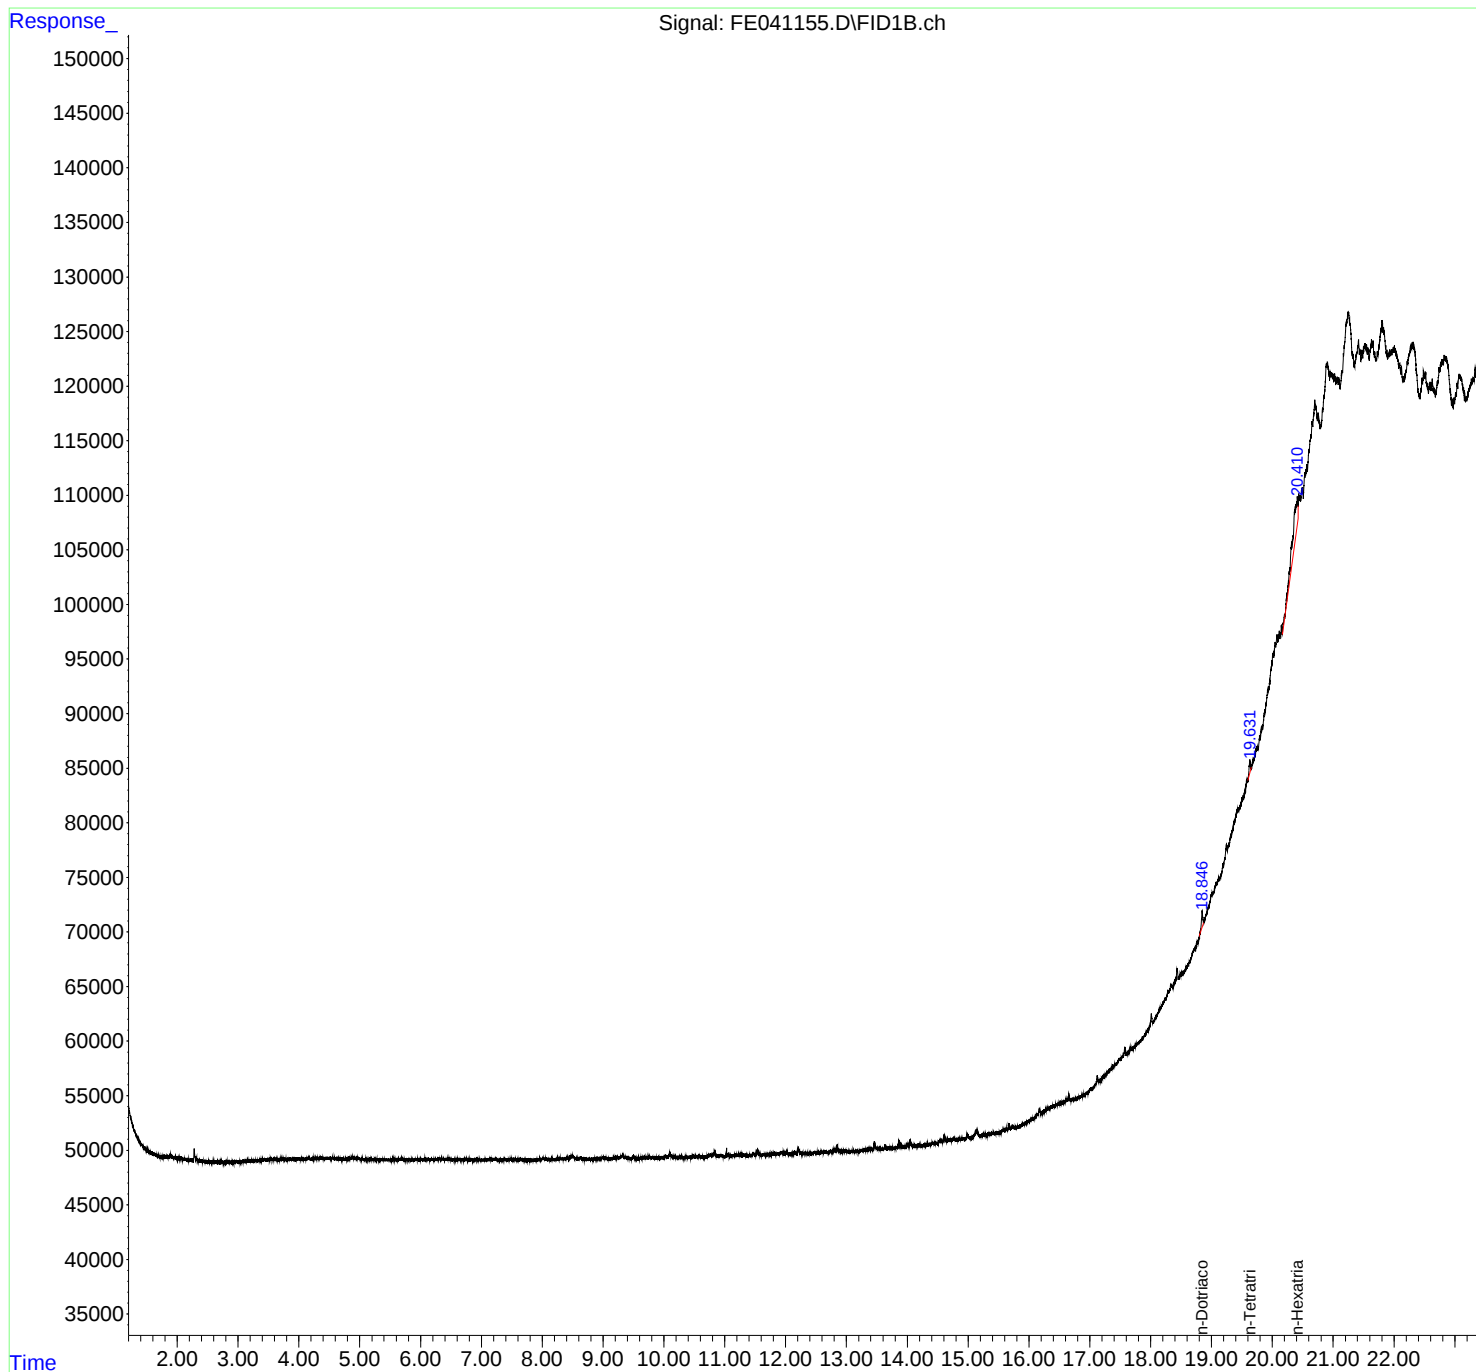


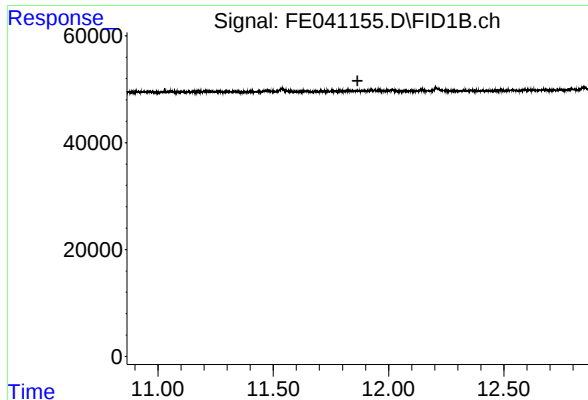

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

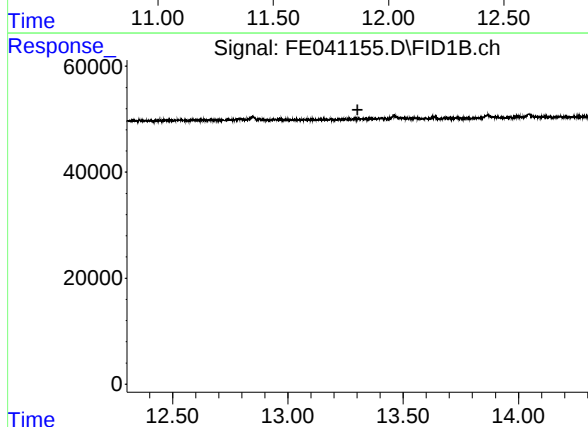


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

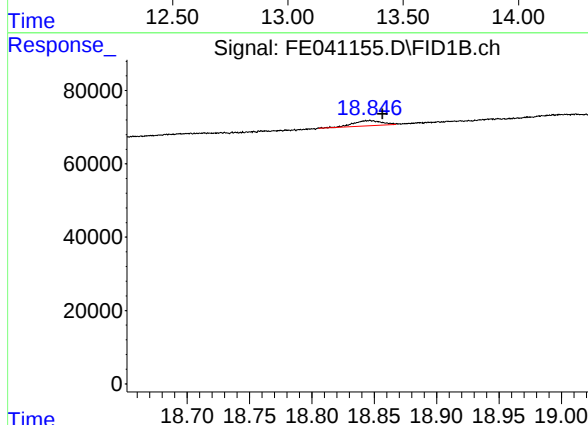


#18 n-Dotriacontane (C32)

R.T.: 18.846 min
Delta R.T.: -0.010 min
Response: 21657
Conc: 0.14 ug/ml

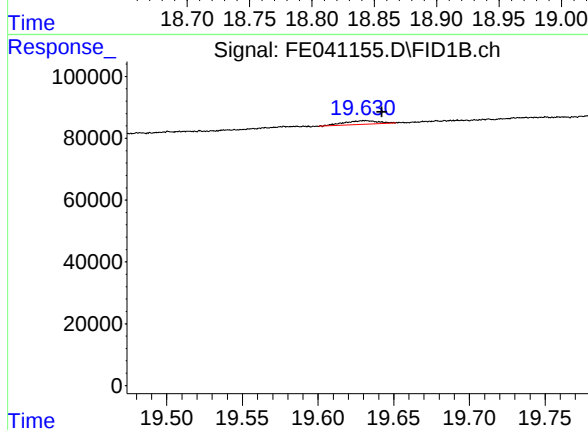

#19 n-Tetratriacontane (C34)

R.T.: 19.631 min
Delta R.T.: -0.011 min
Response: 18478
Conc: 0.12 ug/ml

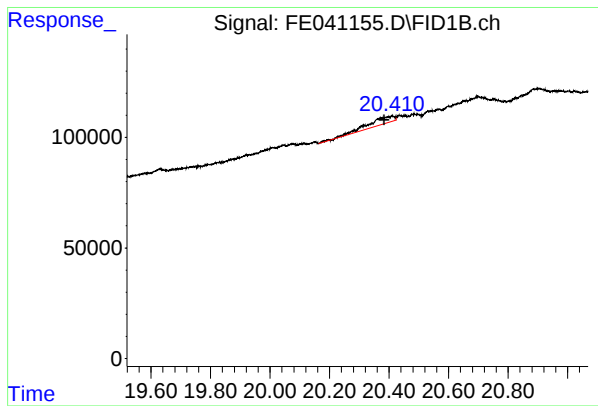

#20 n-Hexatriacontane (C36)

R.T.: 20.411 min
Delta R.T.: 0.027 min
Response: 201742
Conc: 1.33 ug/ml

Instrument :

FID_E

ClientSampleId :