

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040523AL\
Data File : FE041176.D
Signal(s) : FID1B.ch
Acq On : 05 Apr 2023 12:01
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 15:18:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.006	24623	0.161 ug/ml
18) T	n-Dotriacontane (C32)	18.840	37663	0.241 ug/ml
19) T	n-Tetratriacontane (C34)	19.625	25452	0.164 ug/ml
20) T	n-Hexatriacontane (C36)	20.375	6442	0.042 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040523AL\
Data File : FE041176.D
Signal(s) : FID1B.ch
Acq On : 05 Apr 2023 12:01
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 15:18:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

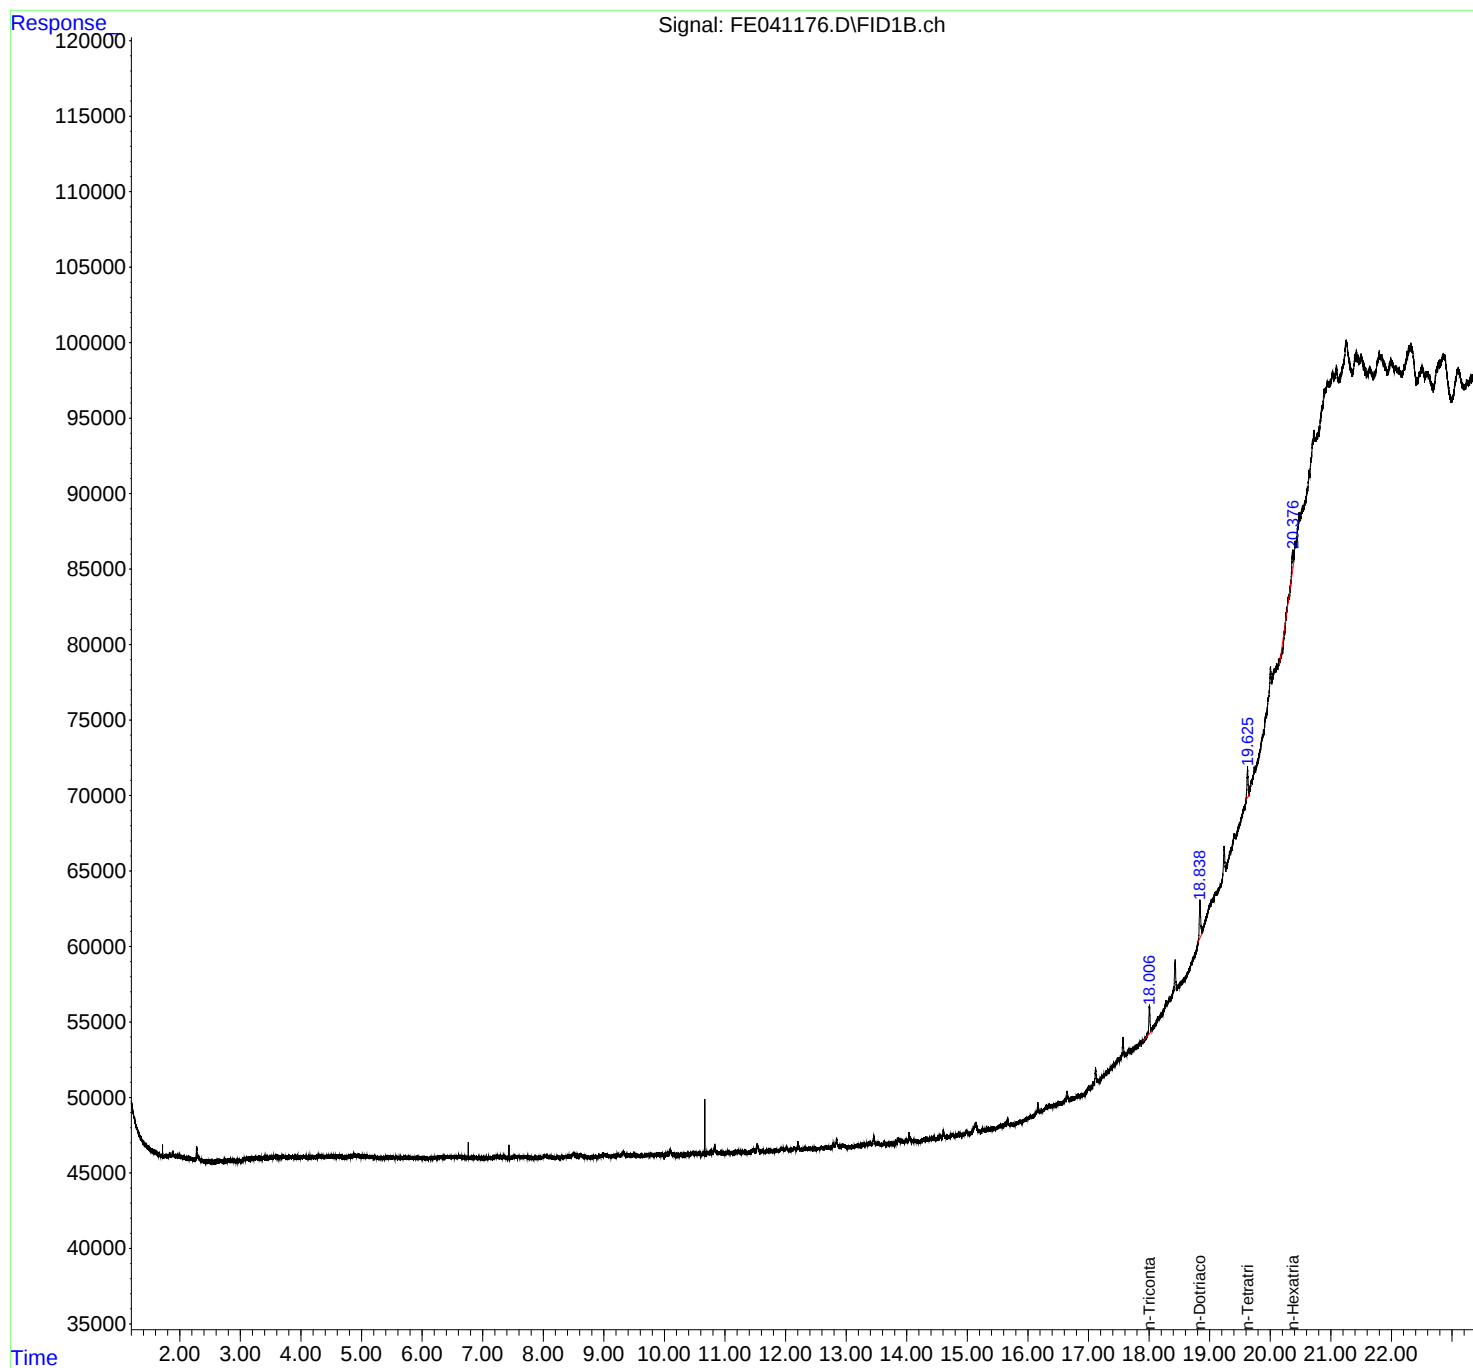


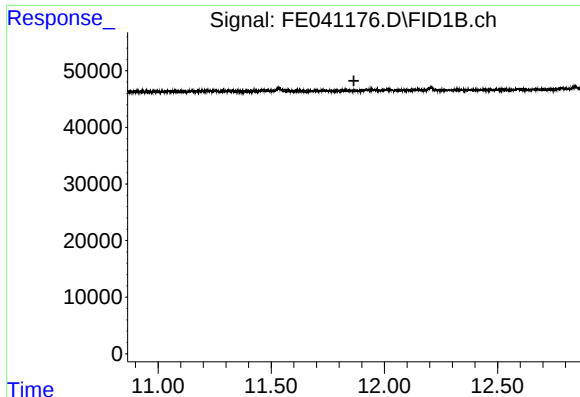

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

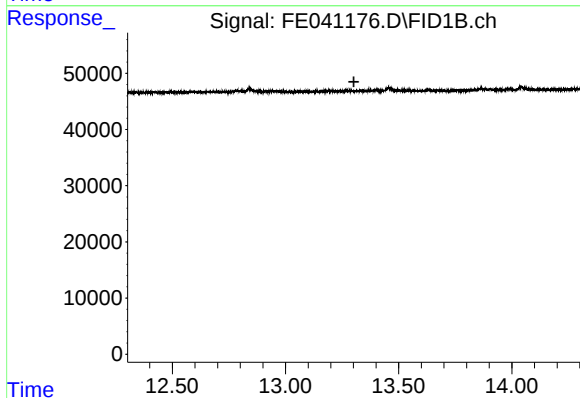


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

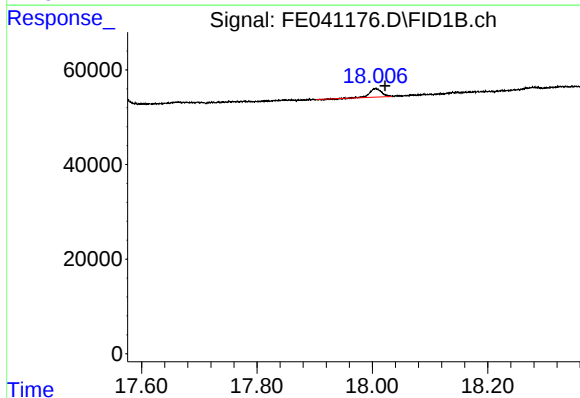


#17 n-Tricontane (C30)

R.T.: 18.006 min
Delta R.T.: -0.017 min
Response: 24623
Conc: 0.16 ug/ml

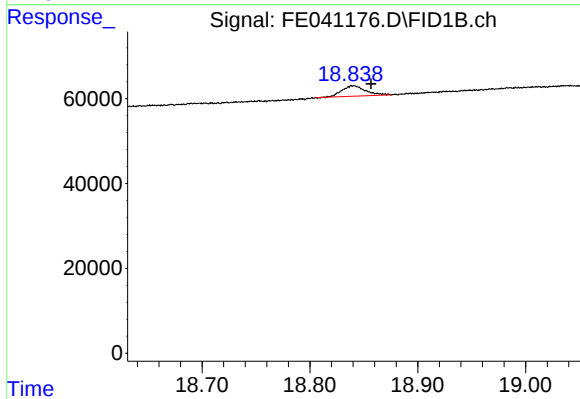

#18 n-Dotriacontane (C32)


R.T.: 18.840 min
Delta R.T.: -0.016 min
Response: 37663
Conc: 0.24 ug/ml

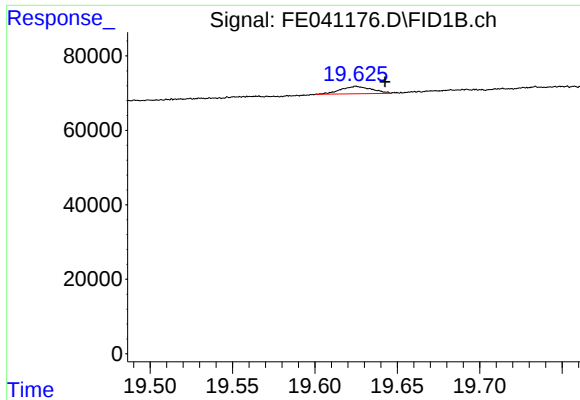

#19 n-Tetratriacontane (C34)

R.T.: 19.625 min
Delta R.T.: -0.017 min
Response: 25452
Conc: 0.16 ug/ml

Instrument :
FID_E
ClientSampleId :

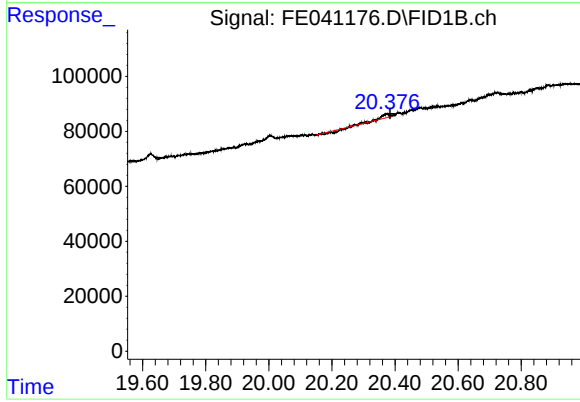

#20 n-Hexatriacontane (C36)

R.T.: 20.375 min
Delta R.T.: -0.009 min
Response: 6442
Conc: 0.04 ug/ml