

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040623\  
Data File : FE041187.D  
Signal(s) : FID1B.ch  
Acq On : 06 Apr 2023 08:08  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/07/2023  
Supervised By :Ankita Jodhani 04/07/2023

Integration File: autoint1.e  
Quant Time: Apr 07 03:14:18 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE040523.M  
Quant Title :  
QLast Update : Thu Apr 06 02:04:41 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.939 | 2424529  | 19.049 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE040623\  
Data File : FE041187.D  
Signal(s) : FID1B.ch  
Acq On : 06 Apr 2023 08:08  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
I.BLK


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/07/2023  
Supervised By :Ankita Jodhani 04/07/2023

Integration File: autoint1.e  
Quant Time: Apr 07 03:14:18 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE040523.M  
Quant Title :  
QLast Update : Thu Apr 06 02:04:41 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

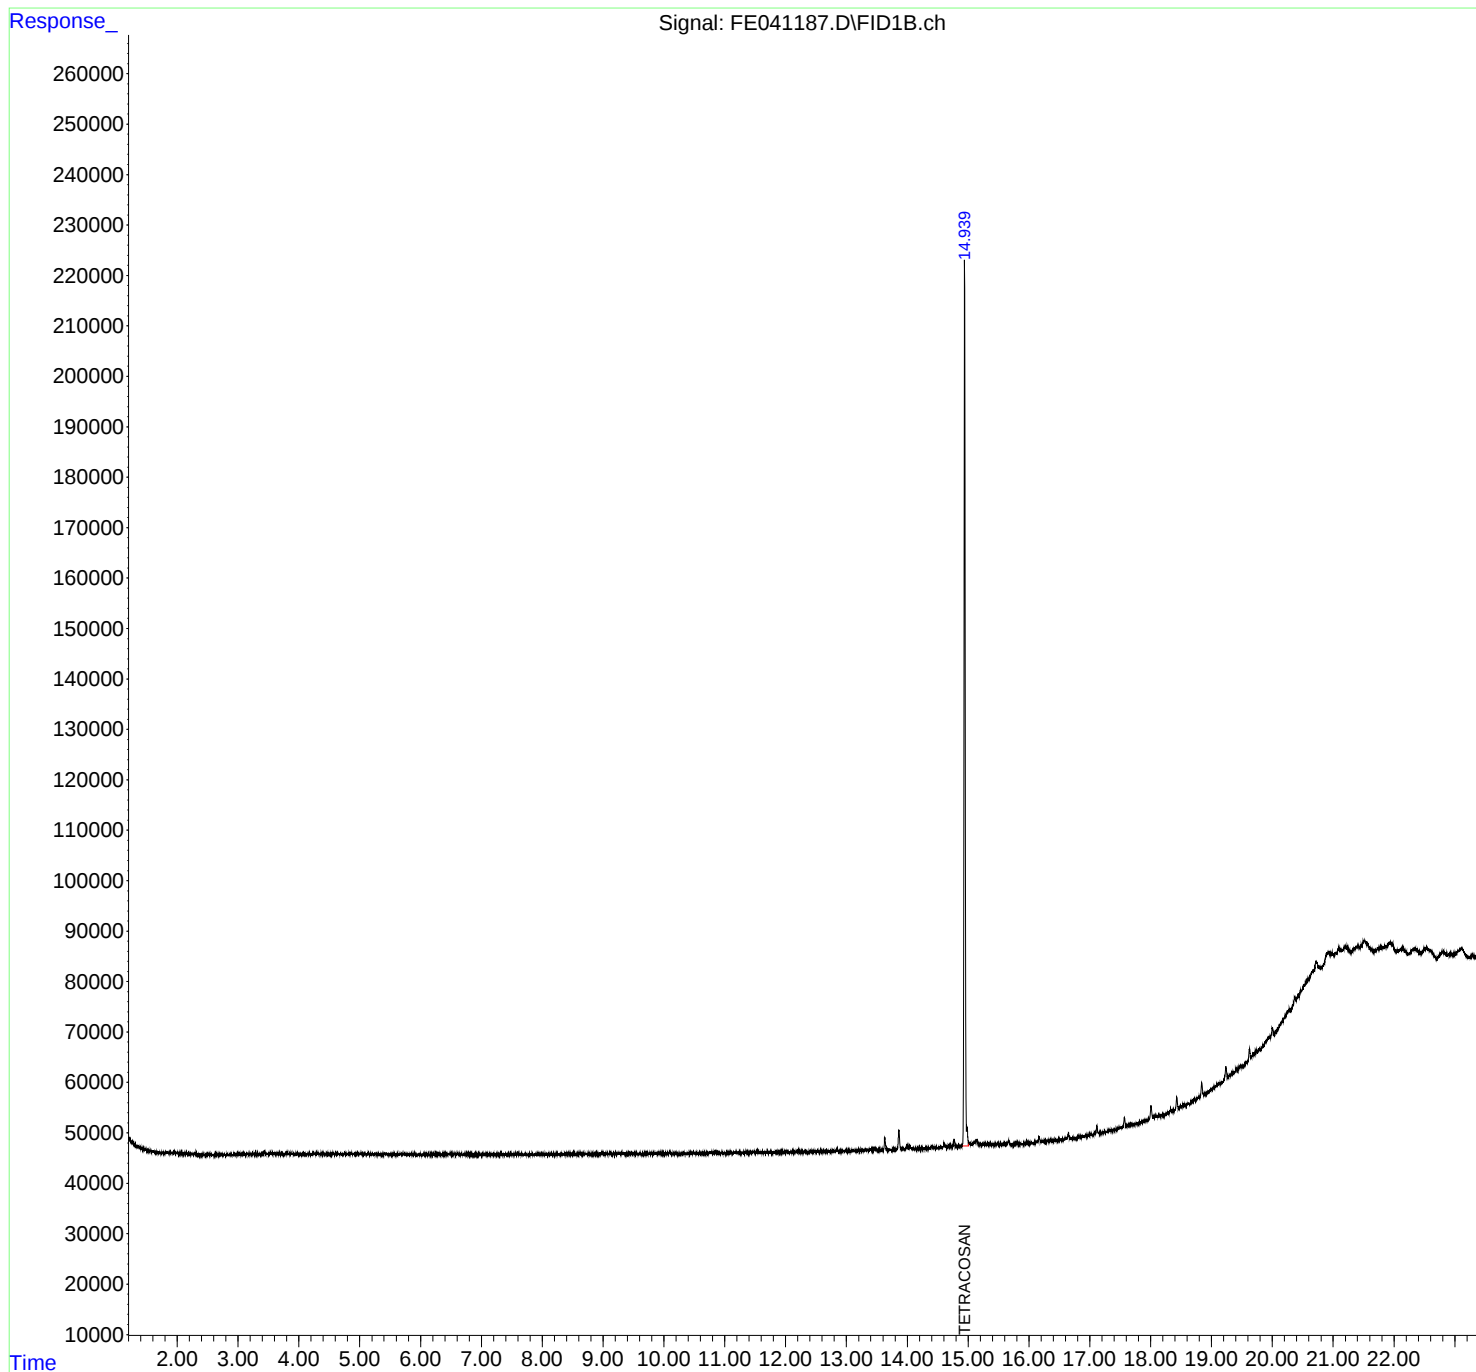

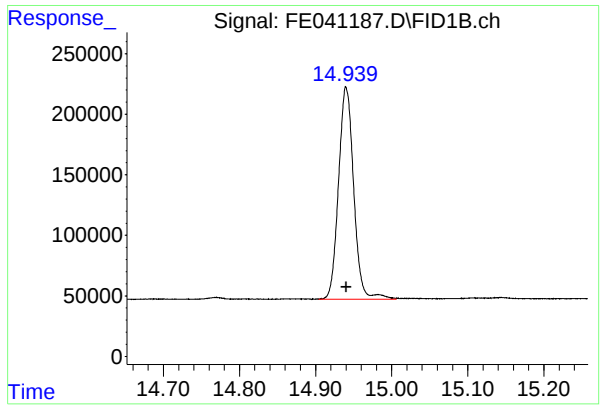

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.939 min  
Delta R.T.: -0.001 min  
Response: 2424529  
Conc: 19.05 ug/ml

Instrument :

FID\_E

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/07/2023

Supervised By :Ankita Jodhani 04/07/2023