

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040623\
Data File : FE041194.D
Signal(s) : FID1B.ch
Acq On : 06 Apr 2023 14:20
Operator : YP\AJ
Sample : PB151919BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB151919BL

Integration File: autoint1.e
Quant Time: Apr 07 03:15:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.940	2302981	18.094 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040623\
Data File : FE041194.D
Signal(s) : FID1B.ch
Acq On : 06 Apr 2023 14:20
Operator : YP\AJ
Sample : PB151919BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB151919BL

Integration File: autoint1.e
Quant Time: Apr 07 03:15:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

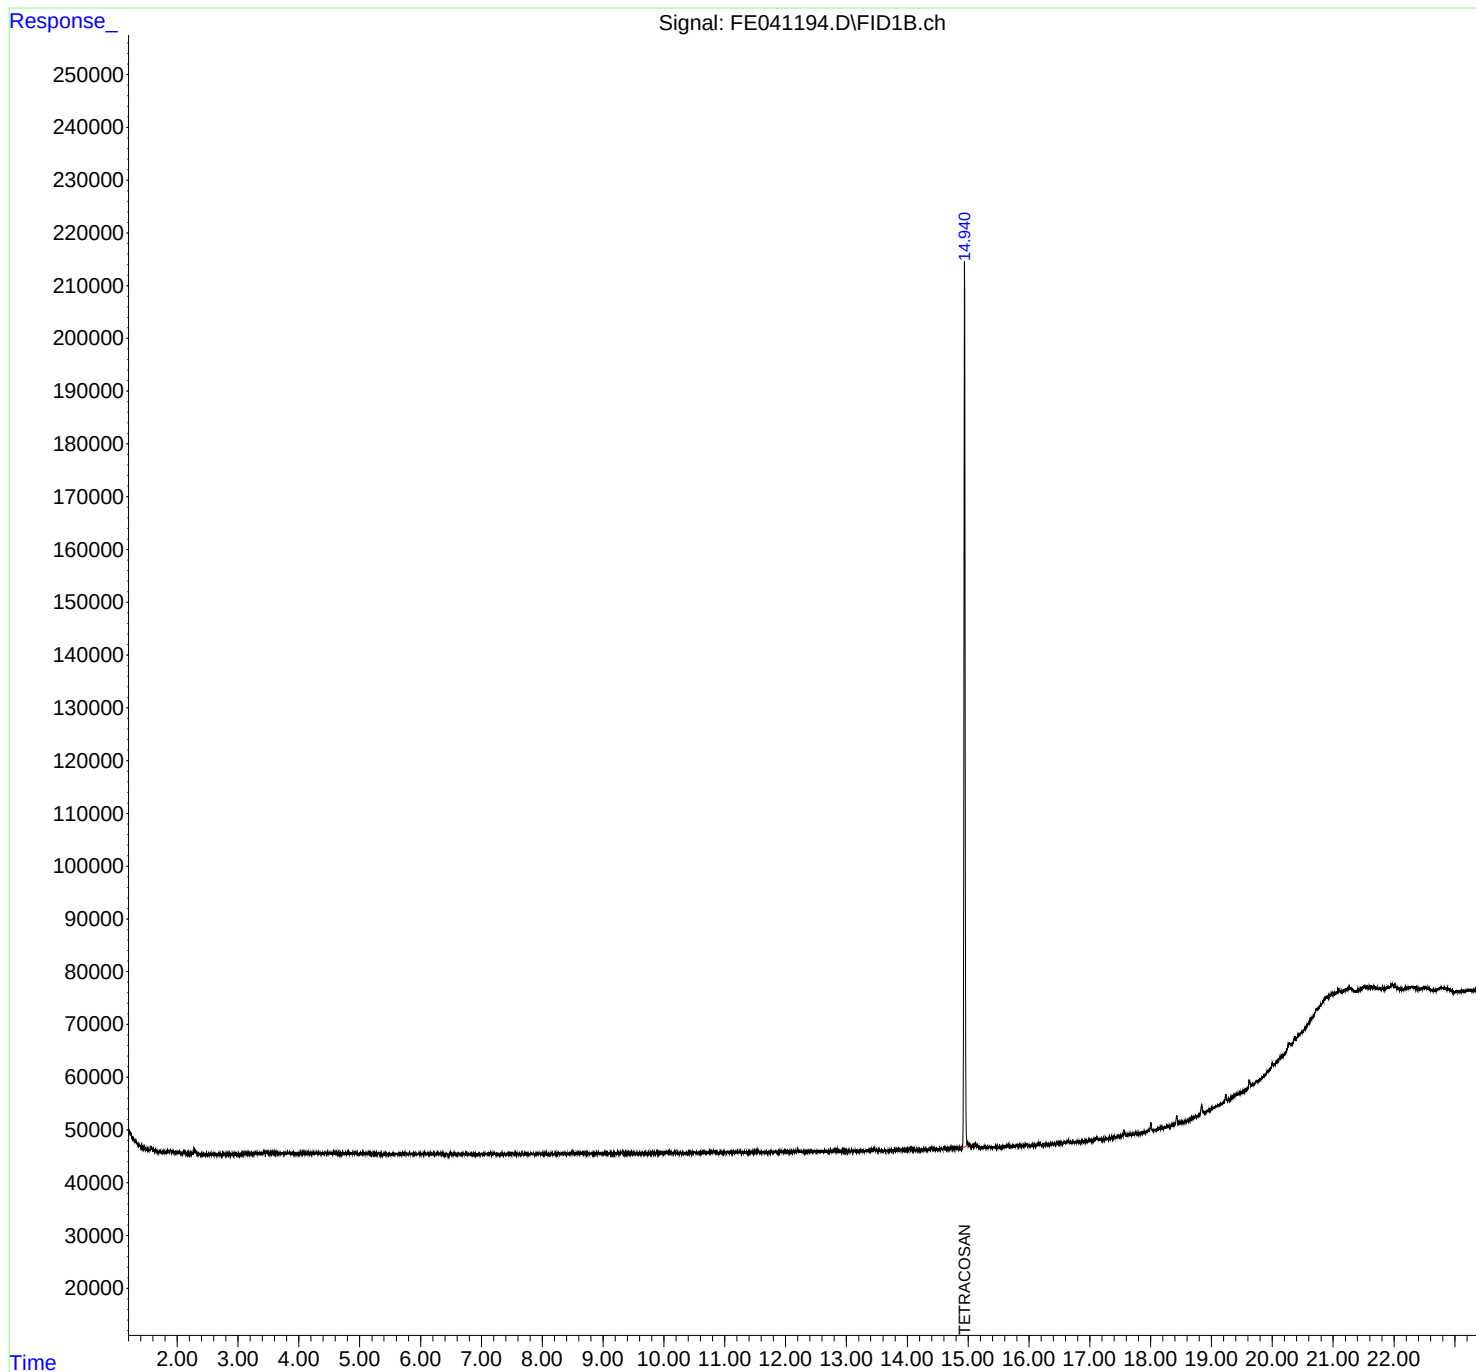

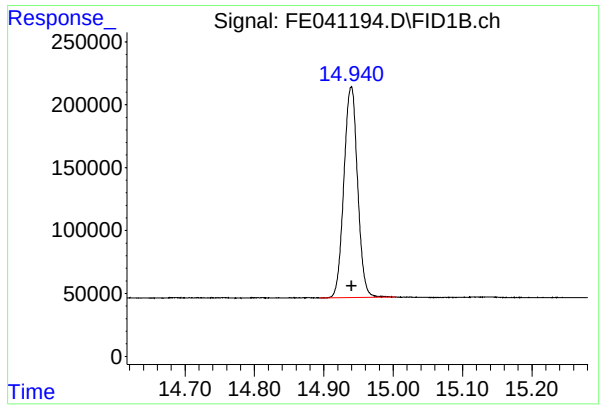

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.940 min
Delta R.T.: 0.000 min
Response: 2302981
Conc: 18.09 ug/ml

Instrument :

FID_E

ClientSampleId :

PB151919BL