

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040623\
 Data File : FE041198.D
 Signal(s) : FID1B.ch
 Acq On : 06 Apr 2023 16:25
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File: autoint1.e
 Quant Time: Apr 07 03:15:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
 Quant Title :
 QLast Update : Thu Apr 06 02:04:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.939	2342205	18.402 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040623\
Data File : FE041198.D
Signal(s) : FID1B.ch
Acq On : 06 Apr 2023 16:25
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

Integration File: autoint1.e
Quant Time: Apr 07 03:15:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

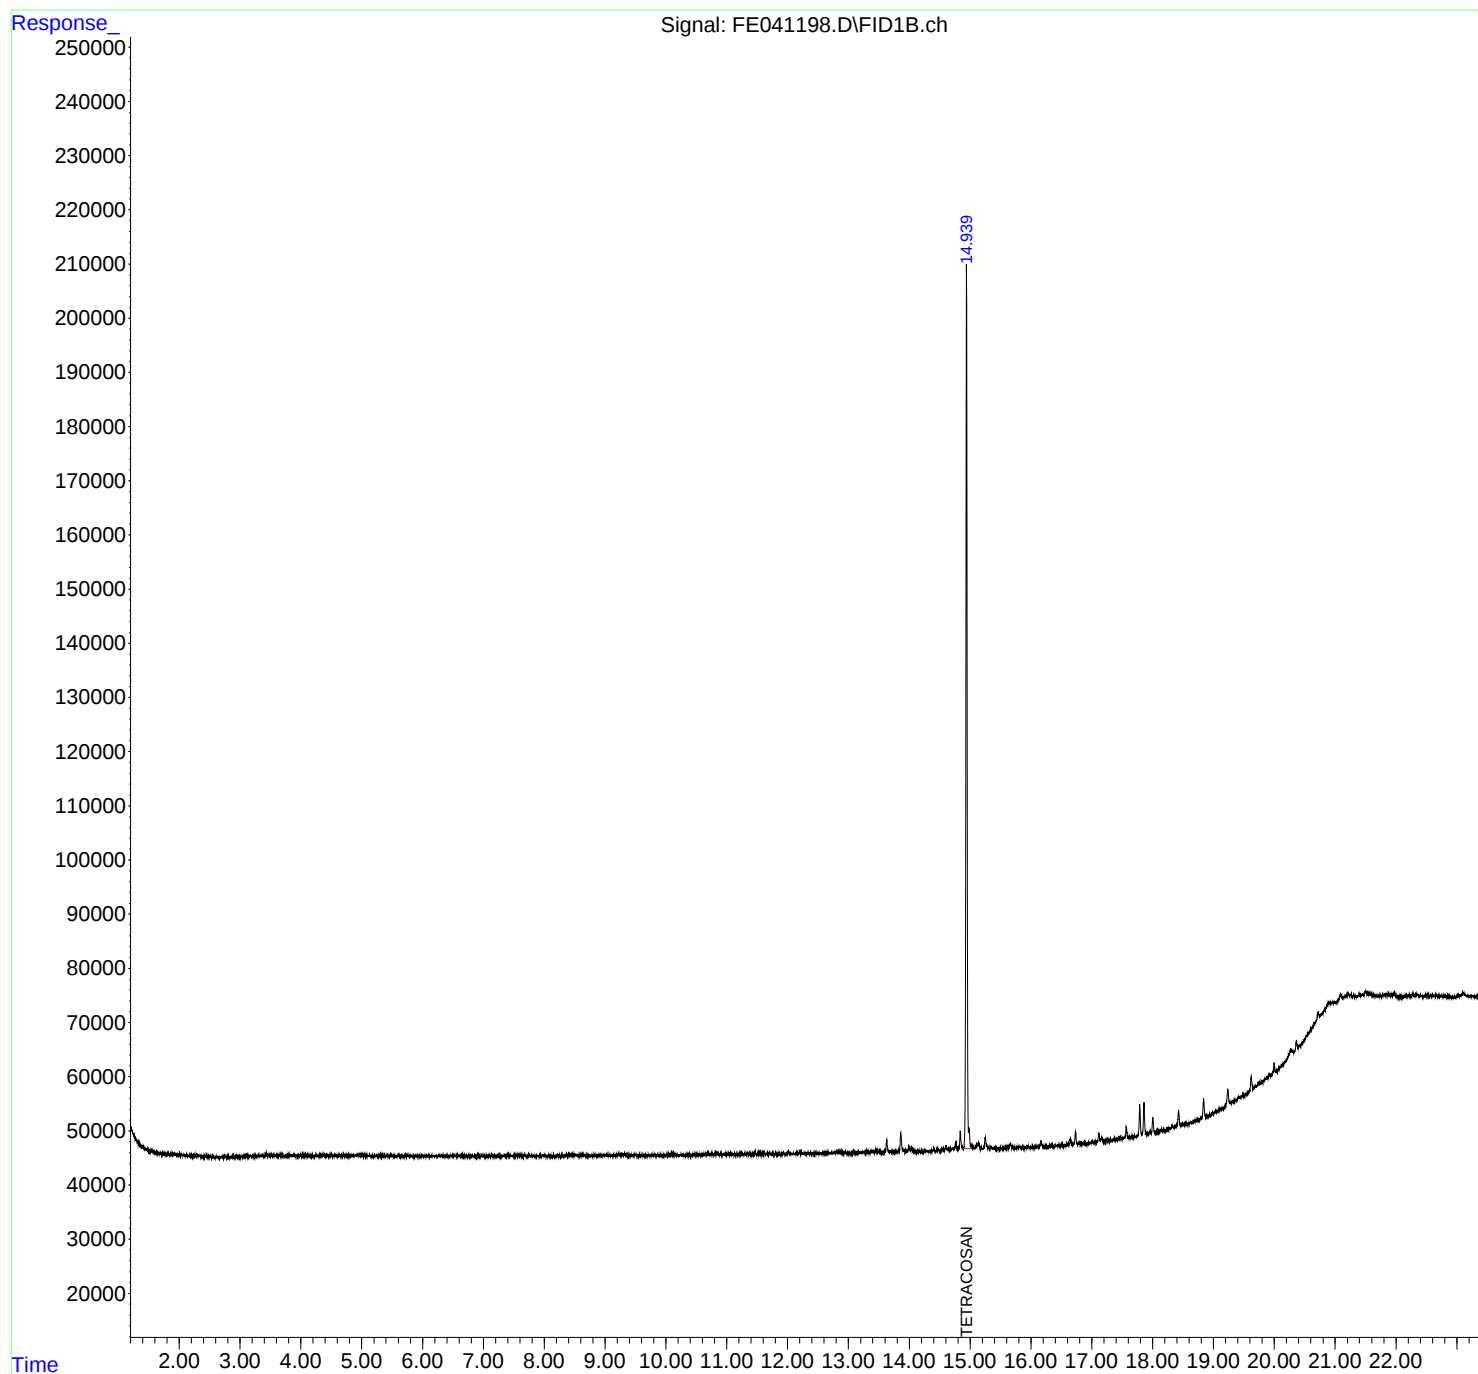

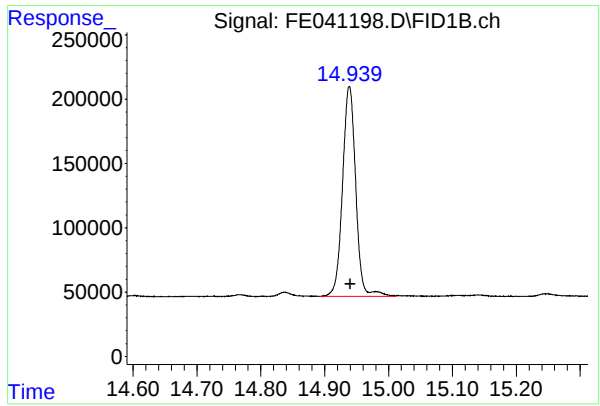

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.939 min
Delta R.T.: -0.002 min
Response: 2342205
Conc: 18.40 ug/ml

Instrument :

FID_E

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/07/2023

Supervised By :Ankita Jodhani 04/07/2023