

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040723\
Data File : FE041236.D
Signal(s) : FID1B.ch
Acq On : 07 Apr 2023 23:09
Operator : YP\AJ
Sample : PB151967BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 02:15:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.932	2367397	18.600 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.828	60119	0.451 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040723\
Data File : FE041236.D
Signal(s) : FID1B.ch
Acq On : 07 Apr 2023 23:09
Operator : YP\AJ
Sample : PB151967BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 02:15:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

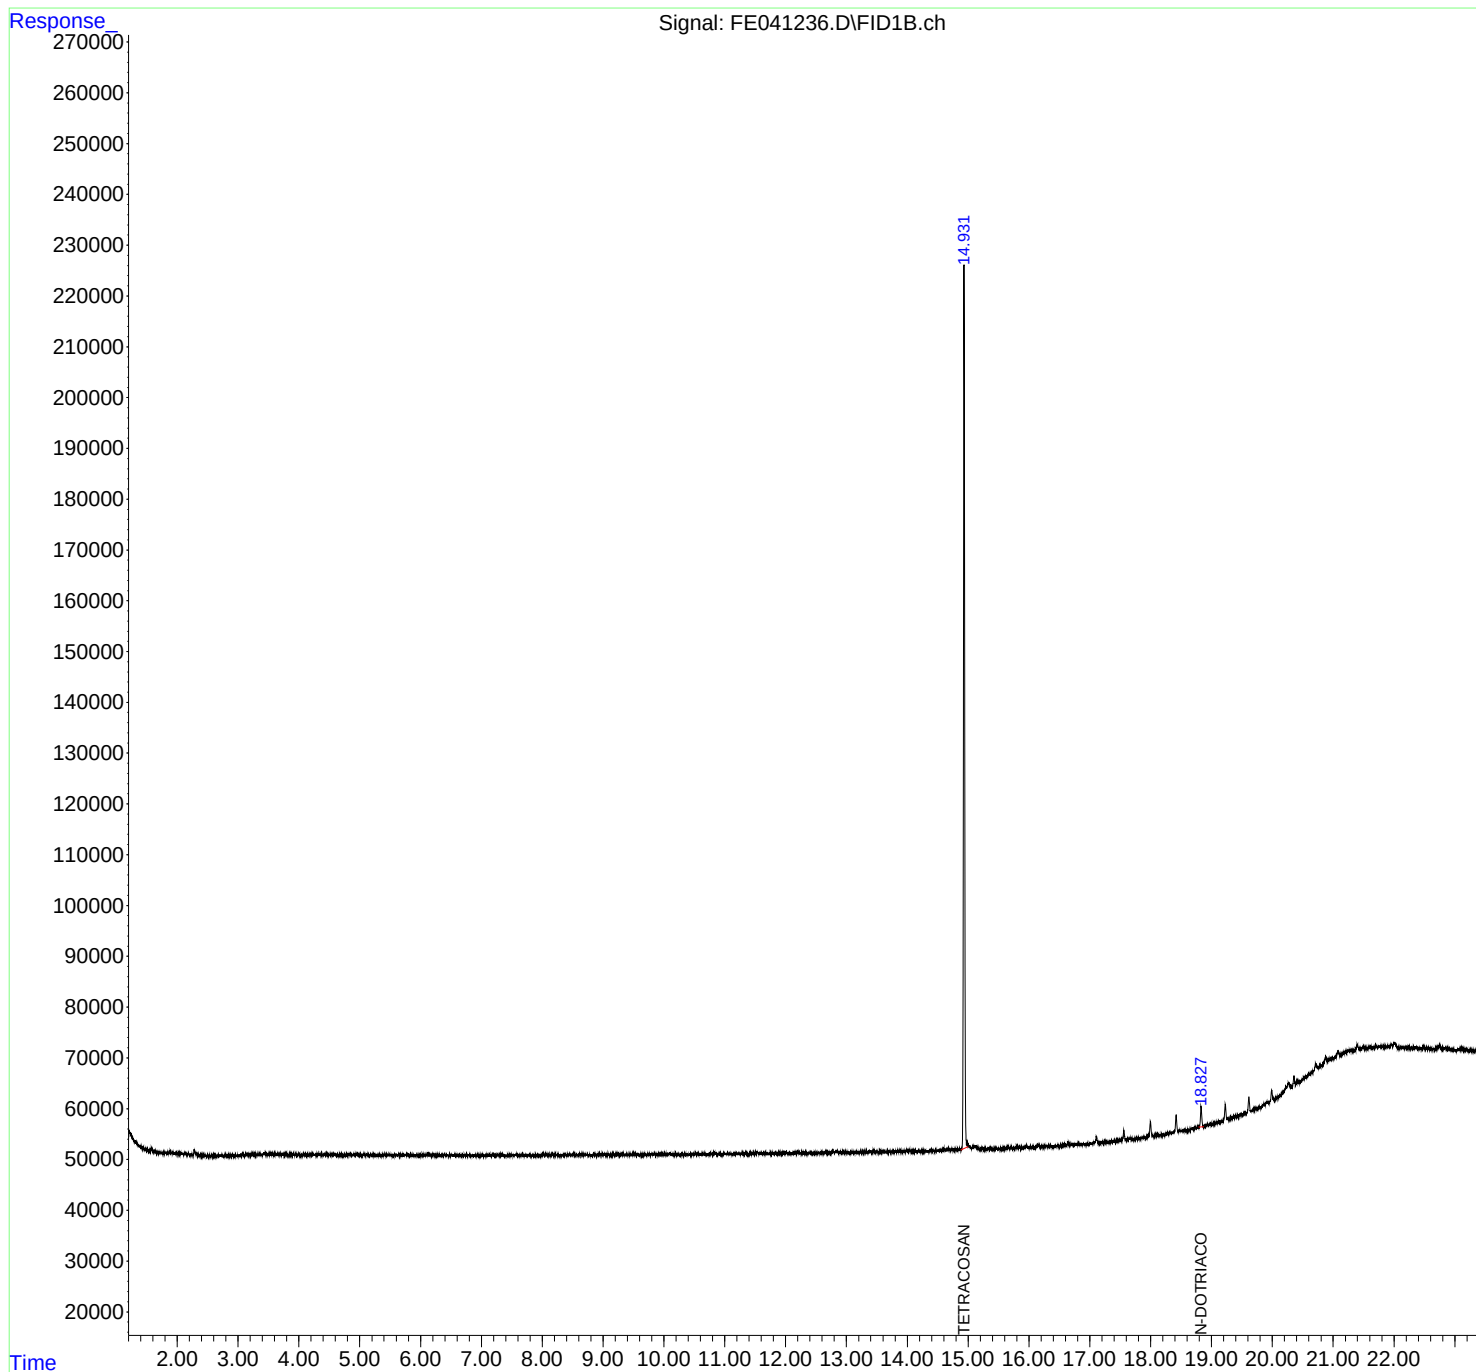

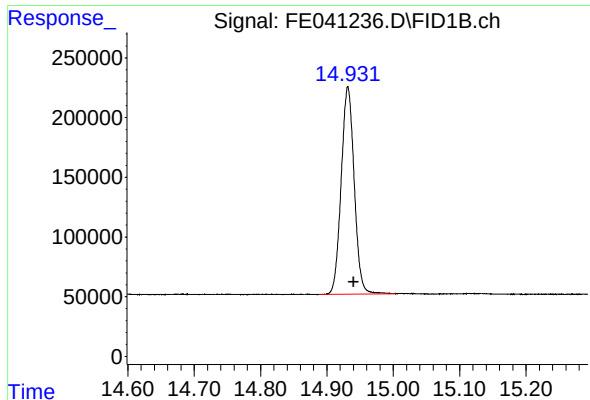


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.932 min
Delta R.T.: -0.009 min
Response: 2367397
Conc: 18.60 ug/ml

Instrument :

FID_E

ClientSampleId :

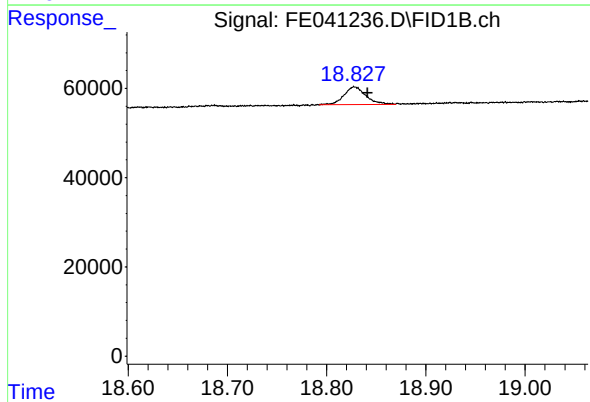

#14 N-DOTRIACONTANE

R.T.: 18.828 min
Delta R.T.: -0.014 min
Response: 60119
Conc: 0.45 ug/ml